

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
 Data File : VW019323.D
 Acq On : 25 Jun 2021 13:00
 Operator : SY/VA
 Sample : M2808-15
 Misc : 5.60G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDW0

Quant Time: Jun 26 00:38:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 26 00:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	543807	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	471208	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	185399	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	163492	22.736	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.960%
7) Chloroethane-d5	2.898	69	144220	23.548	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.200%
11) 1,1-Dichloroethene-d2	4.019	63	244246	17.095	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.400%
21) 2-Butanone-d5	7.086	46	54923	29.158	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.320%
24) Chloroform-d	7.647	84	352209	24.090	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.360%
26) 1,2-Dichloroethane-d4	8.305	65	170397	20.778	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.120%
32) Benzene-d6	8.275	84	693175	25.820	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.280%
36) 1,2-Dichloropropane-d6	9.275	67	206248	25.341	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.360%
41) Toluene-d8	10.323	98	609090	24.704	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.800%
43) trans-1,3-Dichloroprop...	10.579	79	73069	20.729	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.920%
47) 2-Hexanone-d5	10.927	63	44038	31.908	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.820%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	121172	18.048	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	148739	22.985	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5574	0.473	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
Data File : VW019323.D
Acq On : 25 Jun 2021 13:00
Operator : SY/VA
Sample : M2808-15
Misc : 5.60G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDW0

Quant Time: Jun 26 00:38:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 26 00:36:39 2021
Response via : Initial Calibration

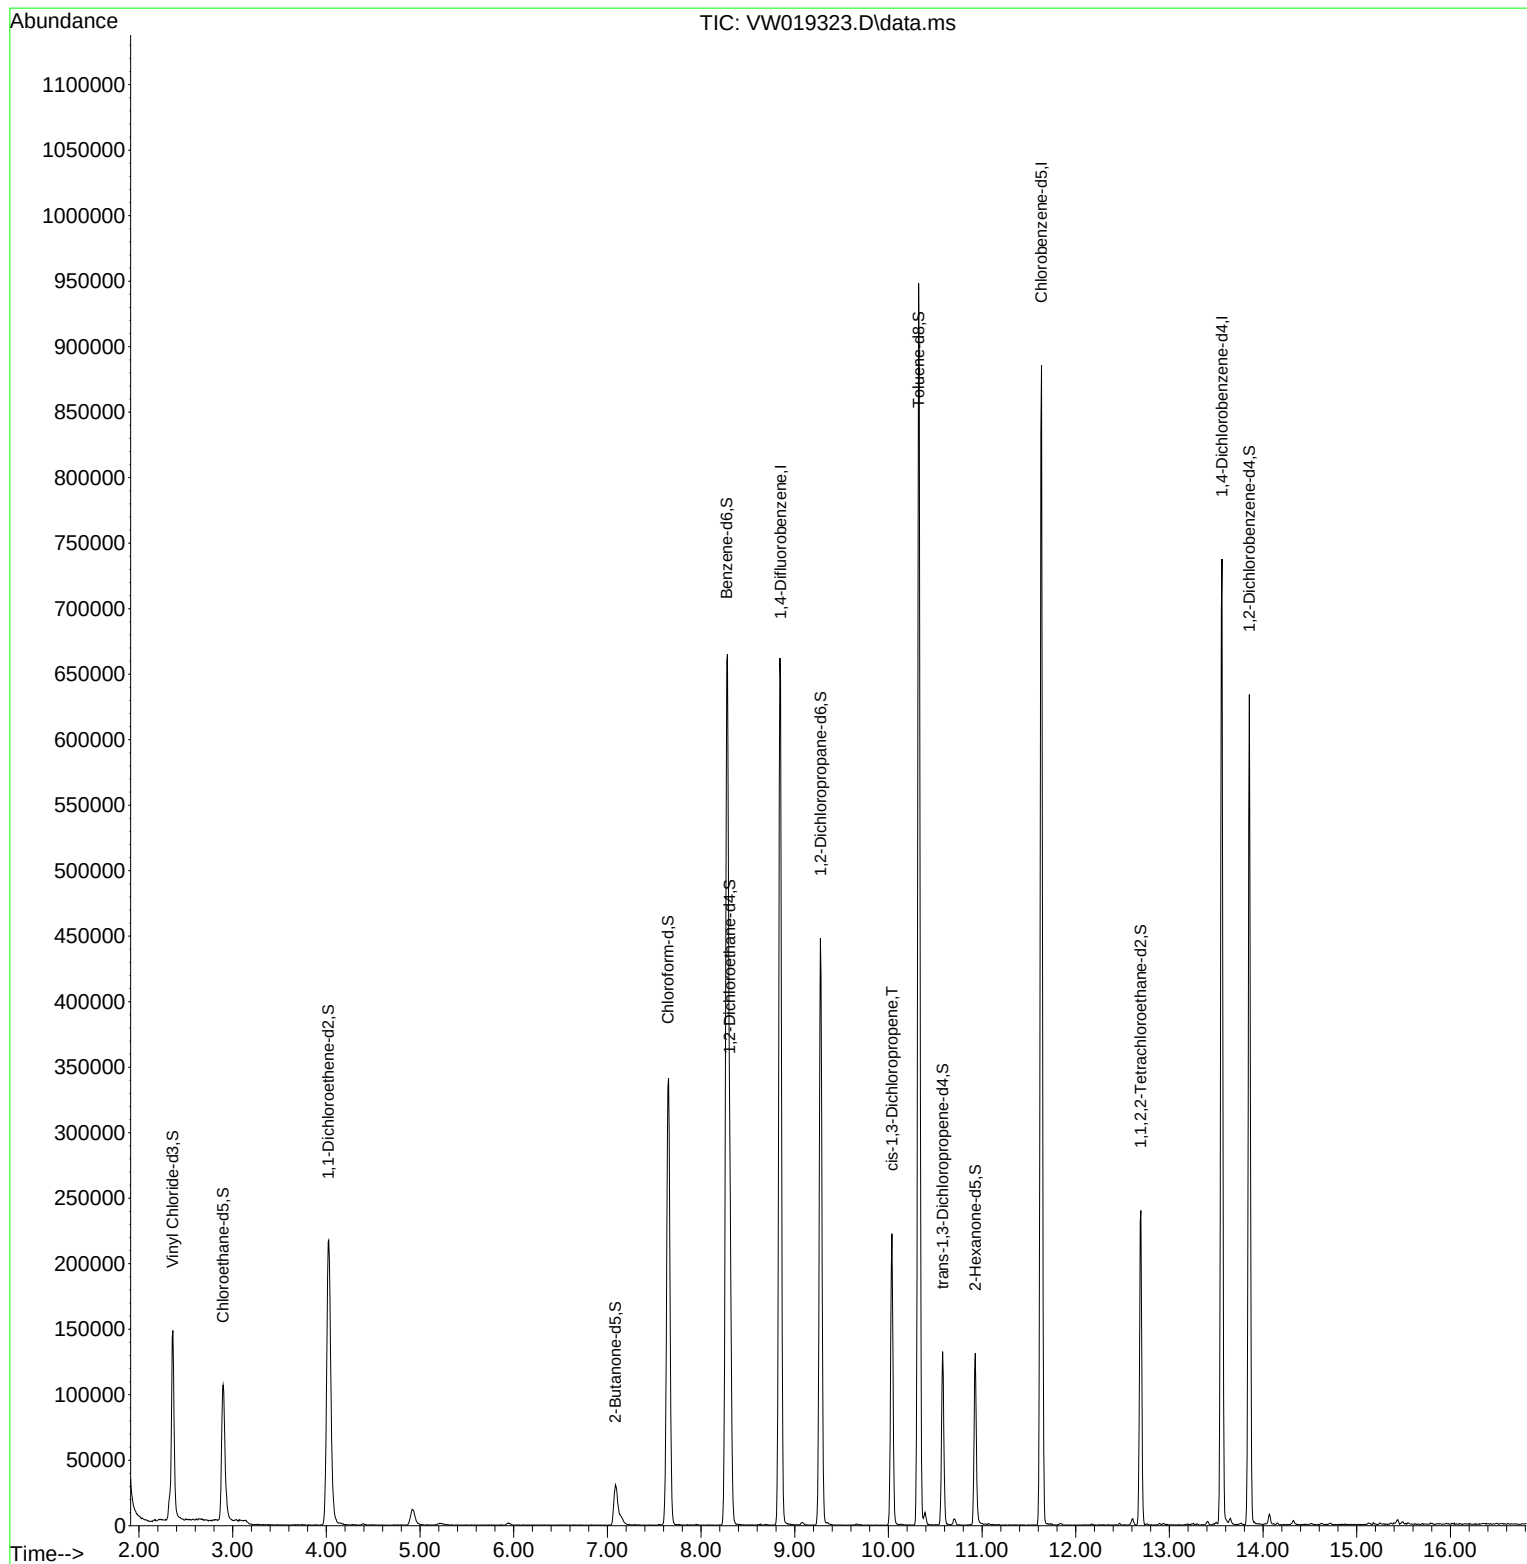

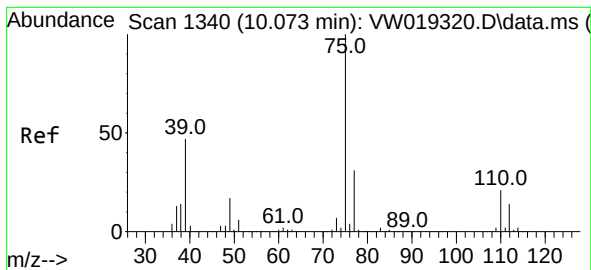

#39
 cis-1,3-Dichloropropene
 Concen: 0.473 ug/L
 RT: 10.037 min Scan# 1334
 Delta R.T. -0.037 min
 Lab File: VW019323.D
 Acq: 25 Jun 2021 13:00

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDW0

Tgt Ion: 75 Resp: 5574
 Ion Ratio Lower Upper
 75 100
 77 53.9 22.6 42.0#

