

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
 Data File : VW019337.D
 Acq On : 25 Jun 2021 18:35
 Operator : SY/VA
 Sample : M2808-18
 Misc : 4.36G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD7

Manual Integrations
 APPROVED

MMDadoda
 6/28/2021 11:58:37 AM

Quant Time: Jun 26 02:10:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 26 00:36:39 2021
 Response via : Initial Calibration

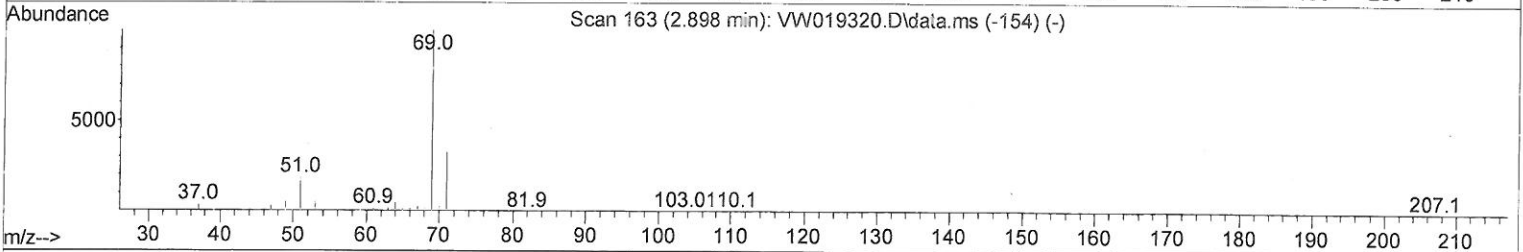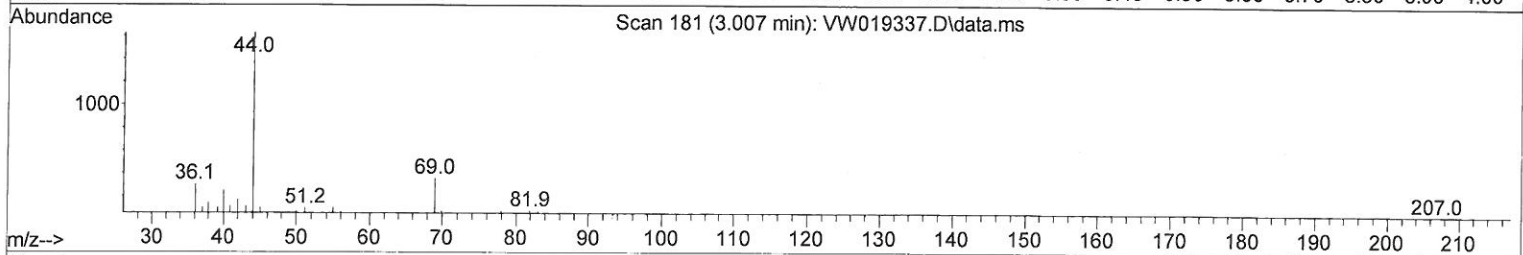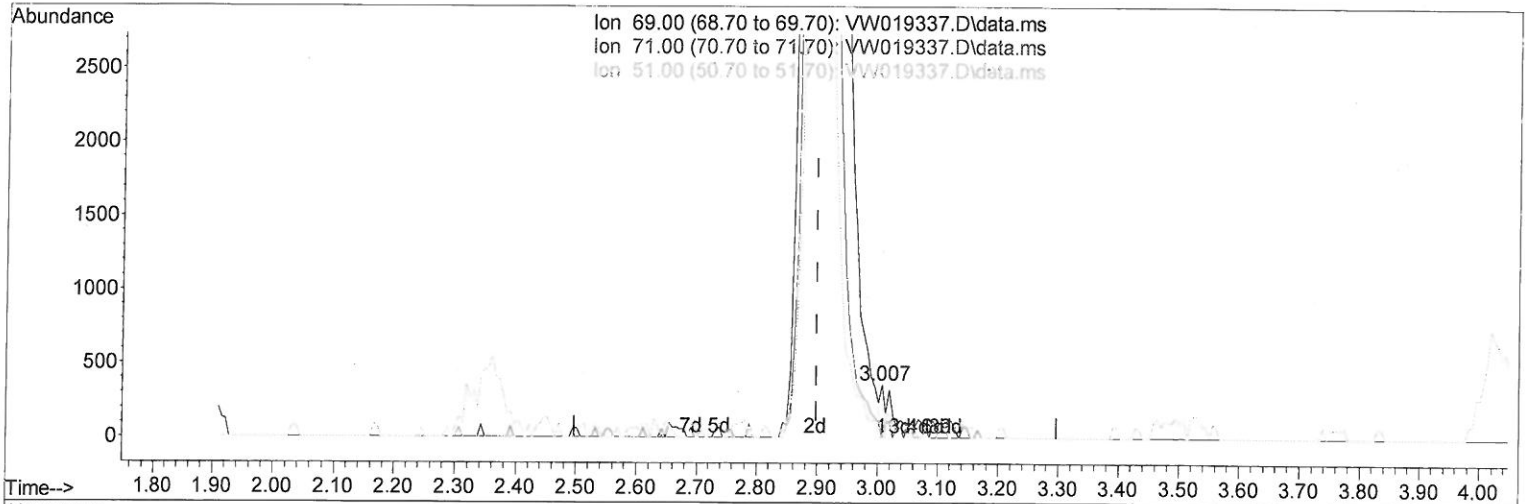

TIC: VW019337.D\data.ms

(7) Chloroethane-d5 (S)

3.007min (+ 0.110) 0.04 ug/L

response 190

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	38.42
51.00	28.40	28.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
 Data File : VW019337.D
 Acq On : 25 Jun 2021 18:35
 Operator : SY/VA
 Sample : M2808-18
 Misc : 4.36G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD7

Manual Integrations
 APPROVED

MMDadoda
 6/28/2021 11:58:37 AM

Quant Time: Jun 26 00:41:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 26 00:36:39 2021
 Response via : Initial Calibration

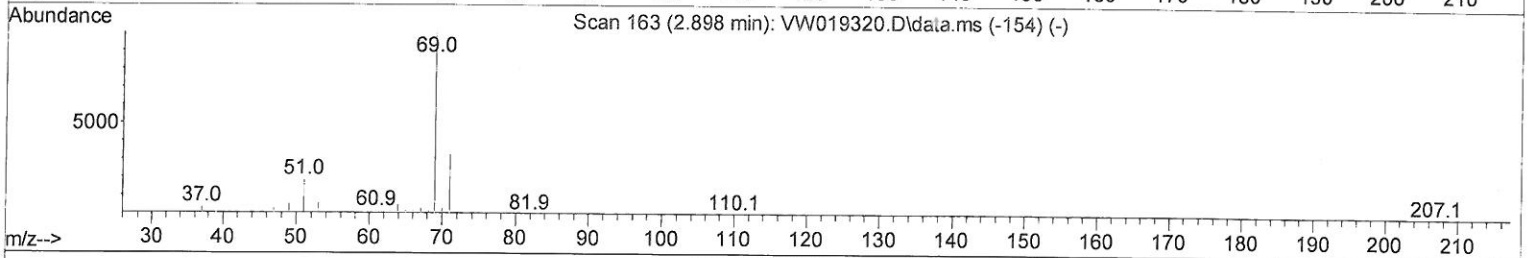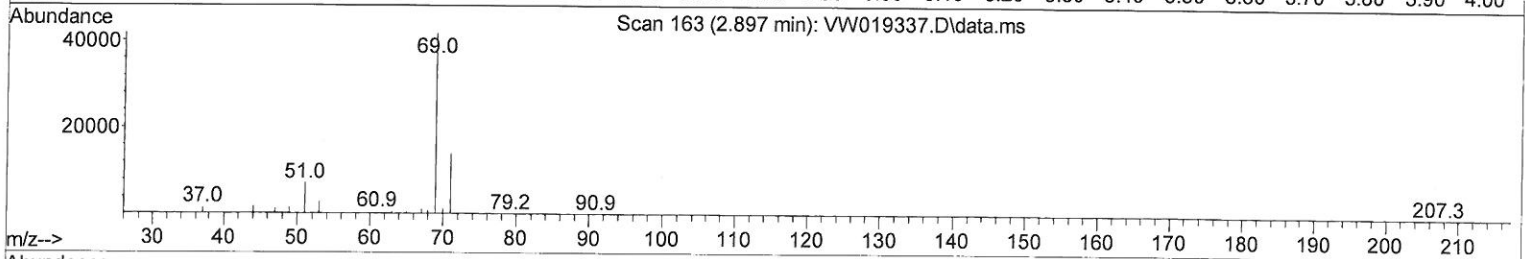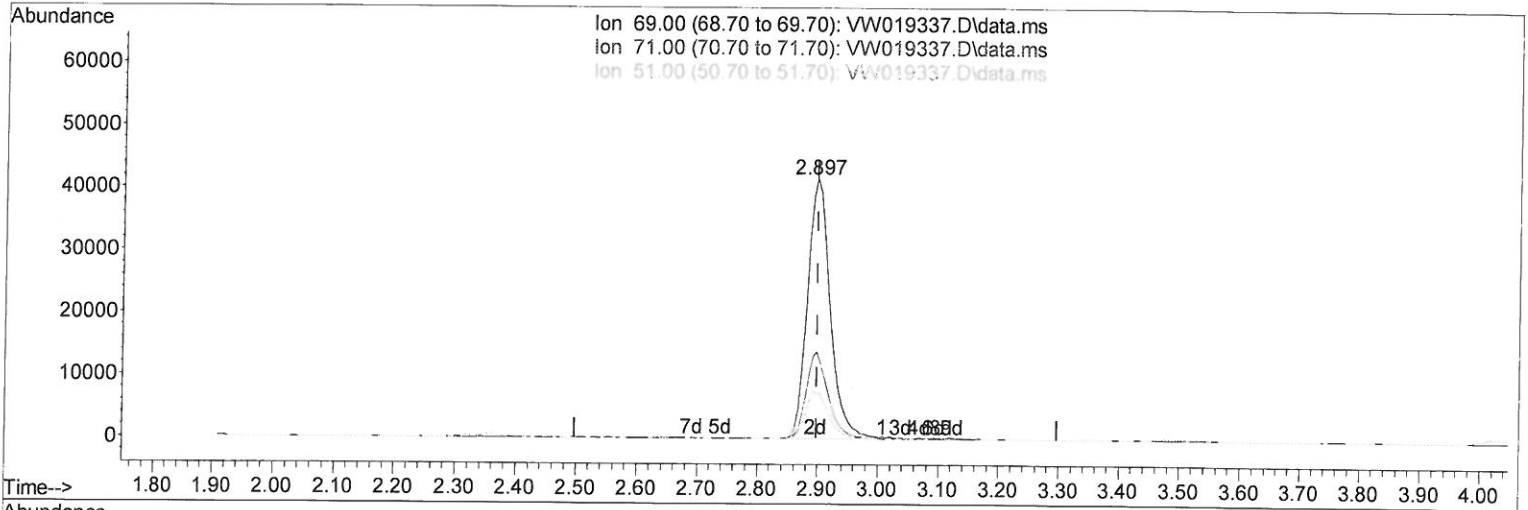

TIC: VW019337.D\data.ms

(7) Chloroethane-d5 (S)

2.897min (-0.000) 21.07 ug/L m

response 110036

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.07#
51.00	28.40	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
 Data File : VW019337.D
 Acq On : 25 Jun 2021 18:35
 Operator : SY/VA
 Sample : M2808-18
 Misc : 4.36G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD7

Manual Integrations
 APPROVED

MMDadoda
 6/28/2021 11:58:37 AM

Quant Time: Jun 26 00:41:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 26 00:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	463651	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	387331	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	128004	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	123544	20.151	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.600%		
7) Chloroethane-d5	2.897	69	110036m	21.072	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.280%		
11) 1,1-Dichloroethene-d2	4.025	63	181445	14.895	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.600%		
21) 2-Butanone-d5	7.080	46	63692	39.659	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.320%		
24) Chloroform-d	7.653	84	286344	22.971	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.880%		
26) 1,2-Dichloroethane-d4	8.311	65	151361	21.647	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.600%		
32) Benzene-d6	8.281	84	552963	25.057	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.240%		
36) 1,2-Dichloropropane-d6	9.274	67	170476	25.482	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.920%		
41) Toluene-d8	10.323	98	460102	22.702	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.800%		
43) trans-1,3-Dichloroprop...	10.579	79	60754	20.968	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.880%		
47) 2-Hexanone-d5	10.927	63	49144	43.319	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.640%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	111046	20.122	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.480%		
66) 1,2-Dichlorobenzene-d4	13.853	152	100344	22.459	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.840%		
Target Compounds						
13) Acetone	4.123	43	39400	27.686	ug/L	89
14) Carbon disulfide	4.397	76	10593	0.510	ug/L	98
16) Methylene chloride	4.922	84	15940	1.853	ug/L	94
22) 2-Butanone	7.171	43	18655	9.804	ug/L	97
42) Toluene	10.390	91	101971	3.720	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062521\
 Data File : VW019337.D
 Acq On : 25 Jun 2021 18:35
 Operator : SY/VA
 Sample : M2808-18
 Misc : 4.36G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD7

Manual Integrations
 APPROVED

MMDadoda
 6/28/2021 11:58:37 AM

Quant Time: Jun 26 00:41:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 26 00:36:39 2021
 Response via : Initial Calibration

