

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072720\
 Data File : VW015963.D
 Acq On : 27 Jul 2020 11:44
 Operator : SY/VA
 Sample : L3458-02
 Misc : 4.32G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAY30

Manual Integrations
 APPROVED

MMDadoda
 7/29/2020 7:52:15 PM

Quant Time: Jul 28 02:07:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 28 01:36:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	293362	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	256156	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	100733	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	86923	21.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.00%
7) Chloroethane-d5	2.89	69	67827	20.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.68%
10) 1,1-Dichloroethene-d2	4.01	63	125989	15.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.20%
20) 2-Butanone-d5	7.09	46	122760	112.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	225.80%#
24) Chloroform-d	7.65	84	162470	19.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.88%
26) 1,2-Dichloroethane-d4	8.31	65	101024	22.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.36%
29) Benzene-d6	8.28	84	329830	21.15	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.60%
33) 1,2-Dichloropropane-d6	9.28	67	102798	21.99	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.96%
37) Toluene-d8	10.33	98	288015	20.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.56%
38) trans-1,3-Dichloropropene-	10.59	79	44420	22.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.20%
39) 2-Hexanone-d5	10.93	63	87615	112.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	225.14%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	119179	33.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	132.68%#
61) 1,2-Dichlorobenzene-d4	13.86	152	84845	21.60	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	10138	11.102	ug/L	75
15) Methyl Acetate	4.68	43	10444	6.066	ug/L	96
16) Methylene chloride	4.92	84	7610m	1.583	ug/L	
21) 2-Butanone	7.19	43	3034m	2.687	ug/L	
34) Benzene	8.33	78	13233	0.851	ug/L	100
36) Methylcyclohexane	9.34	83	11186	1.584	ug/L	91
44) Toluene	10.39	91	33761	2.069	ug/L	98
53) Ethylbenzene	11.74	91	21930	1.195	ug/L	98
54) m,p-Xylene	11.84	106	5971	0.870	ug/L	93
55) o-xylene	12.17	106	2268	0.351	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072720\
Data File : VW015963.D
Acq On : 27 Jul 2020 11:44
Operator : SY/VA
Sample : L3458-02
Misc : 4.32G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GAY30

Manual Integrations
APPROVED

MMDadoda
7/29/2020 7:52:15 PM

Quant Time: Jul 28 02:07:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 28 01:36:11 2020
Response via : Initial Calibration

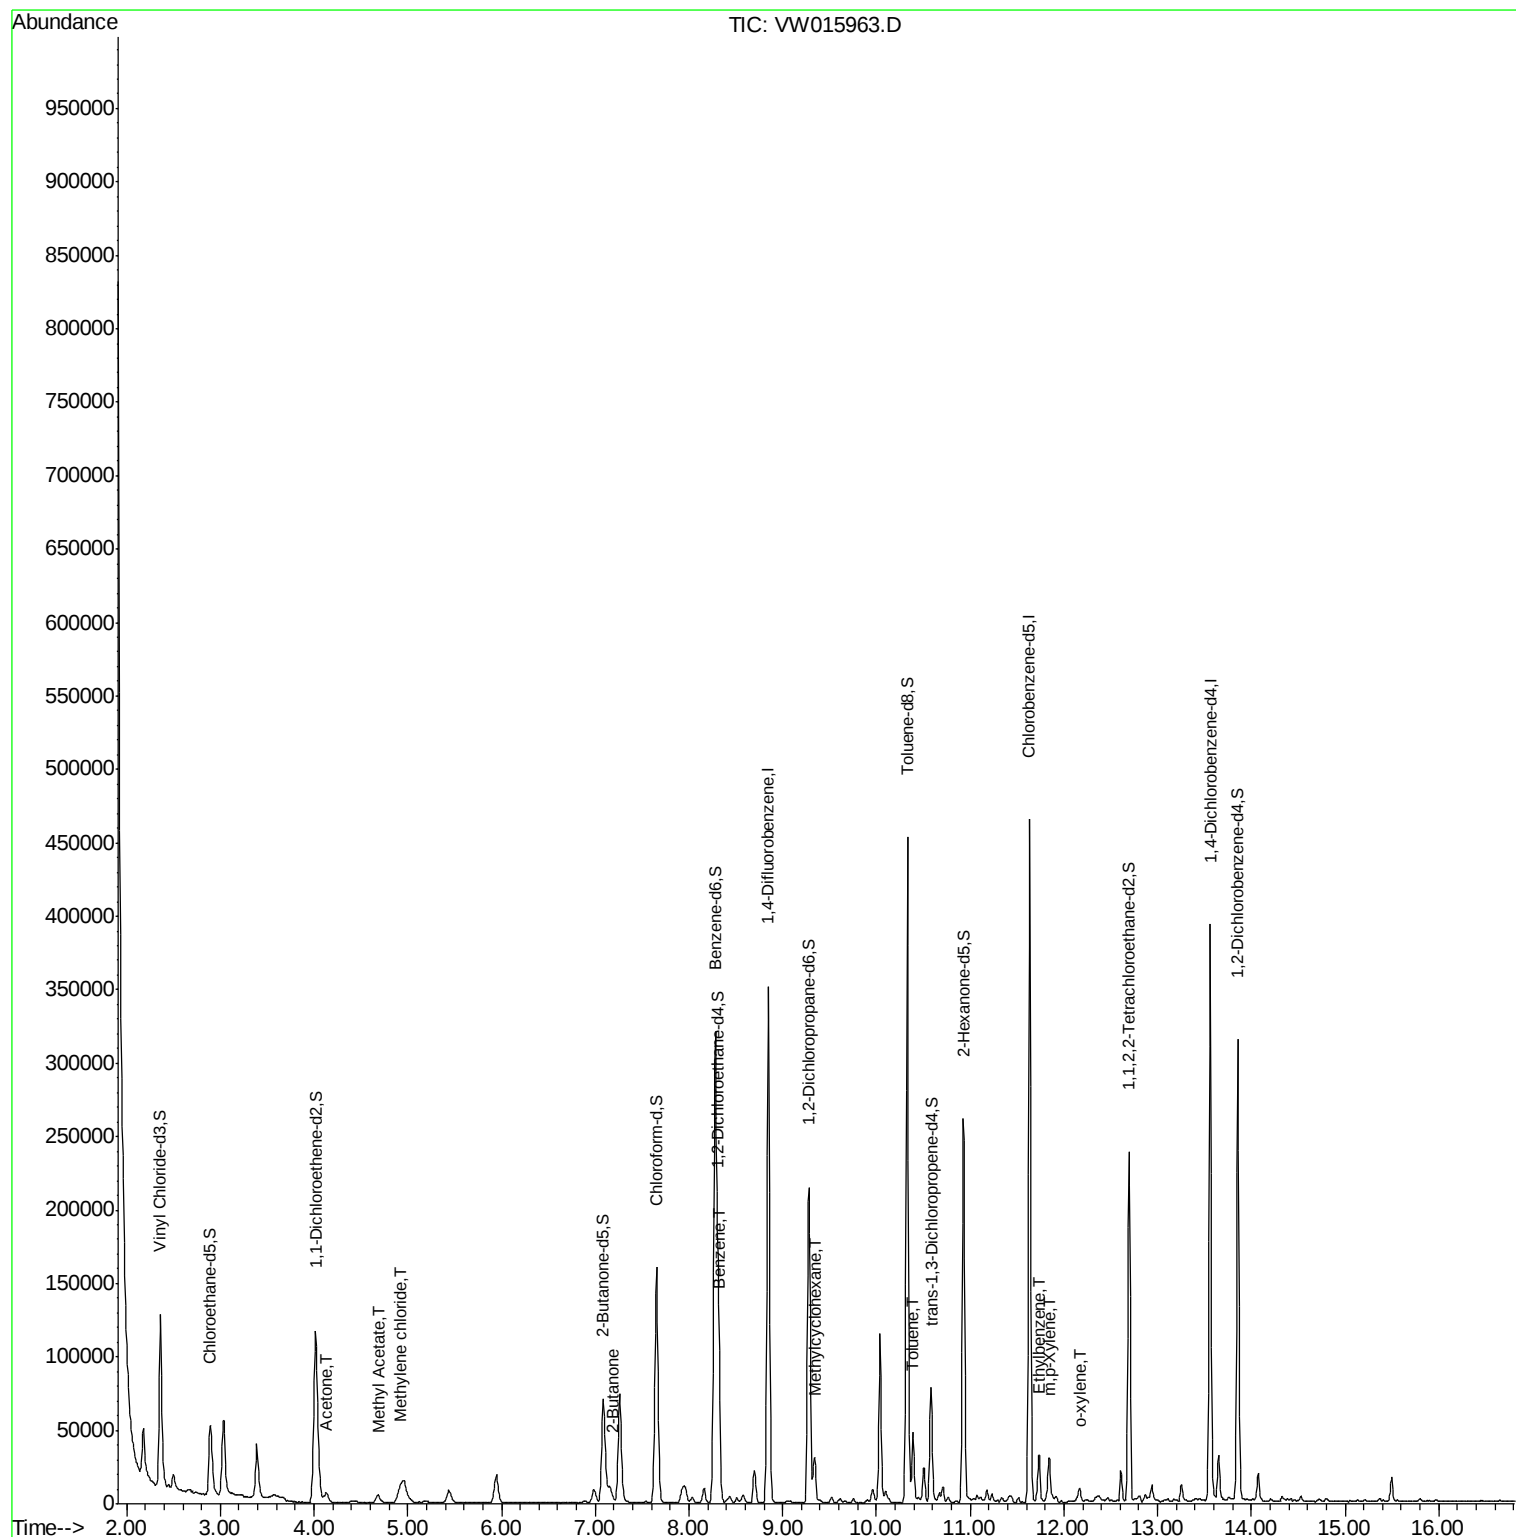

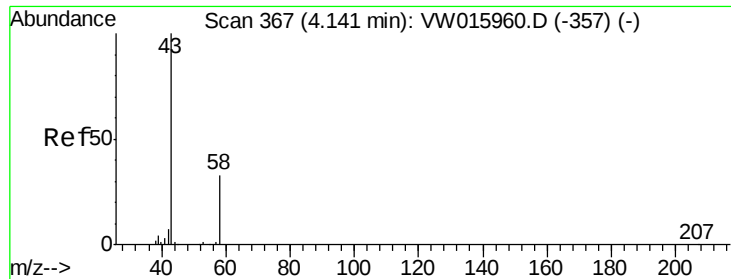

#13

Acetone

Concen: 11.102 ug/L

RT: 4.14 min Scan# 366

Delta R.T. -0.01 min

Lab File: VW015963.D

Acq: 27 Jul 2020 11:44

Instrument :

MSVOA_W

ClientSampled :

GAY30

Tot Ion: 43 Resp: 10138

Ion Ratio Lower Upper

43 100





58 15.9 0.0 58.2

Manual Integrations

APPROVED

MMDadoda

7/29/2020 7:52:15 PM

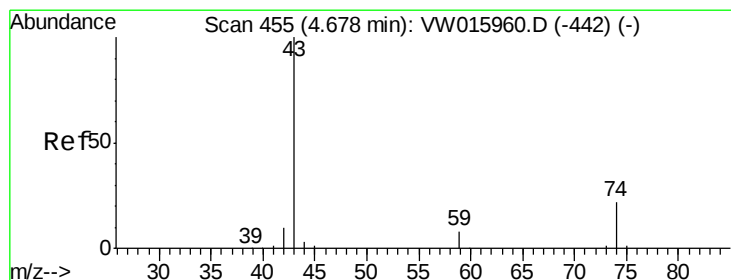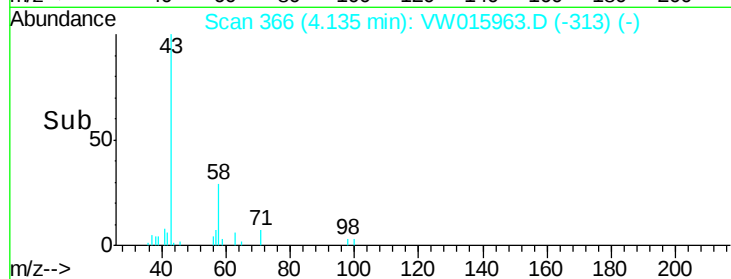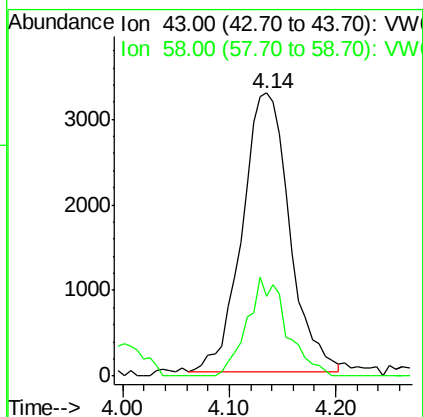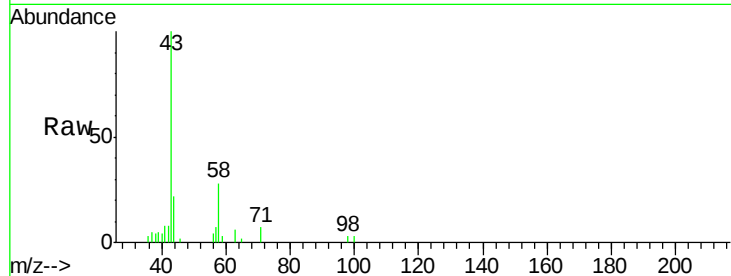

#15

Methyl Acetate

Concen: 6.066 ug/L

RT: 4.68 min Scan# 456

Delta R.T. 0.01 min

Lab File: VW015963.D




Acq: 27 Jul 2020 11:44


Tgt Ion: 43 Resp: 10444

Ion Ratio Lower Upper

43 100

74 20.6 18.2 27.2

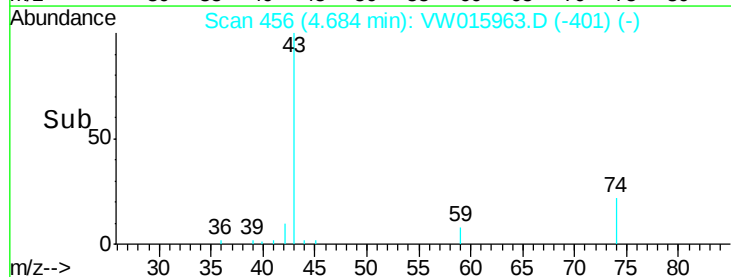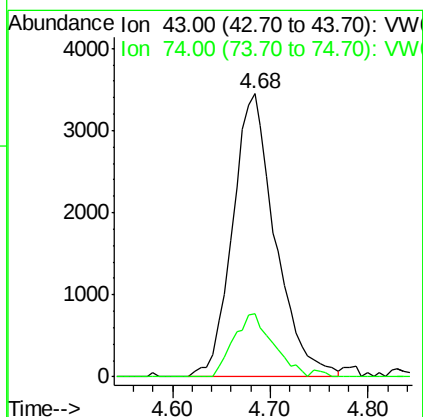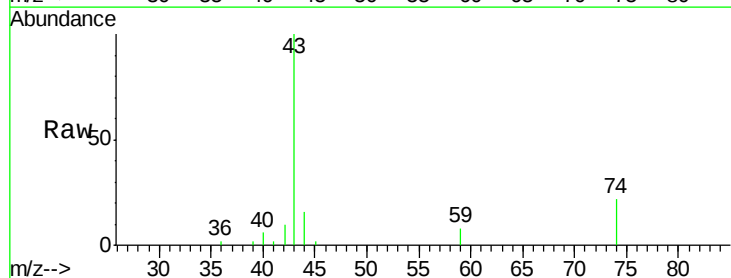

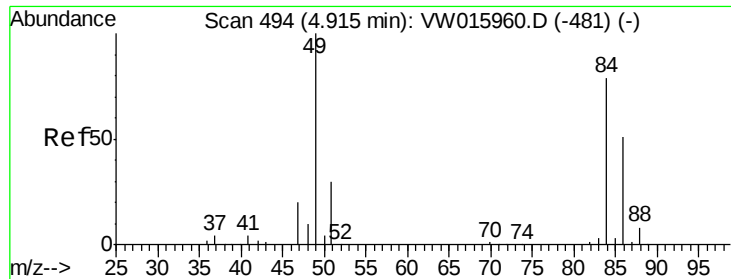





#16
Methvlene chloride
Concen: 1.583 ug/L m
RT: 4.92 min Scan# 495
Delta R.T. 0.01 min
Lab File: VW015963.D
Acq: 27 Jul 2020 11:44

Instrument :
MSVOA_W
ClientSampled :
GAY30

Tot Ion	84	Resp	7610
Ion Ratio	Lower	Upper	
84	100		
49	109.2	91.1	169.1
86	59.2	46.0	85.4




Manual Integrations
APPROVED


MMDadoda
7/29/2020 7:52:15 PM

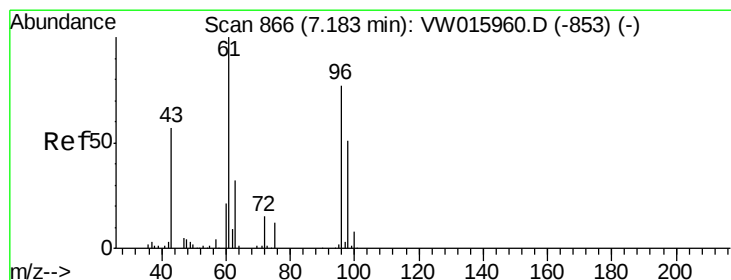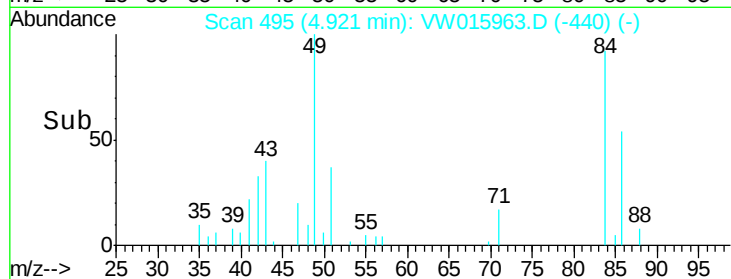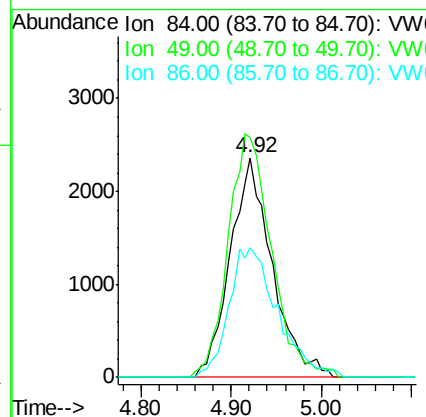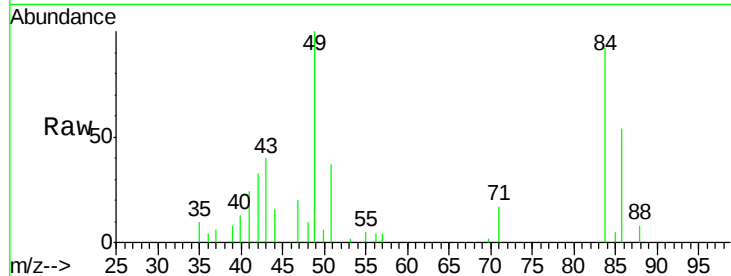

#21
2-Butanone
Concen: 2.687 ug/L m
RT: 7.19 min Scan# 867
Delta R.T. 0.01 min
Lab File: VW015963.D
Acq: 27 Jul 2020 11:44

Tgt Ion	43	Resp	3034
Ion Ratio	Lower	Upper	
43	100		
72	13.5	13.9	41.7#

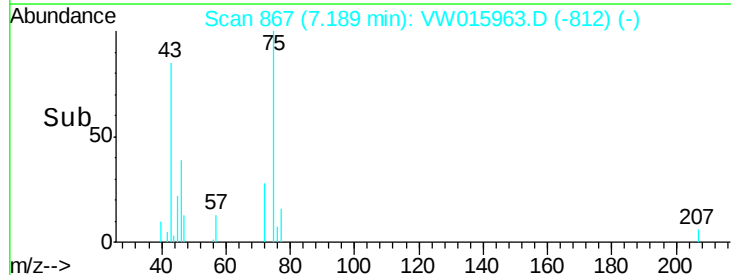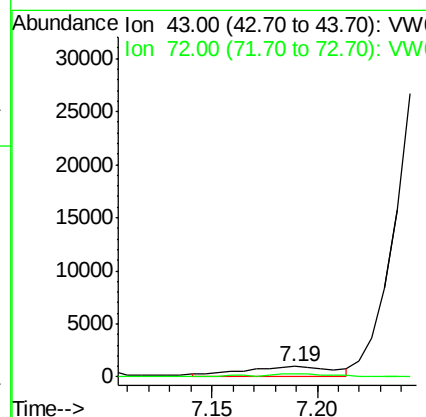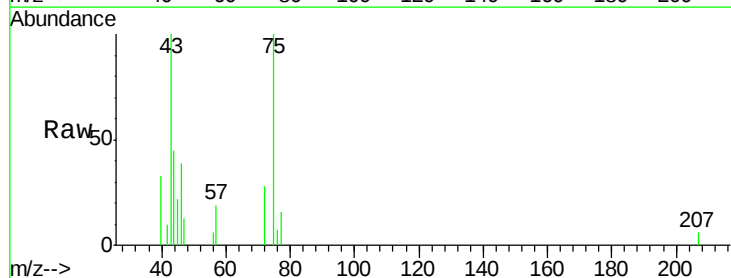

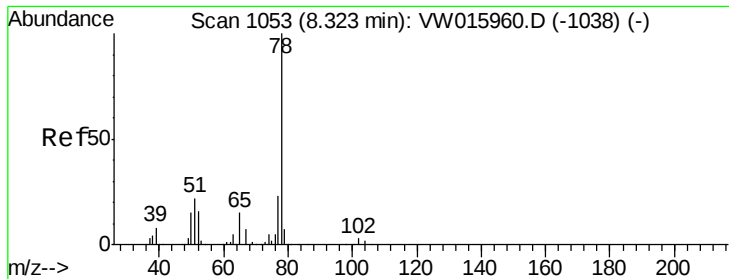

#34

Benzene

Concen: 0.851 ug/L

RT: 8.33 min Scan# 1054

Delta R.T. 0.01 min

Lab File: VW015963.D

Acq: 27 Jul 2020 11:44

Instrument :

MSVOA_W





ClientSampleId :

GAY30

Tgt Ion: 78 Resp: 13233

Manual Integrations
APPROVED

MMDadoda
7/29/2020 7:52:15 PM

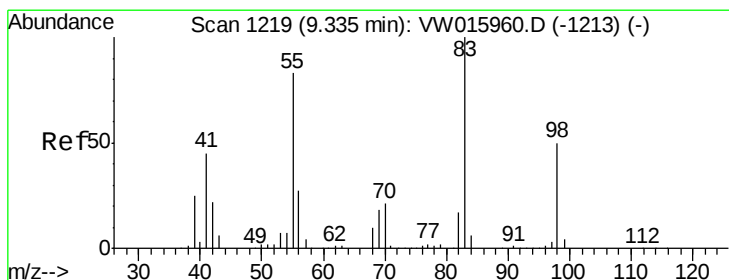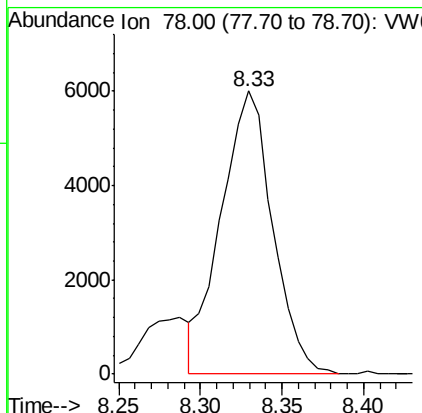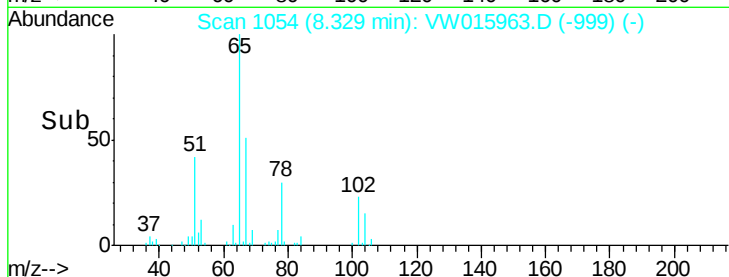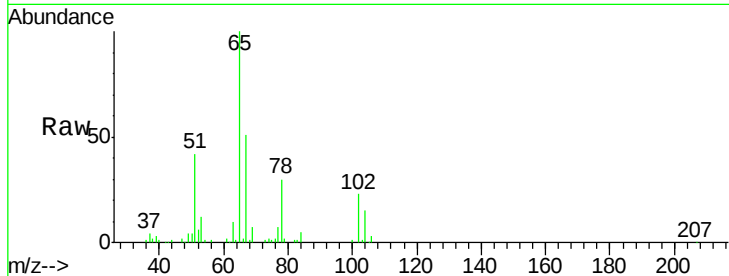

#36

Methylcyclohexane

Concen: 1.584 ug/L

RT: 9.34 min Scan# 1220




Delta R.T. 0.01 min


Lab File: VW015963.D

Acq: 27 Jul 2020 11:44

Tgt Ion: 83 Resp: 11186

Ion	Ratio	Lower	Upper
83	100		
55	90.5	63.5	95.3
98	50.0	39.0	58.4

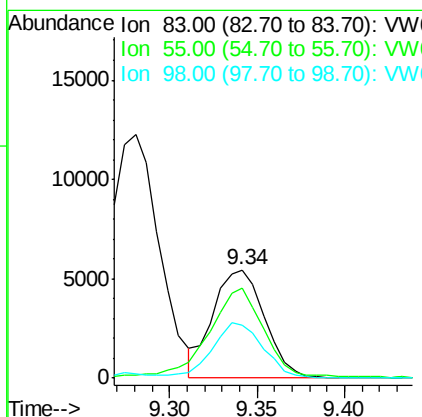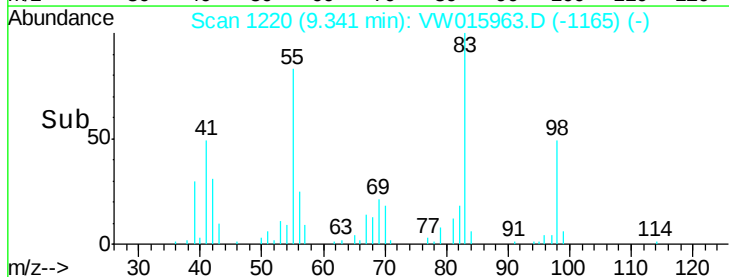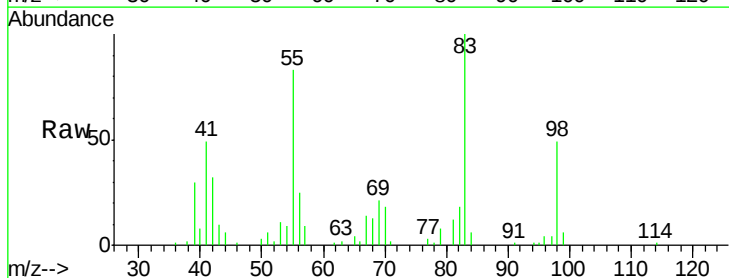

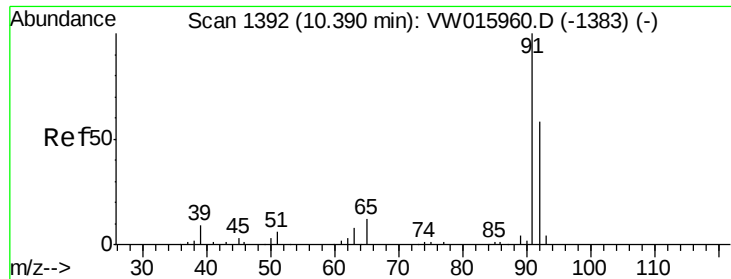





#44
Toluene
Concen: 2.069 ug/L
RT: 10.39 min Scan# 1392
Delta R.T. -0.00 min
Lab File: VW015963.D
Acq: 27 Jul 2020 11:44

Instrument :
MSVOA_W
ClientSampled :
GAY30

Tot Ion: 91 Resp: 33761
Ion Ratio Lower Upper
91 100
92 57.2 41.2 76.4




Manual Integrations
APPROVED


MMDadoda
7/29/2020 7:52:15 PM

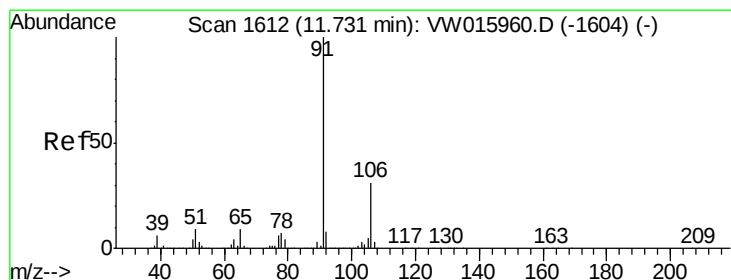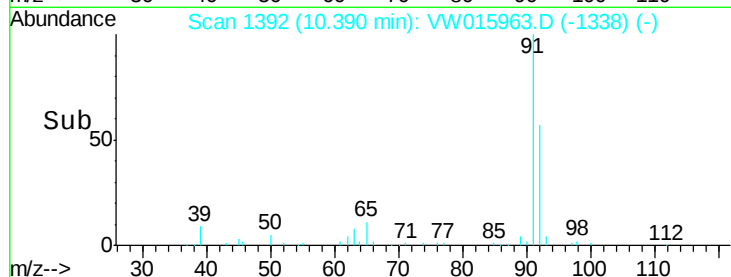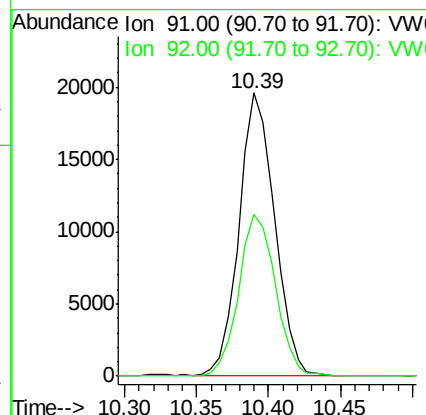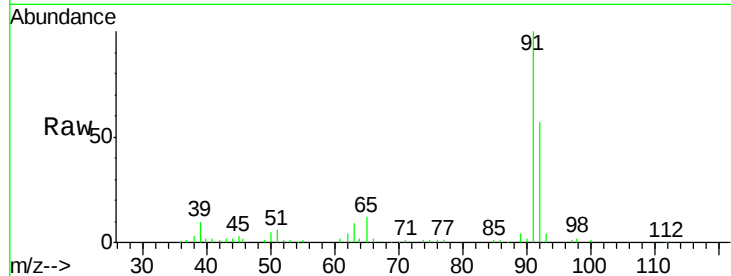

#53
Ethylbenzene
Concen: 1.195 ug/L
RT: 11.74 min Scan# 1613
Delta R.T. 0.01 min
Lab File: VW015963.D
Acq: 27 Jul 2020 11:44

Tgt Ion: 91 Resp: 21930
Ion Ratio Lower Upper
91 100
106 30.8 22.4 41.6

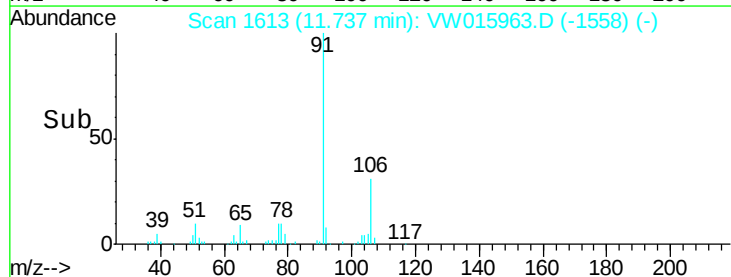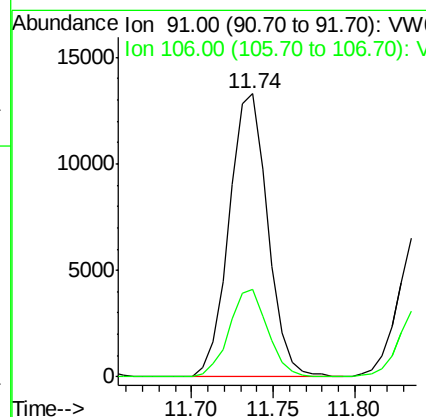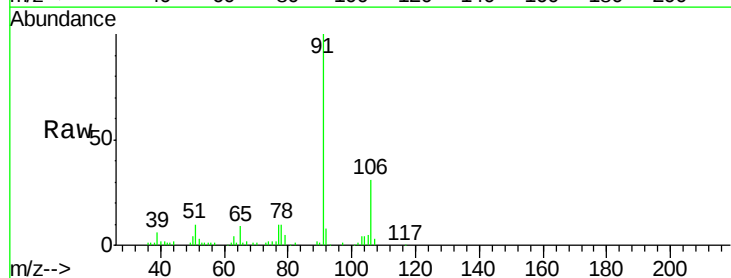

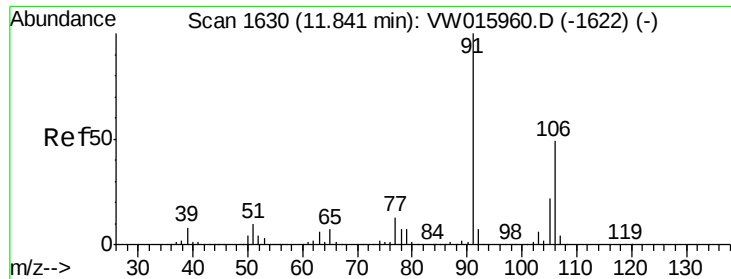

#54

m,p-Xylene

Concen: 0.870 ug/L

RT: 11.84 min Scan# 1630

Delta R.T. -0.00 min

Lab File: VW015963.D

Acq: 27 Jul 2020 11:44

Instrument :

MSVOA_W

ClientSampled :

GAY30

Tot Ion:106 Resp: 5971

Ion Ratio Lower Upper


106 100

91 195.7 144.1 267.5

Manual Integrations
APPROVED




MMDadoda

7/29/2020 7:52:15 PM

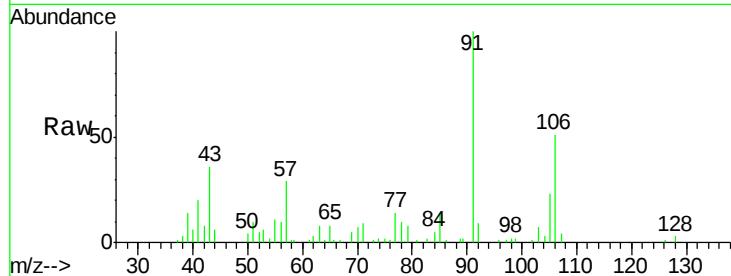

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

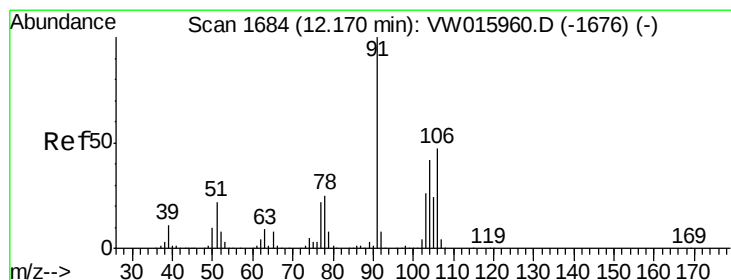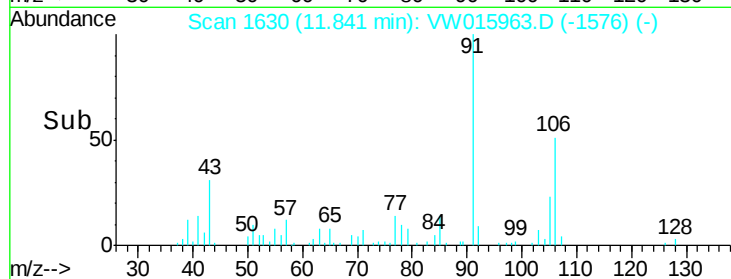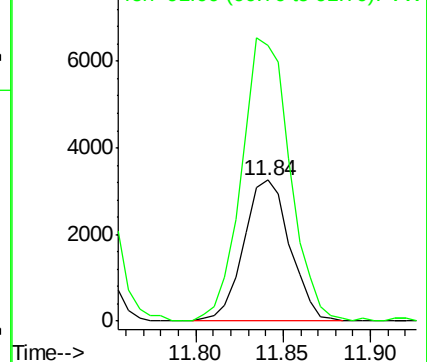

#55

o-xylene

Concen: 0.351 ug/L

RT: 12.17 min Scan# 1684

Delta R.T. -0.00 min

Lab File: VW015963.D


Acq: 27 Jul 2020 11:44

Tgt Ion:106 Resp: 2268

Ion Ratio Lower Upper

106 100

91 204.7 146.8 272.6

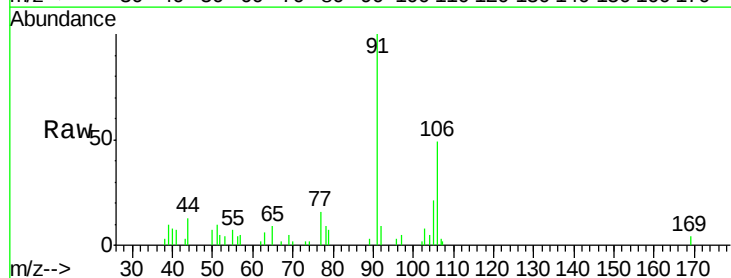

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

