


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW072720\
 Data File : VW015959.D
 Acq On : 27 Jul 2020 08:52
 Operator : SY/VA
 Sample : BFB25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB25

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Title : VOC Analysis
 Last Update : Tue Jul 28 01:36:11 2020

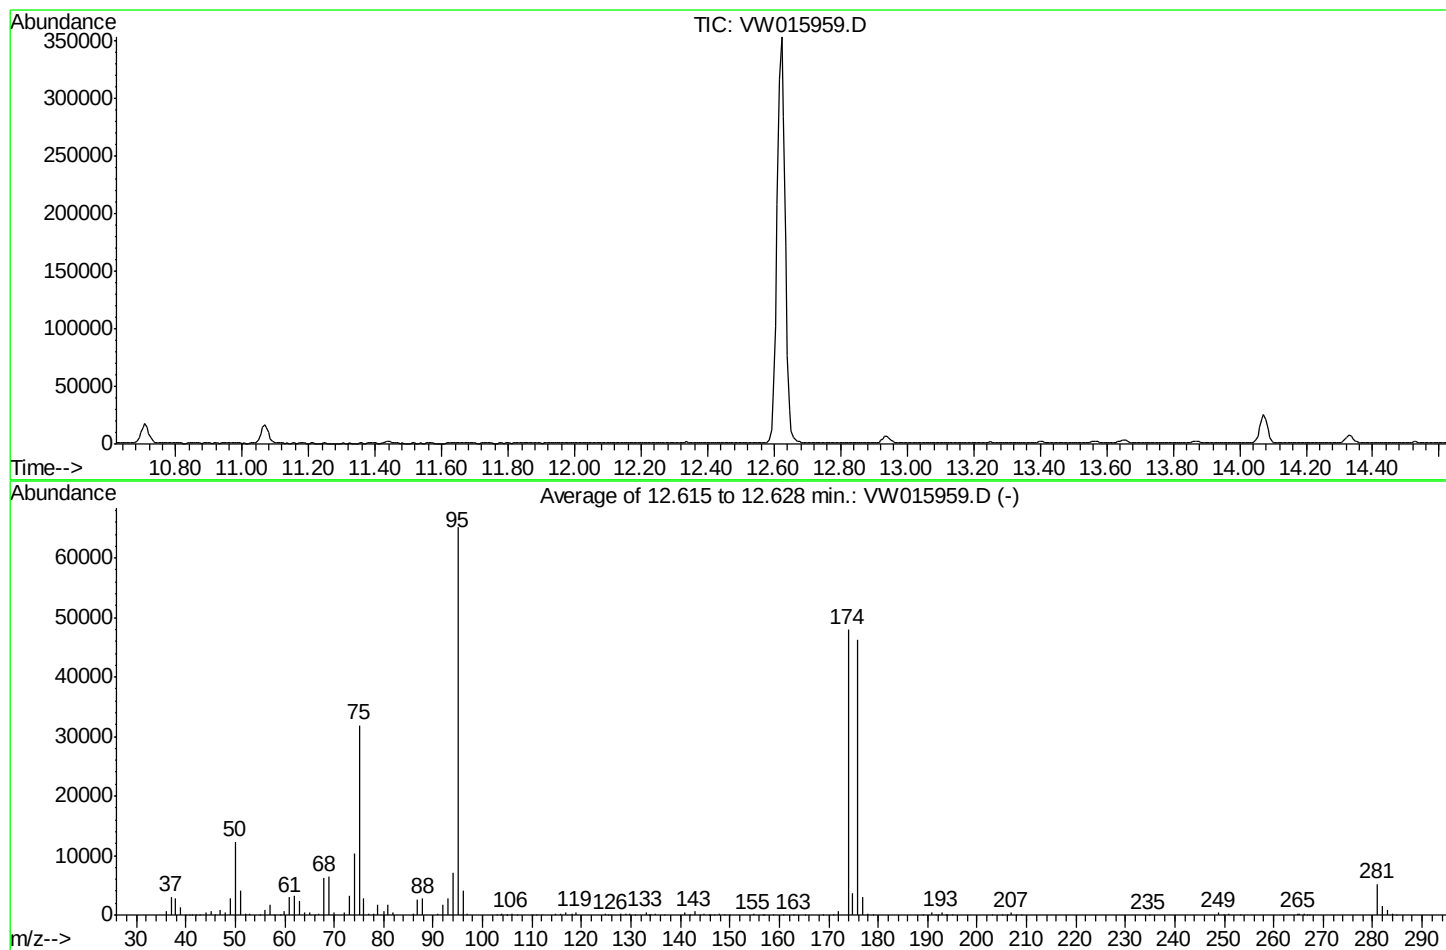

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	12313	PASS
75	95	30	80	49.0	31936	PASS
95	95	100	100	100.0	65162	PASS
96	95	5	9	6.4	4192	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	47946	PASS
175	174	5	9	7.6	3623	PASS
176	174	95	101	96.4	46208	PASS
177	176	5	9	6.7	3073	PASS

m/z	Abundance
36.00	918.0
37.00	3333.0
38.00	3369.0
39.00	1271.0
39.90	349.0
40.80	81.0
41.90	61.0
42.80	87.0
44.00	658.0
45.00	693.0
46.00	116.0
47.00	784.0
47.90	426.0
49.00	2793.0
50.00	12873.0
51.00	4237.0
52.00	200.0
52.90	145.0
55.00	208.0
56.00	969.0
57.00	1816.0
57.90	90.0
59.00	152.0
60.00	665.0
60.90	3012.0
62.00	3512.0
63.00	2695.0
64.00	399.0
65.00	548.0
65.90	101.0
67.10	154.0
68.00	6183.0
69.00	6653.0
70.00	531.0
72.00	416.0
73.00	3548.0
74.00	10293.0
75.00	32120.0
76.00	2798.0
76.90	347.0
77.90	277.0
78.90	1883.0
80.00	638.0
80.90	1785.0
81.90	441.0
85.80	187.0
86.90	2875.0
87.90	2776.0
90.90	250.0
91.90	1628.0
92.90	2549.0
94.00	7274.0
95.00	64248.0
96.00	4113.0
96.90	166.0
102.80	165.0
103.70	276.0
104.80	112.0
105.90	278.0
106.80	98.0
109.90	92.0
111.00	114.0
112.00	118.0
114.80	161.0
115.80	230.0
116.90	427.0
118.10	226.0
118.90	514.0
124.80	267.0
125.90	107.0
127.90	193.0
128.90	123.0
129.80	190.0
130.90	95.0
133.00	802.0
134.90	154.0
136.80	121.0
140.90	527.0
141.90	63.0
142.80	589.0
144.80	216.0
145.80	86.0
146.80	167.0
147.80	184.0
149.00	79.0
149.90	87.0
154.80	180.0
156.80	103.0
158.80	77.0
160.90	132.0
162.90	160.0
165.10	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

169.00	94.0
170.80	69.0
171.90	666.0
173.90	42560.0
174.90	3515.0
175.90	41448.0
176.90	2767.0
177.90	211.0
178.90	161.0
188.90	101.0
191.00	523.0
192.10	154.0
192.90	751.0
193.80	128.0
194.90	91.0
202.90	96.0
205.00	168.0
206.10	93.0
206.90	625.0
208.90	72.0
234.80	77.0
248.90	443.0
249.90	94.0
250.90	331.0
264.80	499.0
266.20	220.0
267.10	270.0
281.00	7826.0
282.00	1955.0
283.10	1424.0
283.90	278.0
284.90	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
35.90	956.0
37.00	3354.0
38.00	3495.0
39.00	1507.0
39.90	247.0
40.80	118.0
41.90	81.0
43.00	143.0
44.00	786.0
45.00	732.0
46.10	118.0
46.90	911.0
47.90	522.0
49.00	2999.0
50.00	13354.0
51.00	4443.0
52.10	155.0
52.90	119.0
54.90	208.0
55.90	1026.0
57.00	1844.0
57.90	89.0
59.10	94.0
59.90	732.0
61.00	3306.0
62.00	3301.0
63.00	2765.0
63.90	385.0
65.00	576.0
66.00	116.0
66.90	275.0
68.00	6904.0
69.00	7344.0
70.00	583.0
71.90	438.0
73.00	3313.0
74.00	11710.0
75.00	35184.0
76.00	3169.0
76.90	289.0
78.00	272.0
78.90	1970.0
79.90	607.0
80.90	1805.0
81.80	492.0
85.90	113.0
86.90	2944.0
87.90	3082.0
90.90	280.0
92.00	1851.0
93.00	3029.0
94.00	7930.0
95.00	71664.0
96.00	4534.0
97.00	149.0
102.80	104.0
103.90	280.0
105.00	118.0
105.90	295.0
106.90	62.0
110.00	85.0
110.80	102.0
111.90	99.0
114.90	107.0
115.80	185.0
116.90	457.0
118.00	295.0
118.80	404.0
124.80	143.0
125.40	82.0
127.70	213.0
128.80	62.0
129.90	247.0
130.80	103.0
133.00	431.0
133.70	101.0
134.00	109.0
134.90	136.0
136.90	146.0
141.00	562.0
141.80	93.0
142.90	706.0
144.00	53.0
144.90	167.0
146.00	96.0
146.80	111.0
147.90	117.0
149.90	76.0
154.80	142.0
156.70	110.0
158.90	81.0
160.90	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

162.90	115.0
168.90	73.0
170.80	51.0
171.90	734.0
173.90	57176.0
174.90	3876.0
175.90	50976.0
176.90	3311.0
177.80	169.0
178.80	91.0
188.90	53.0
190.90	318.0
191.70	86.0
192.90	468.0
194.00	101.0
194.90	58.0
204.90	121.0
207.00	403.0
208.00	63.0
208.90	78.0
248.90	373.0
251.00	177.0
253.10	56.0
265.00	628.0
266.00	121.0
266.80	83.0
281.00	5249.0
282.00	1644.0
283.10	827.0
284.00	219.0
284.90	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
36.00	749.0
37.10	2572.0
38.00	2192.0
39.00	1138.0
39.90	238.0
41.10	61.0
42.70	65.0
44.00	477.0
44.90	393.0
45.10	413.0
45.90	66.0
47.00	668.0
48.00	374.0
49.00	2389.0
50.00	10714.0
51.00	3364.0
52.00	152.0
52.90	84.0
55.00	188.0
55.90	731.0
57.00	1579.0
57.90	61.0
60.00	552.0
61.00	2568.0
62.00	2715.0
62.90	1894.0
63.90	218.0
65.00	518.0
67.00	164.0
68.00	5807.0
69.00	5641.0
69.90	363.0
72.00	313.0
73.00	2825.0
74.00	9185.0
75.00	28504.0
76.00	2273.0
77.00	319.0
78.00	225.0
78.80	1586.0
80.00	458.0
80.90	1533.0
81.90	403.0
86.00	155.0
86.90	2235.0
87.90	2308.0
91.00	216.0
92.00	1571.0
92.90	2653.0
94.00	6125.0
95.00	59576.0
96.00	3930.0
96.90	127.0
103.90	235.0
105.80	213.0
106.80	63.0
111.90	69.0
114.90	81.0
115.70	157.0
116.90	320.0
117.90	260.0
118.90	430.0
124.90	111.0
127.90	208.0
128.90	180.0
129.80	220.0
130.80	76.0
133.00	294.0
134.80	172.0
136.80	62.0
140.90	510.0
141.80	77.0
143.00	587.0
144.80	158.0
145.90	75.0
147.90	153.0
150.00	79.0
154.90	186.0
157.00	76.0
160.80	58.0
168.90	101.0
172.00	753.0
173.90	44104.0
174.90	3479.0
175.90	46200.0
176.90	3143.0
177.80	150.0
190.90	287.0
193.00	193.0
207.00	174.0
248.80	126.0
249.00	125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

250.80	104.0
265.00	241.0
266.10	53.0
281.10	2745.0
282.00	719.0
283.00	418.0
283.90	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

Scan 1749 (12.567 min): VW015959.D
BFB25

m/z	Abundance
36.00	302.0
37.90	186.0
40.00	184.0
43.00	59.0
43.90	287.0
54.90	101.0
169.00	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25