

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080520\
 Data File : VW016038.D
 Acq On : 05 Aug 2020 11:26
 Operator : SY/VA
 Sample : VW0805SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK26

Quant Time: Aug 06 02:53:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 05 03:09:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	249387	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	232702	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	106308	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	82547	23.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.84%
7) Chloroethane-d5	2.90	69	62556	21.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.56%
10) 1,1-Dichloroethene-d2	4.01	63	129925	18.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.04%
20) 2-Butanone-d5	7.09	46	45939	49.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.40%
24) Chloroform-d	7.65	84	172874	24.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.72%
26) 1,2-Dichloroethane-d4	8.31	65	94626	24.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.44%
29) Benzene-d6	8.27	84	347851	24.56	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.24%
33) 1,2-Dichloropropane-d6	9.27	67	102806	24.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.84%
37) Toluene-d8	10.33	98	328643	25.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.44%
38) trans-1,3-Dichloropropene-	10.58	79	45247	25.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.00%
39) 2-Hexanone-d5	10.93	63	35123	49.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82531	25.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	111359	26.86	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.44%


Target Compounds					Ovalue
42) cis-1,3-Dichloropropene	10.04	75	3191	0.598 ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW080520\
Data File : VW016038.D
Acq On : 05 Aug 2020 11:26
Operator : SY/VA
Sample : VW0805SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK26

Quant Time: Aug 06 02:53:19 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 05 03:09:52 2020
Response via : Initial Calibration

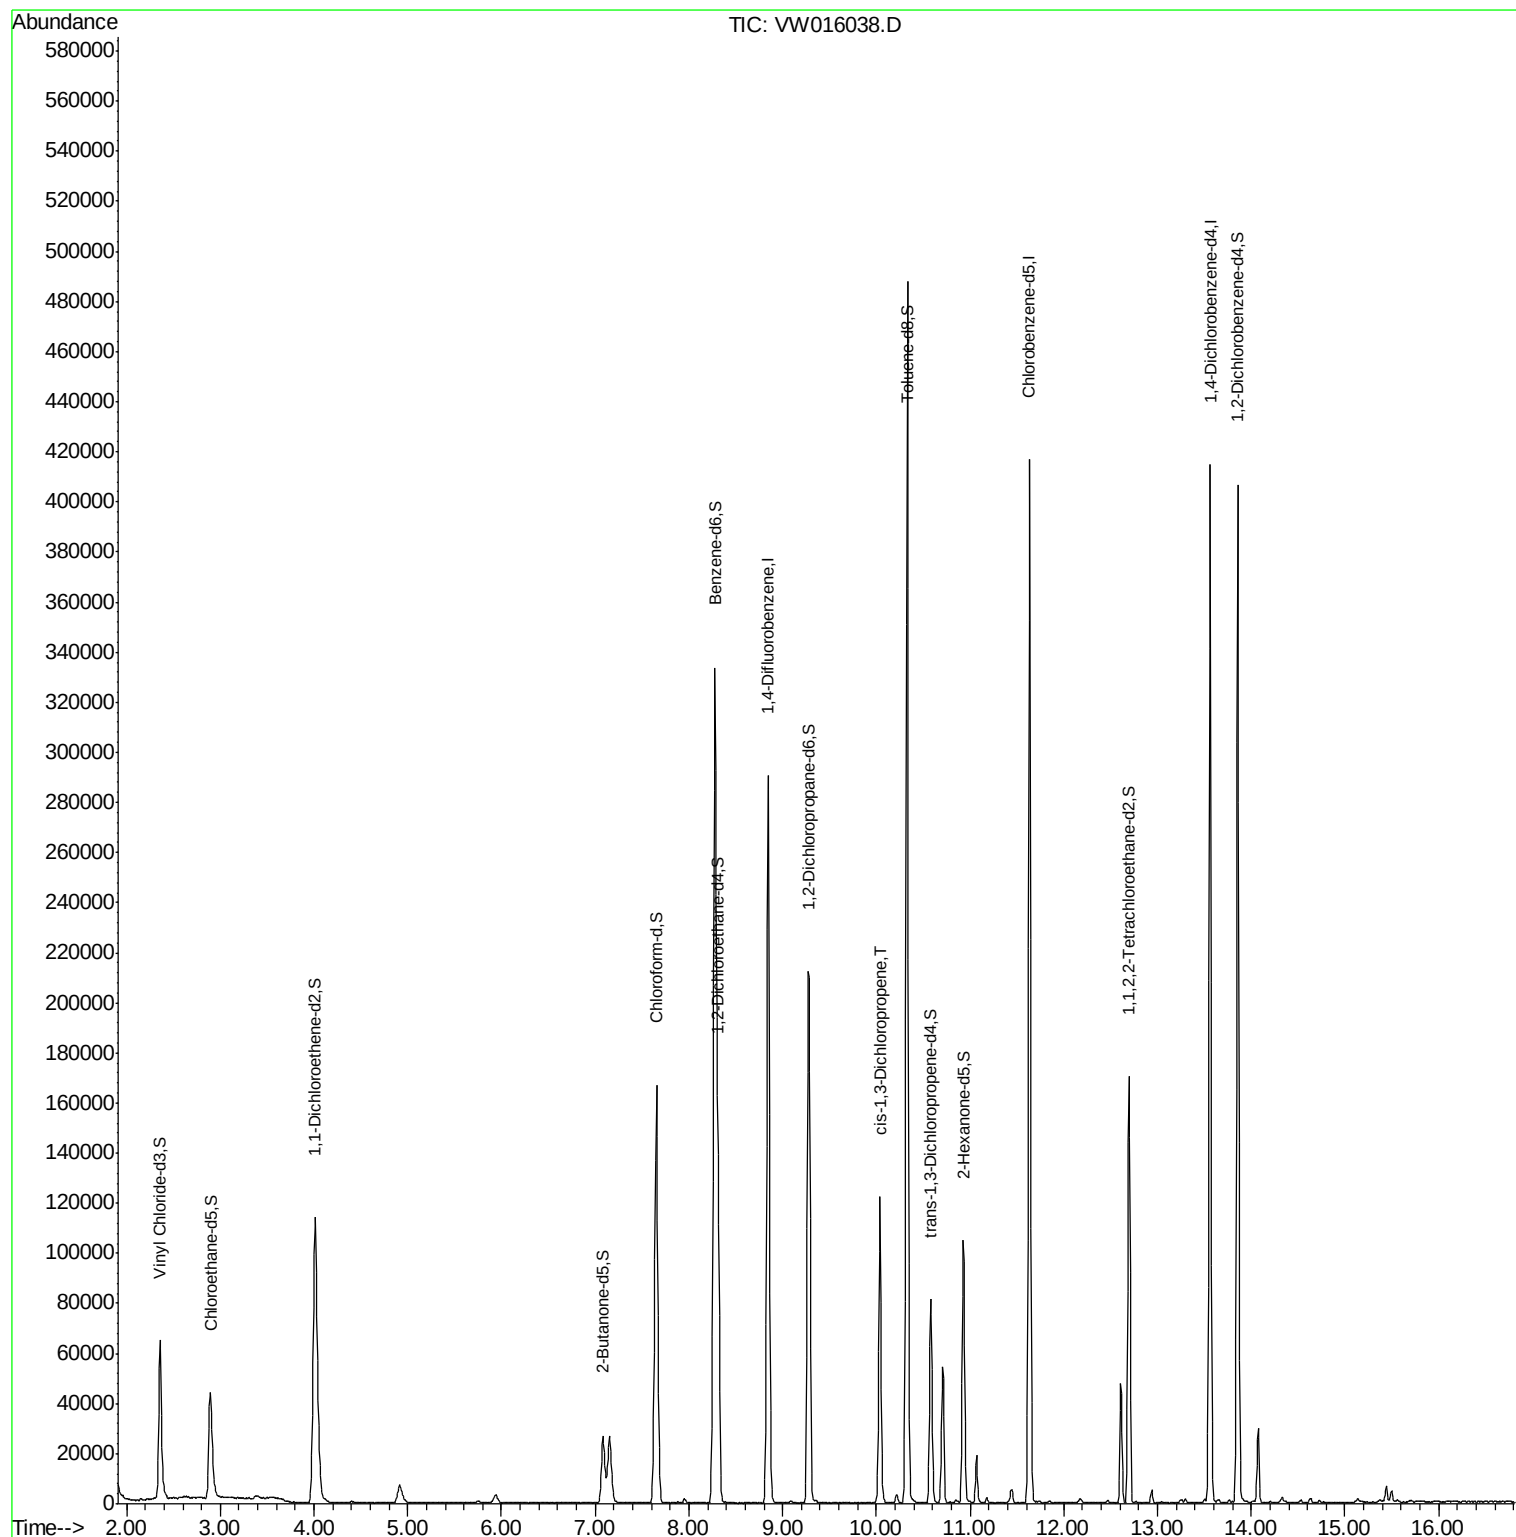

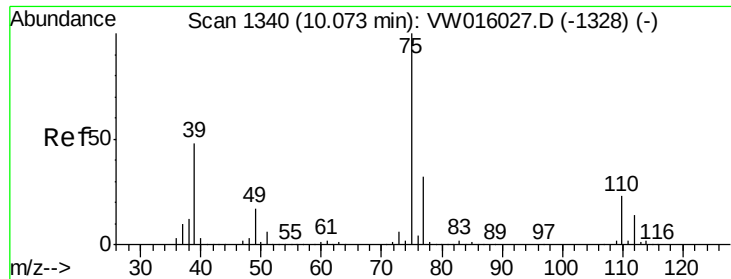

#42

cis-1,3-Dichloropropene

Concen: 0.598 ug/L

RT: 10.04 min Scan# 1334

Delta R.T. -0.04 min

Lab File: VW016038.D

Acq: 05 Aug 2020 11:26

Instrument :

MSVOA_W

ClientSampleId :

VBLK26

Tot Ion: 75 Resp: 3191

Ion Ratio Lower Upper

75 100

77 50.3 22.2 41.2#

