


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW080618\
Data File : VW004475.D
Acq On : 06 Aug 2018 17:17
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W080618S.M
Title : SW846 8260
Last Update : Tue Aug 07 08:22:01 2018

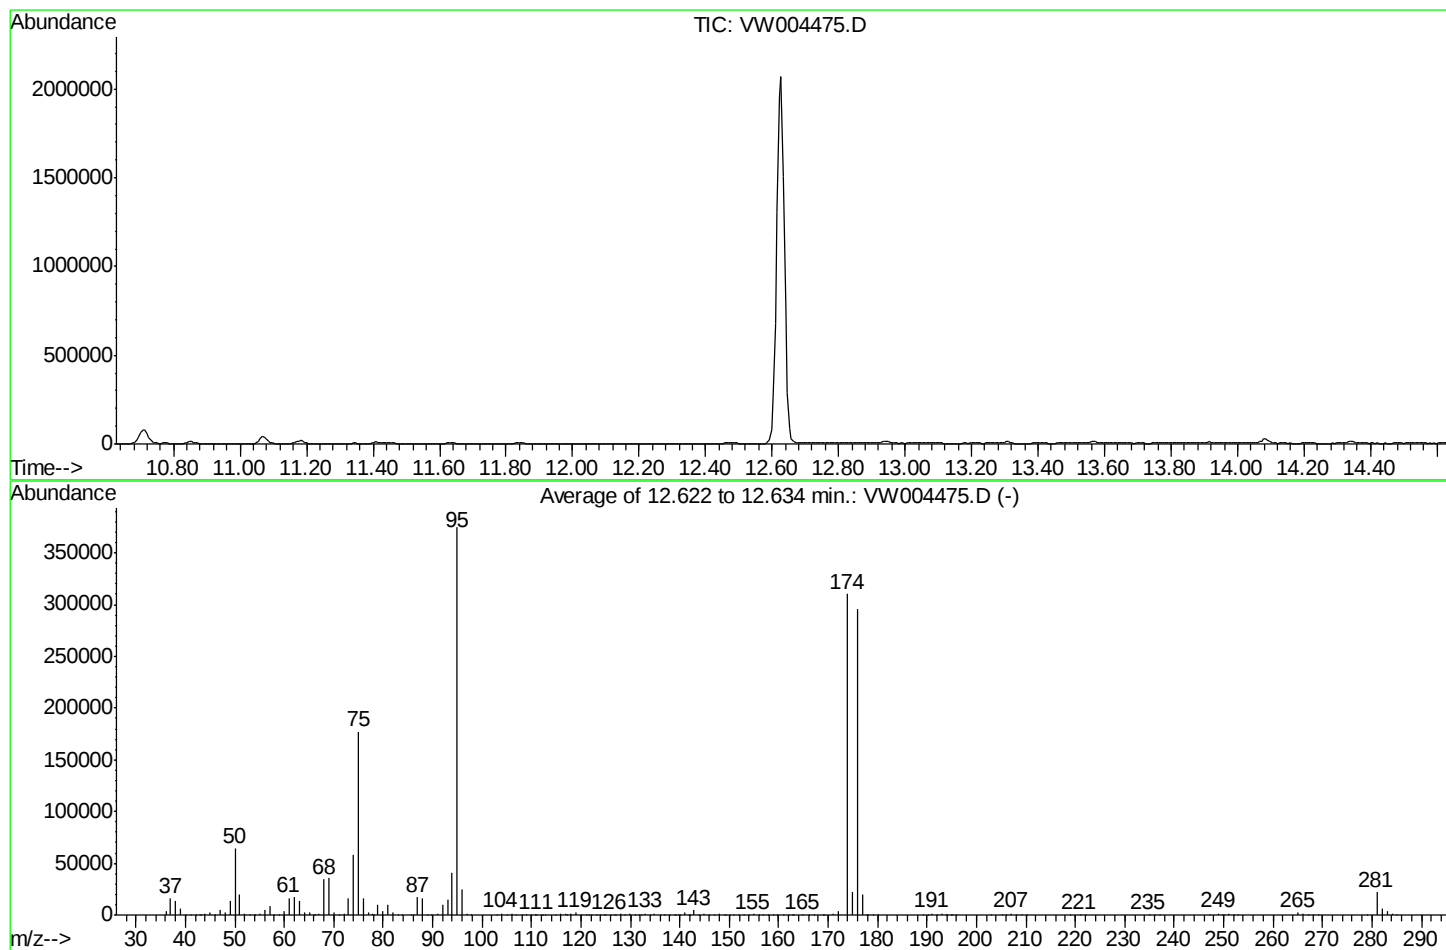

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	64232	PASS
75	95	30	60	47.4	177472	PASS
95	95	100	100	100.0	374677	PASS
96	95	5	9	6.7	25042	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	310421	PASS
175	174	5	9	7.4	22912	PASS
176	174	95	101	95.4	296128	PASS
177	176	5	9	6.6	19528	PASS