

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024208.D
 Acq On : 09 Aug 2022 14:41
 Operator : SY/VA
 Sample : N4110-06
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF9

Quant Time: Aug 10 01:10:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	344648	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	335040	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	155874	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	210772	29.258	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	117.040%
7) Chloroethane-d5	2.873	69	128857	28.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.840%
11) 1,1-Dichloroethene-d2	4.001	63	140230	17.080	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.320%
21) 2-Butanone-d5	7.080	46	60570	45.192	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.380%
24) Chloroform-d	7.641	84	250961	24.066	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.280%
26) 1,2-Dichloroethane-d4	8.299	65	139919	24.167	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.680%
32) Benzene-d6	8.269	84	497840	25.195	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	9.268	67	140866	24.146	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.600%
41) Toluene-d8	10.323	98	464955	25.175	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.680%
43) trans-1,3-Dichloroprop...	10.573	79	59606	23.326	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.320%
47) 2-Hexanone-d5	10.921	63	50946	47.278	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.560%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	126381	22.328	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	154001	26.999	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.000%
Target Compounds						Qvalue
13) Acetone	4.129	43	10050	10.185	ug/L	85
39) cis-1,3-Dichloropropene	10.031	75	5061	0.703	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
Data File : VW024208.D
Acq On : 09 Aug 2022 14:41
Operator : SY/VA
Sample : N4110-06
Misc : 4.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZF9

Quant Time: Aug 10 01:10:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 10 01:09:21 2022
Response via : Initial Calibration




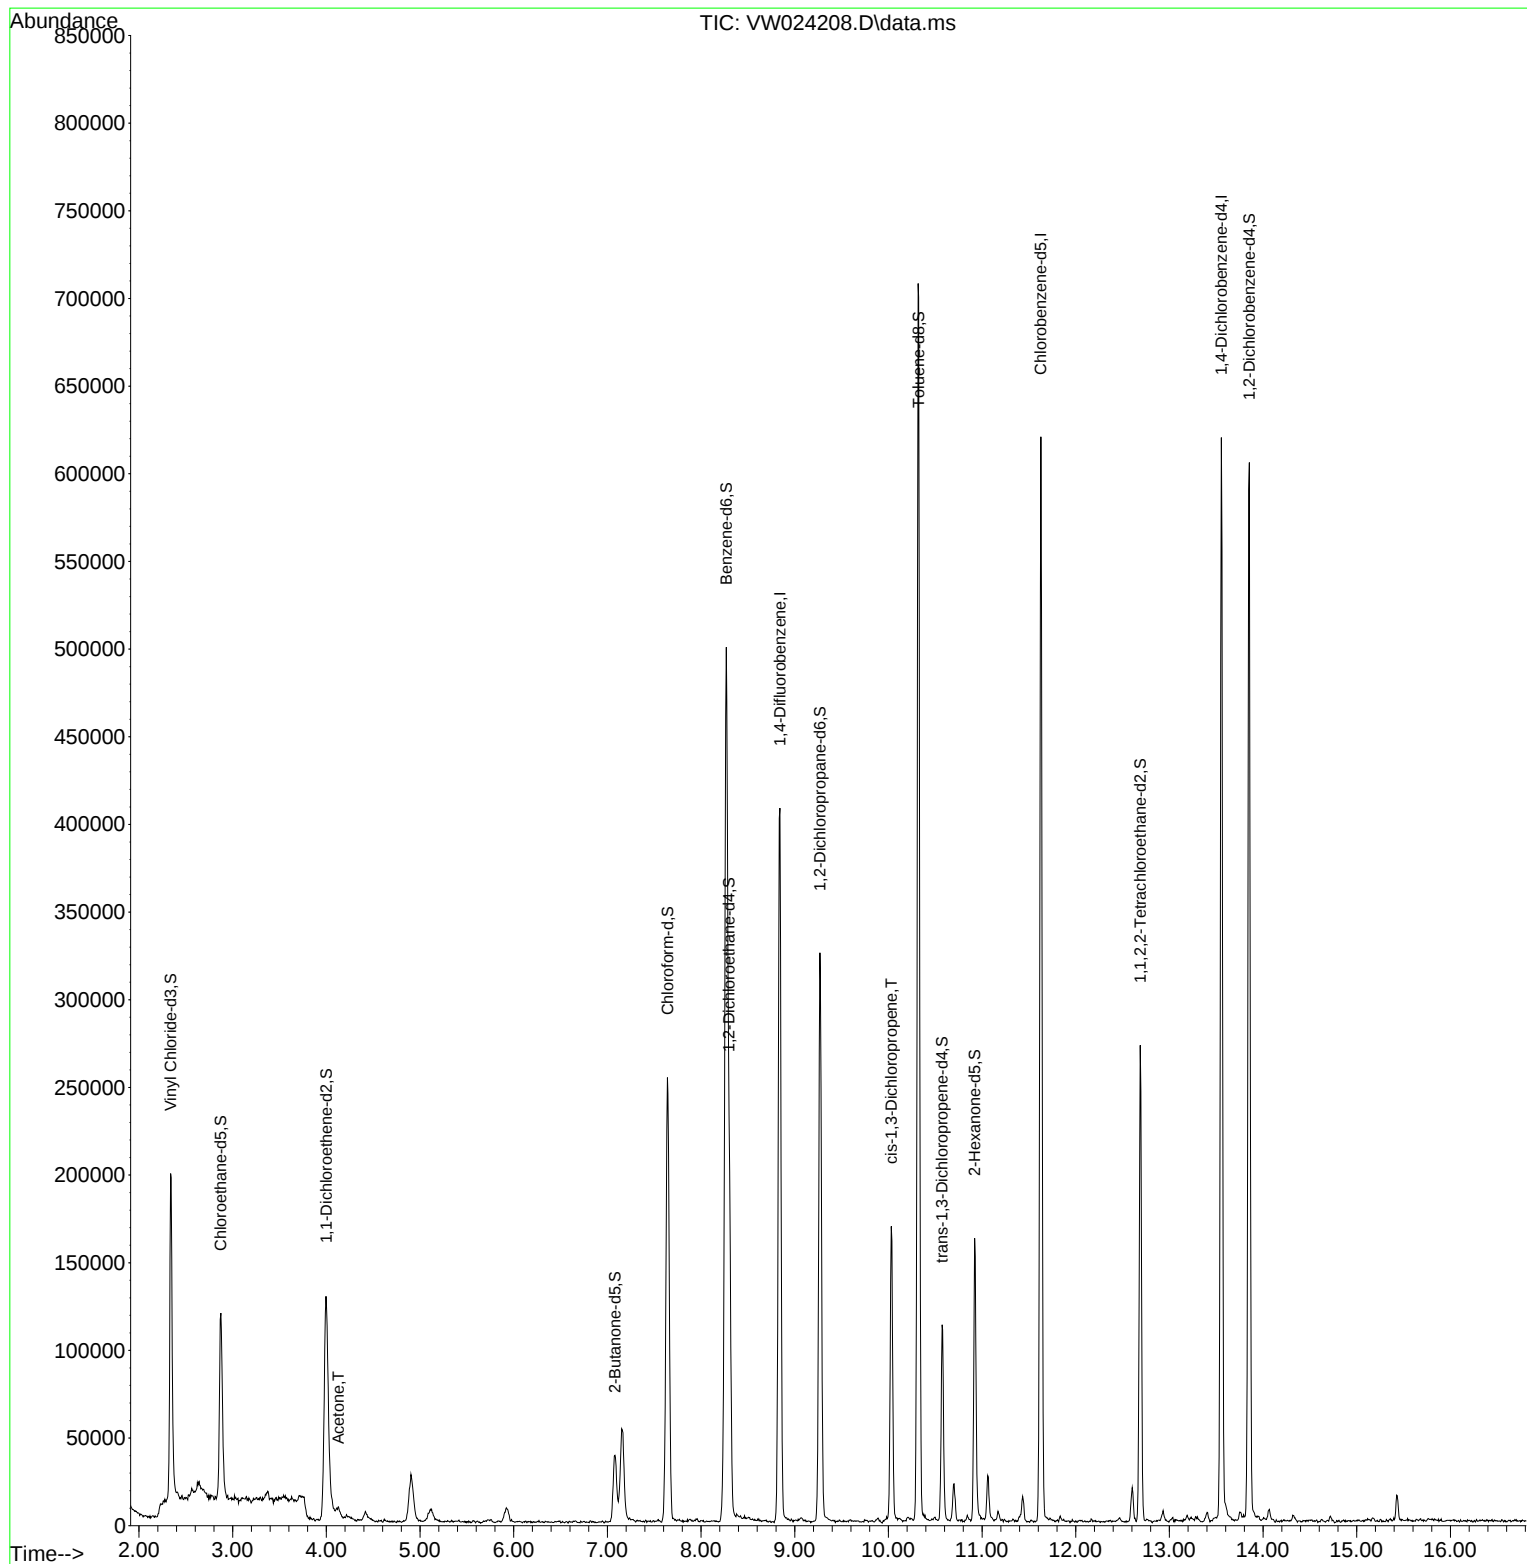


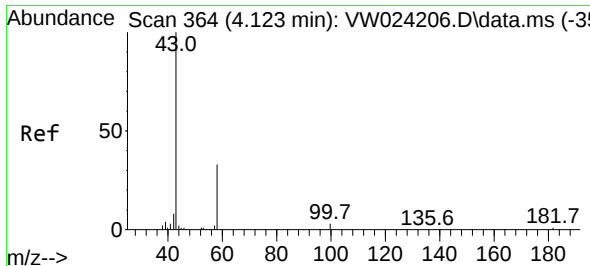

#13
Acetone
Concen: 10.185 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW024208.D
Acq: 09 Aug 2022 14:41

Instrument :
MSVOA_W
ClientSampleId :
C0ZF9

Tgt Ion: 43 Resp: 10050
Ion Ratio Lower Upper
43 100
58 22.3 0.0 31.8

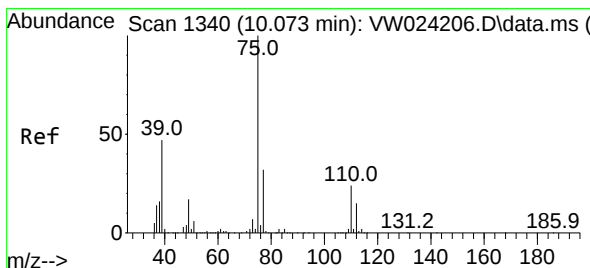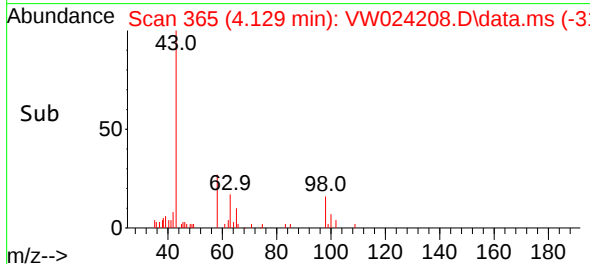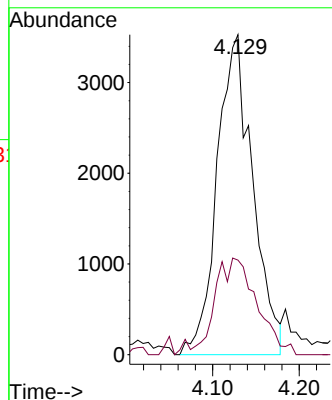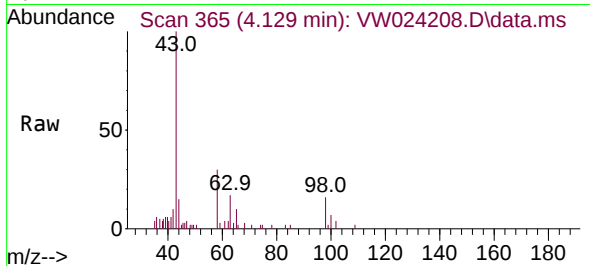

#39
cis-1,3-Dichloropropene
Concen: 0.703 ug/L
RT: 10.031 min Scan# 1333
Delta R.T. -0.043 min
Lab File: VW024208.D
Acq: 09 Aug 2022 14:41

Tgt Ion: 75 Resp: 5061
Ion Ratio Lower Upper
75 100
77 51.3 23.4 43.6#

