




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024209.D
 Acq On : 09 Aug 2022 15:11
 Operator : SY/VA
 Sample : N4110-02
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

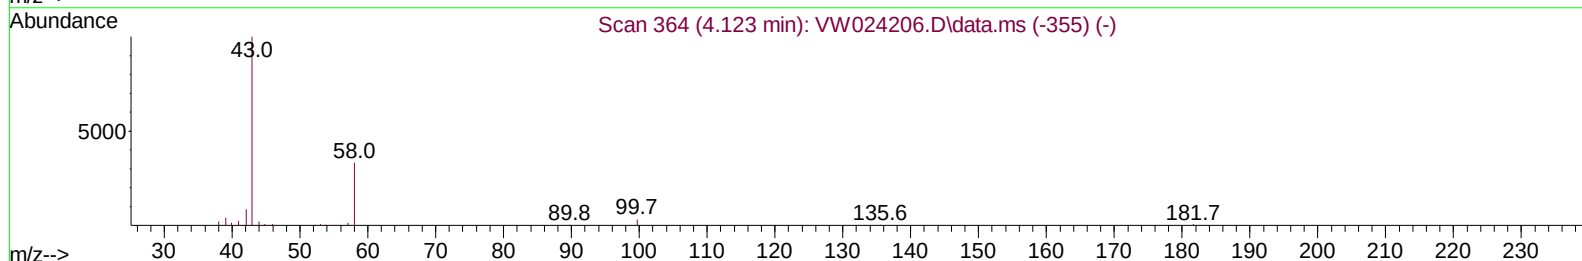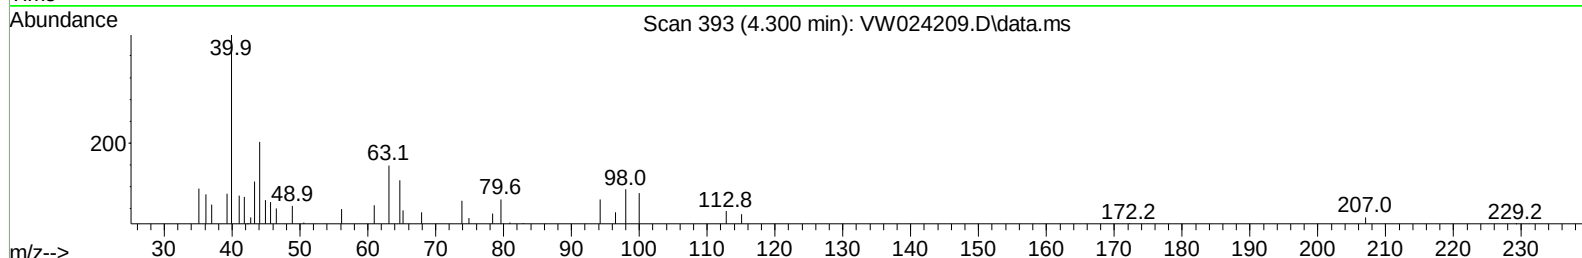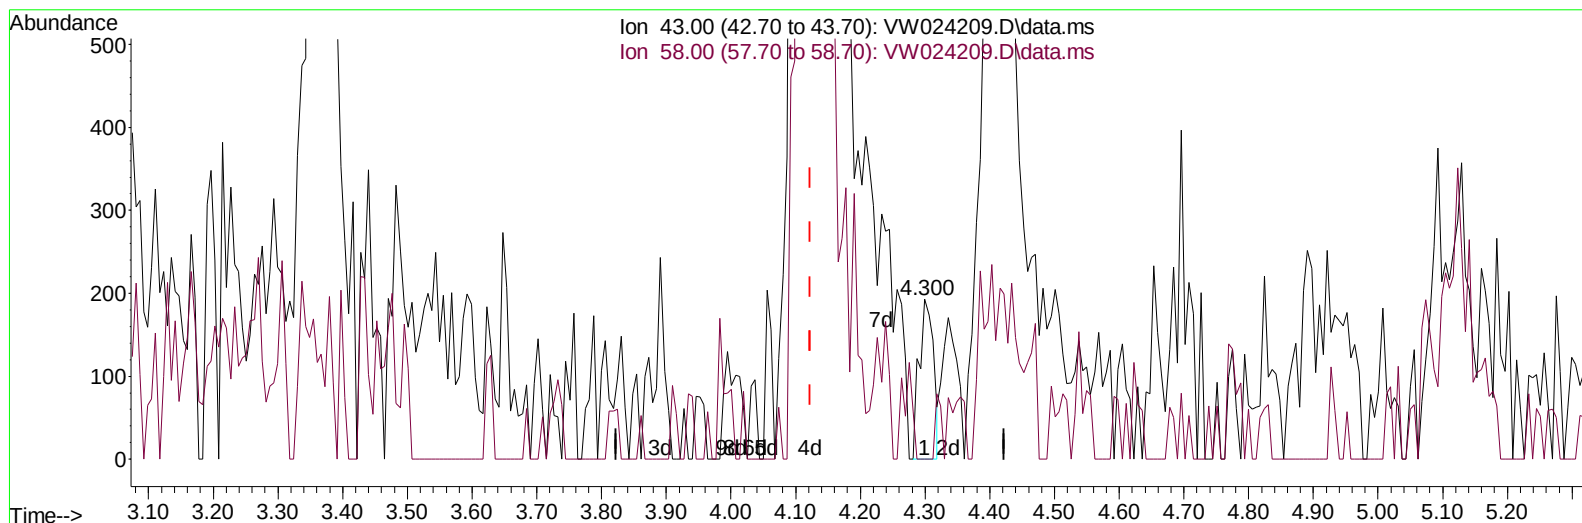

TIC: VW024209.D\data.ms

(13) Acetone (T)

4.300min (+ 0.177) 0.28 ug/L

response 294

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	17.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024209.D
 Acq On : 09 Aug 2022 15:11
 Operator : SY/VA
 Sample : N4110-02
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

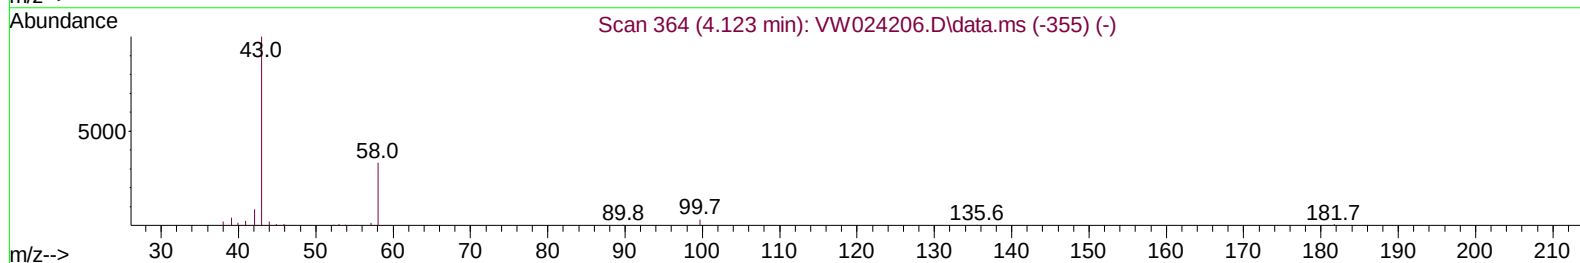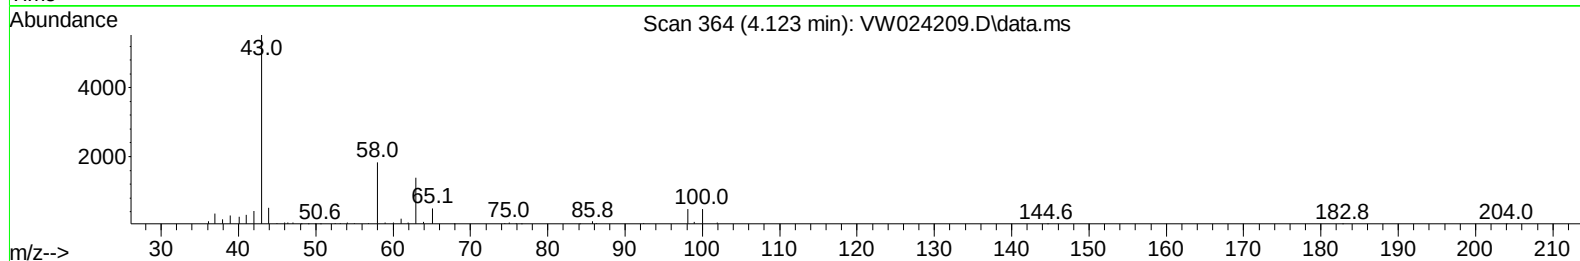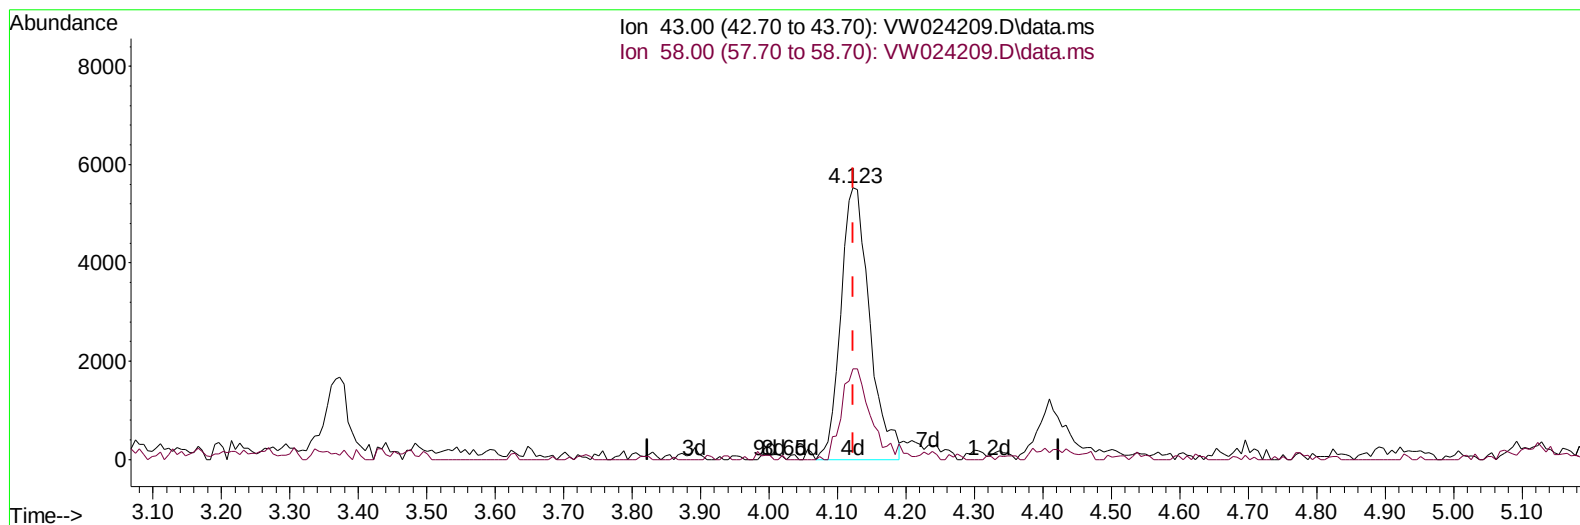

TIC: VW024209.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 15.50 ug/L m

response 16123

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	0.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024209.D
 Acq On : 09 Aug 2022 15:11
 Operator : SY/VA
 Sample : N4110-02
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

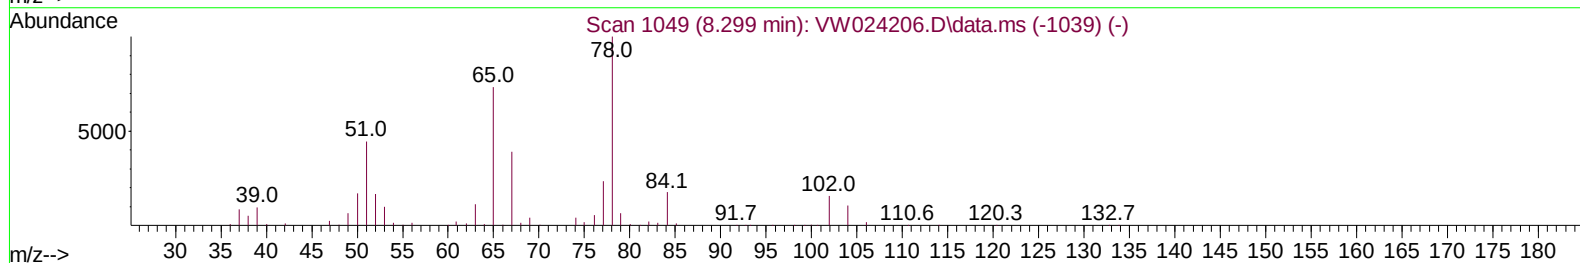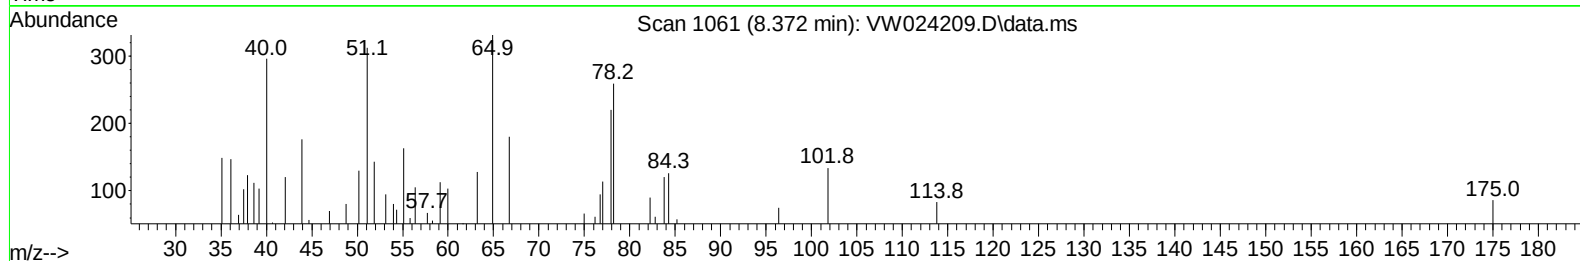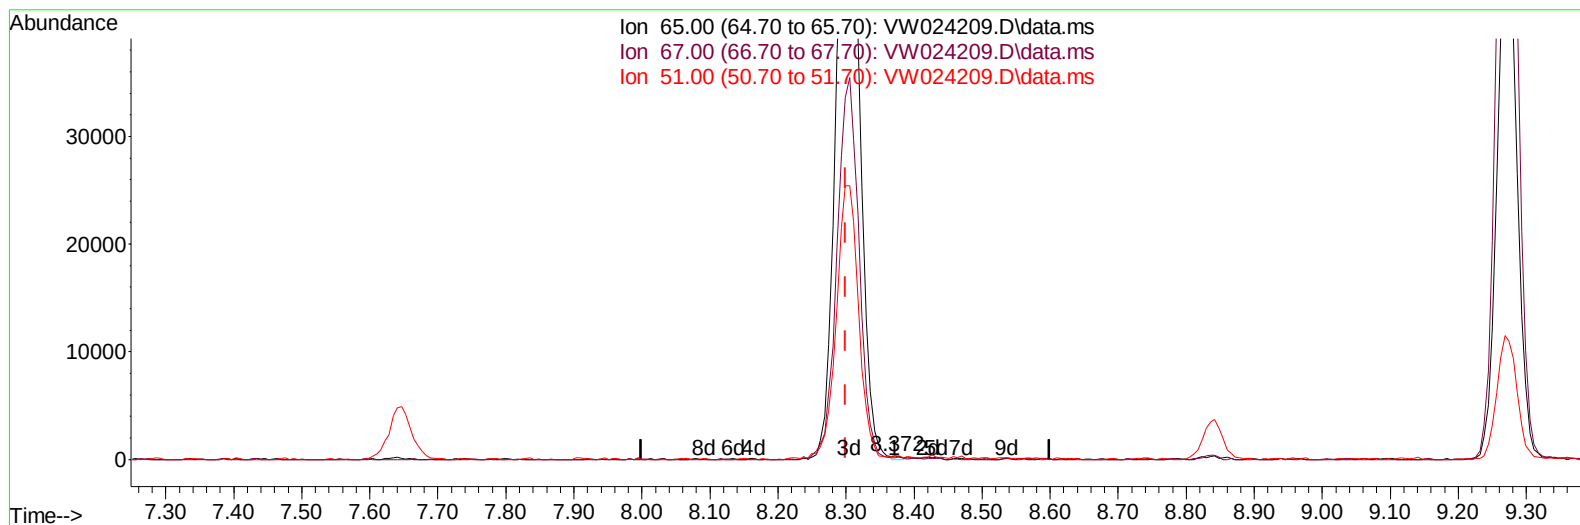

TIC: VW024209.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.372min (+ 0.073) 0.04 ug/L

response 255

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	63.92
51.00	95.20	122.35
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024209.D
 Acq On : 09 Aug 2022 15:11
 Operator : SY/VA
 Sample : N4110-02
 Misc : 5.73g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		363417	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		333270	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		153849	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.337	65		217240	28.598	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	114.400%	
7) Chloroethane-d5	2.873	69		132935	28.092	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	112.360%	
11) 1,1-Dichloroethene-d2	4.007	63		166367	19.217	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	76.880%	
21) 2-Butanone-d5	7.080	46		70145	49.634	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	99.260%	
24) Chloroform-d	7.647	84		271084	24.653	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	8.305	65		154282m	25.272	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	101.080%	
32) Benzene-d6	8.269	84		532529	27.094	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	108.360%	
36) 1,2-Dichloropropane-d6	9.268	67		157893	27.208	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	108.840%	
41) Toluene-d8	10.323	98		498122	27.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	108.440%	
43) trans-1,3-Dichloroprop...	10.573	79		67683	26.628	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	106.520%	
47) 2-Hexanone-d5	10.921	63		55969	52.215	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	104.440%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		138783	24.649	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	98.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152		164694	29.253	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	117.000%	
Target Compounds							
13) Acetone	4.123	43		16123m	15.495	ug/L	
16) Methylene chloride	4.909	84		27520	4.294	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
Data File : VW024209.D
Acq On : 09 Aug 2022 15:11
Operator : SY/VA
Sample : N4110-02
Misc : 5.73g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/11/2022
Supervised By :Mahesh Dadoda 08/11/2022

Quant Time: Aug 10 01:10:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 10 01:09:21 2022
Response via : Initial Calibration

