




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024212.D
 Acq On : 09 Aug 2022 16:26
 Operator : SY/VA
 Sample : N4110-05
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF8

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

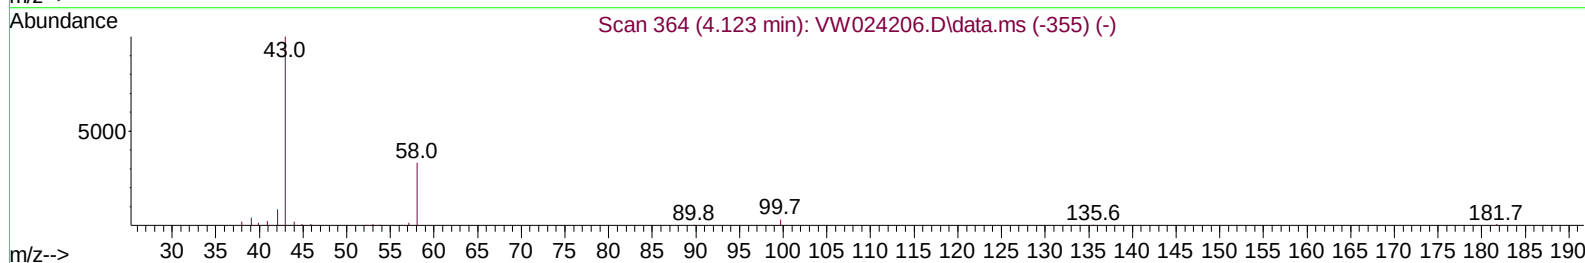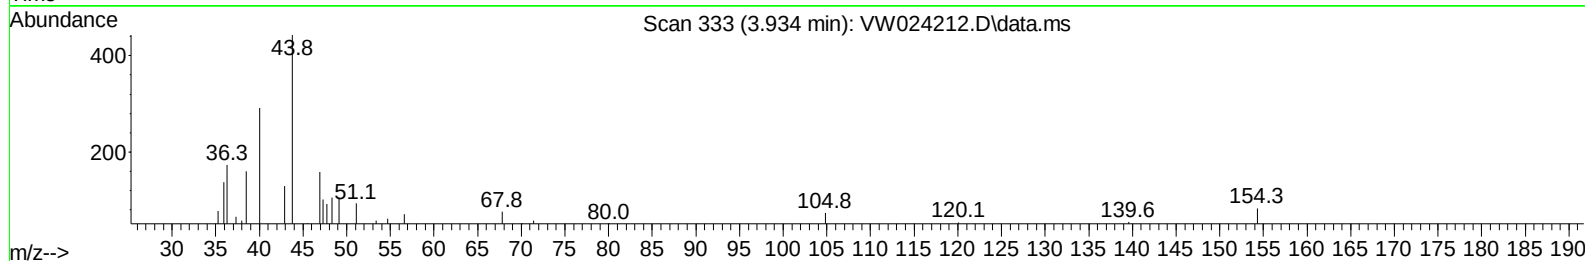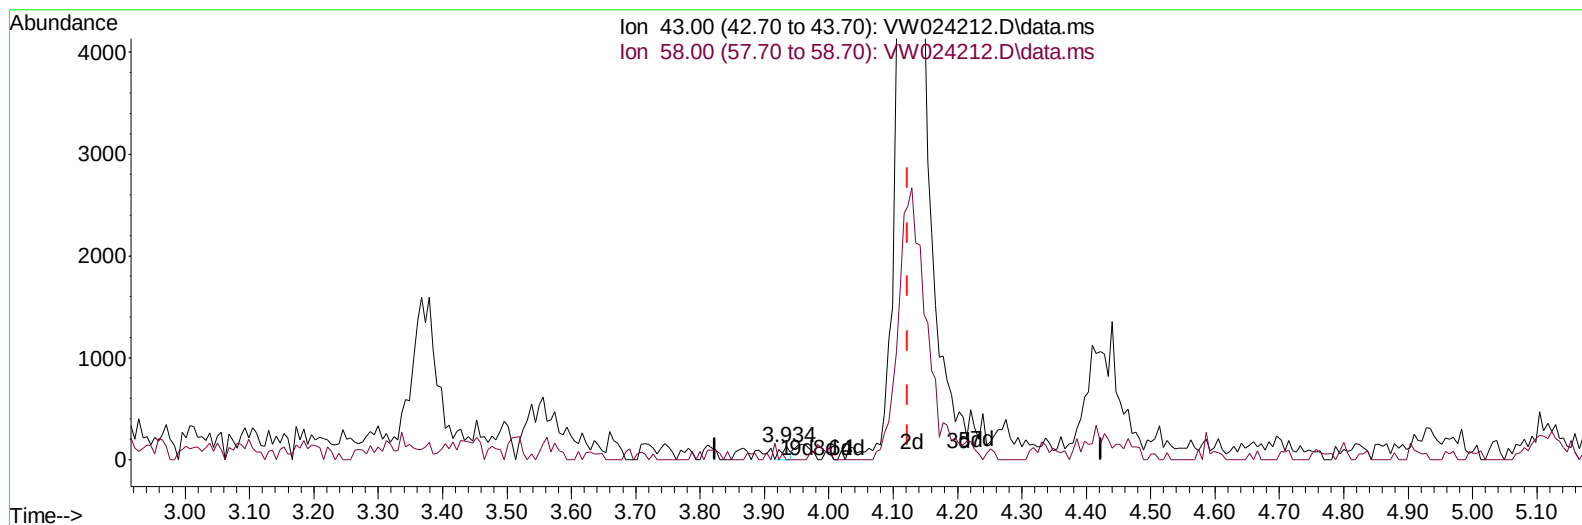

TIC: VW024212.D\data.ms

(13) Acetone (T)

3.934min (-0.189) 0.15 ug/L

response 133

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	14.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024212.D
 Acq On : 09 Aug 2022 16:26
 Operator : SY/VA
 Sample : N4110-05
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF8

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

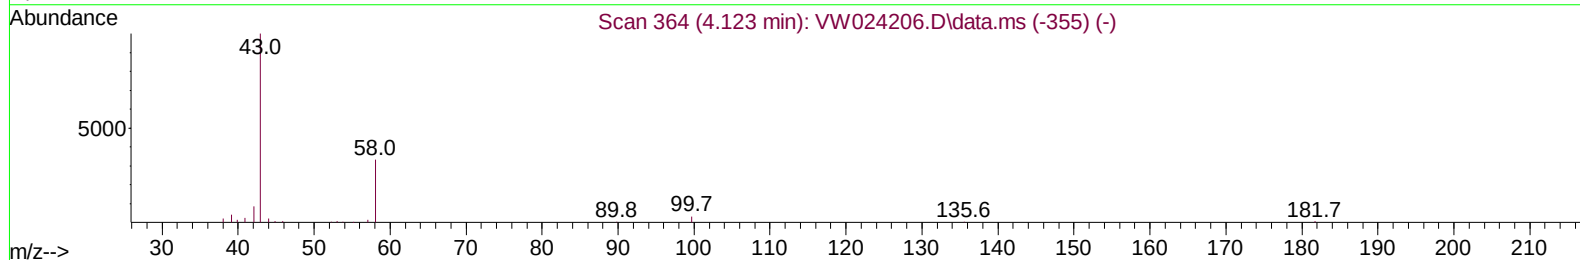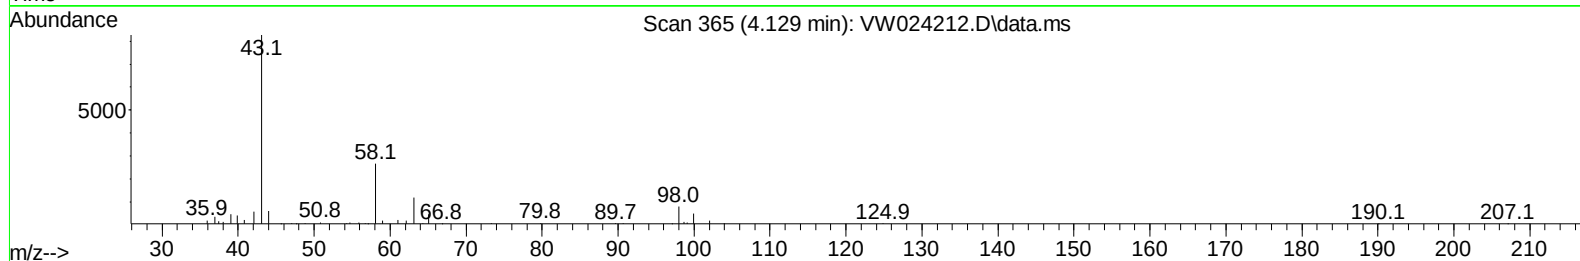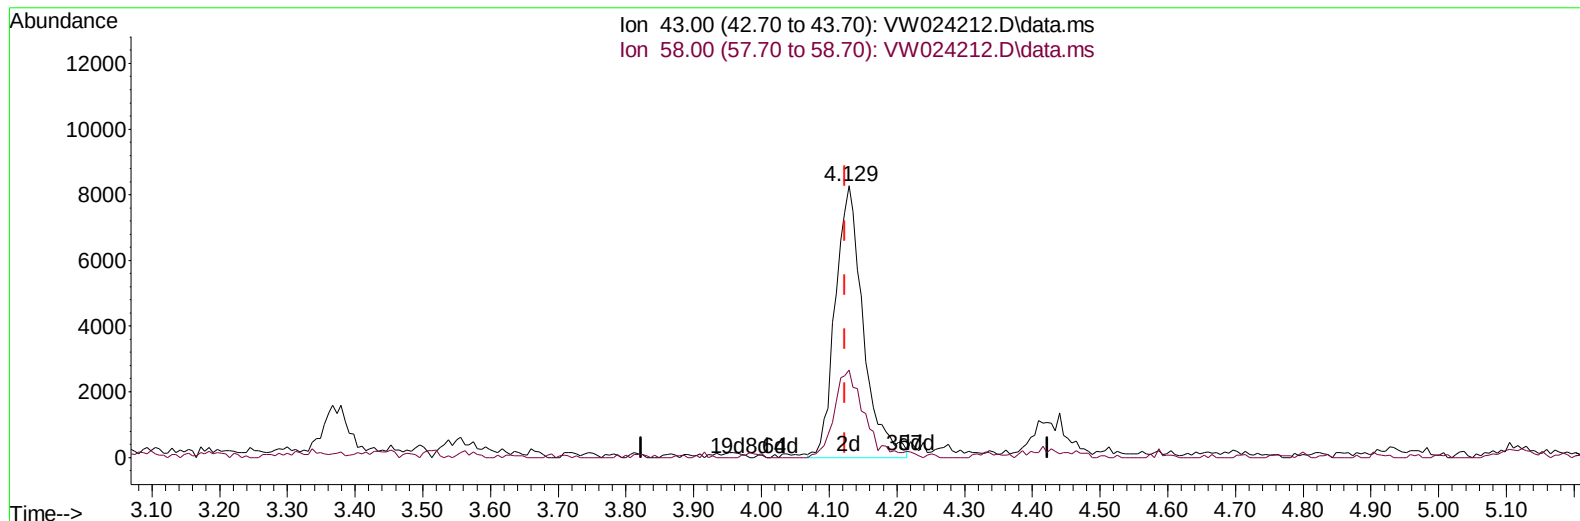

TIC: VW024212.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 26.81 ug/L m

response 23613

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.90	0.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
 Data File : VW024212.D
 Acq On : 09 Aug 2022 16:26
 Operator : SY/VA
 Sample : N4110-05
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZF8

Manual IntegrationsAPPROVED

Quant Time: Aug 10 01:10:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Aug 10 01:09:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/11/2022
 Supervised By :Mahesh Dadoda 08/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	307631	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	291707	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	123850	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	192231	29.895	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	119.560%	
7) Chloroethane-d5	2.873	69	120249	30.020	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	120.080%	
11) 1,1-Dichloroethene-d2	4.001	63	143929	19.640	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	78.560%	
21) 2-Butanone-d5	7.080	46	80452	67.250	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	134.500%	
24) Chloroform-d	7.647	84	238023	25.571	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	102.280%	
26) 1,2-Dichloroethane-d4	8.305	65	141639	27.408	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	109.640%	
32) Benzene-d6	8.275	84	462717	26.896	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	107.600%	
36) 1,2-Dichloropropane-d6	9.275	67	139635	27.490	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.960%	
41) Toluene-d8	10.323	98	417168	25.943	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	103.760%	
43) trans-1,3-Dichloroprop...	10.579	79	58346	26.225	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	104.880%	
47) 2-Hexanone-d5	10.927	63	64771	69.037	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	138.080%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	139840	28.376	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152	125670	27.729	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	110.920%	
Target Compounds						
13) Acetone	4.129	43	23613m	26.809	ug/L	
16) Methylene chloride	4.909	84	21539	3.970	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080922\
Data File : VW024212.D
Acq On : 09 Aug 2022 16:26
Operator : SY/VA
Sample : N4110-05
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZF8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/11/2022
Supervised By :Mahesh Dadoda 08/11/2022

Quant Time: Aug 10 01:10:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM080422SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Aug 10 01:09:21 2022
Response via : Initial Calibration

