


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW081019\
 Data File : VW011779.D
 Acq On : 08 Aug 2019 18:49
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Title : SW846 8260
 Last Update : Sat Jul 27 00:23:30 2019

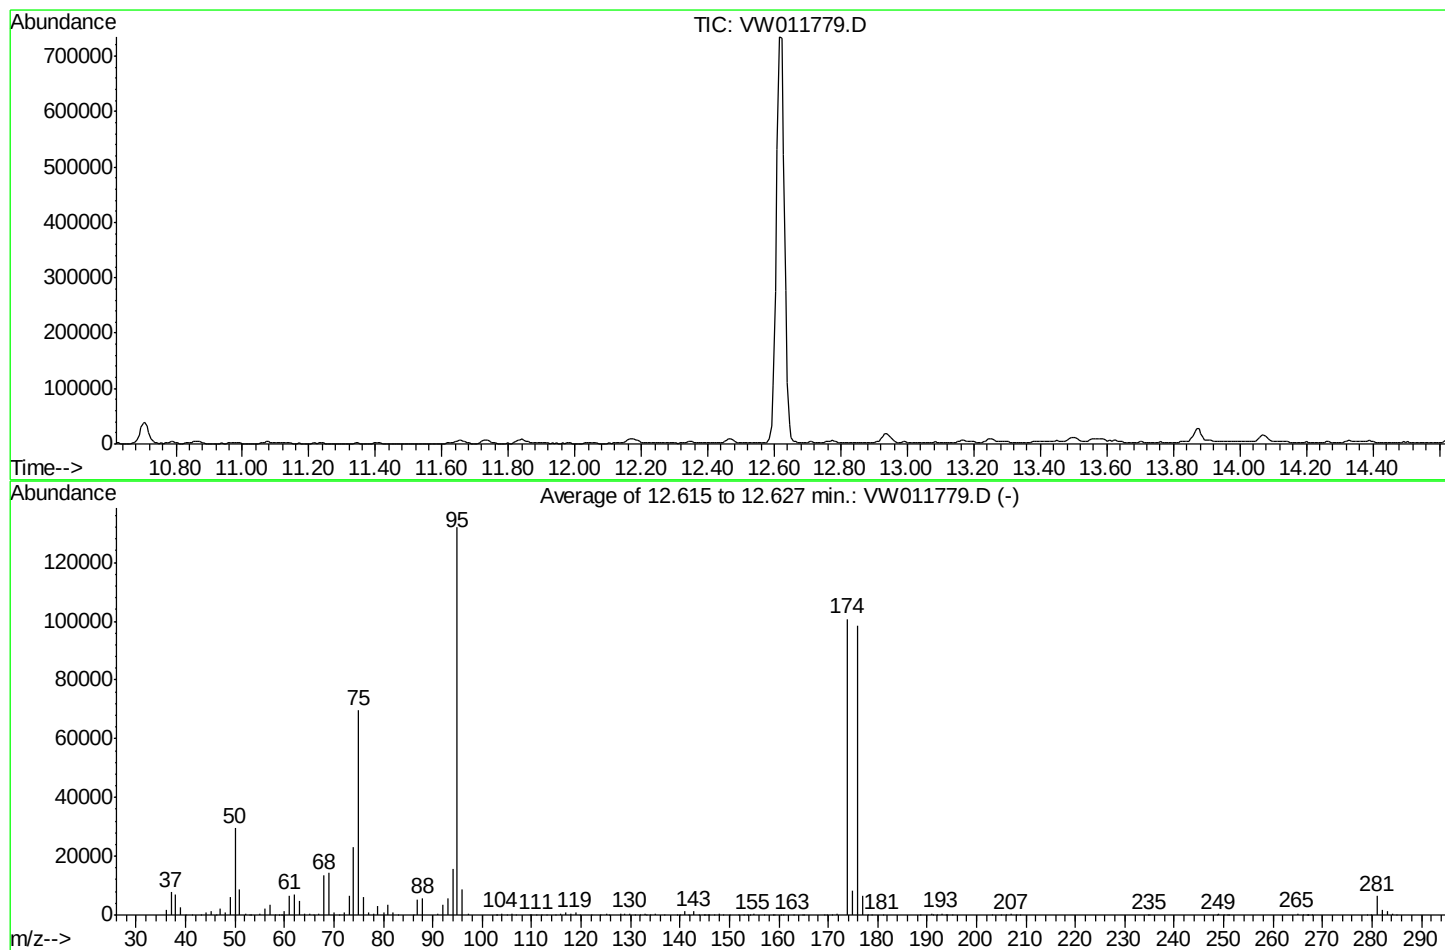

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	29477	PASS
75	95	30	60	52.8	69696	PASS
95	95	100	100	100.0	131962	PASS
96	95	5	9	6.7	8874	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.4	100845	PASS
175	174	5	9	8.1	8191	PASS
176	174	95	101	97.6	98461	PASS
177	176	5	9	6.6	6462	PASS