

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081020\
 Data File : VW016110.D
 Acq On : 10 Aug 2020 19:29
 Operator : SY/VA
 Sample : L3598-13
 Misc : 5.08G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Aug 11 01:59:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 11 01:19:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	327574	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	285958	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	83229	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	92788	22.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.40%
7) Chloroethane-d5	2.89	69	69267	22.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.88%
10) 1,1-Dichloroethene-d2	4.01	63	147692	17.12	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.48%
20) 2-Butanone-d5	7.09	46	91150	85.29	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	170.58%#
24) Chloroform-d	7.65	84	205034	23.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.28%
26) 1,2-Dichloroethane-d4	8.30	65	130651	27.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.92%
29) Benzene-d6	8.27	84	399558	25.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.76%
33) 1,2-Dichloropropane-d6	9.27	67	119319	26.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.32%
37) Toluene-d8	10.32	98	343408	24.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.28%
38) trans-1,3-Dichloropropene-	10.58	79	56062	27.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	109.08%
39) 2-Hexanone-d5	10.93	63	70772	89.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	179.36%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129945	34.89	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	139.56%#
61) 1,2-Dichlorobenzene-d4	13.86	152	80954	27.44	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.76%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Chloromethane	2.18	50	1294	0.394	ug/L	95
13) Acetone	4.13	43	10472	12.953	ug/L	90
16) Methylene chloride	4.92	84	9256	1.789	ug/L	87
30) Cyclohexane	7.93	56	11712	1.882	ug/L #	95
34) Benzene	8.32	78	97811	5.931	ug/L	100
36) Methylcyclohexane	9.34	83	22568	3.090	ug/L	90
42) cis-1,3-Dichloropropene	10.04	75	3810	0.618	ug/L #	73
44) Toluene	10.39	91	97155	5.581	ug/L	99
46) 1,1,2-Trichloroethane	10.76	97	2925	0.918	ug/L #	26
49) 2-Hexanone	10.93	43	10976	6.678	ug/L #	54
53) Ethylbenzene	11.73	91	52691	2.668	ug/L	100
54) m,p-Xylene	11.83	106	6942	0.934	ug/L	88
55) o-xylene	12.16	106	2231	0.319	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081020\
Data File : VW016110.D
Acq On : 10 Aug 2020 19:29
Operator : SY/VA
Sample : L3598-13
Misc : 5.08G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Aug 11 01:59:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 11 01:19:31 2020
Response via : Initial Calibration

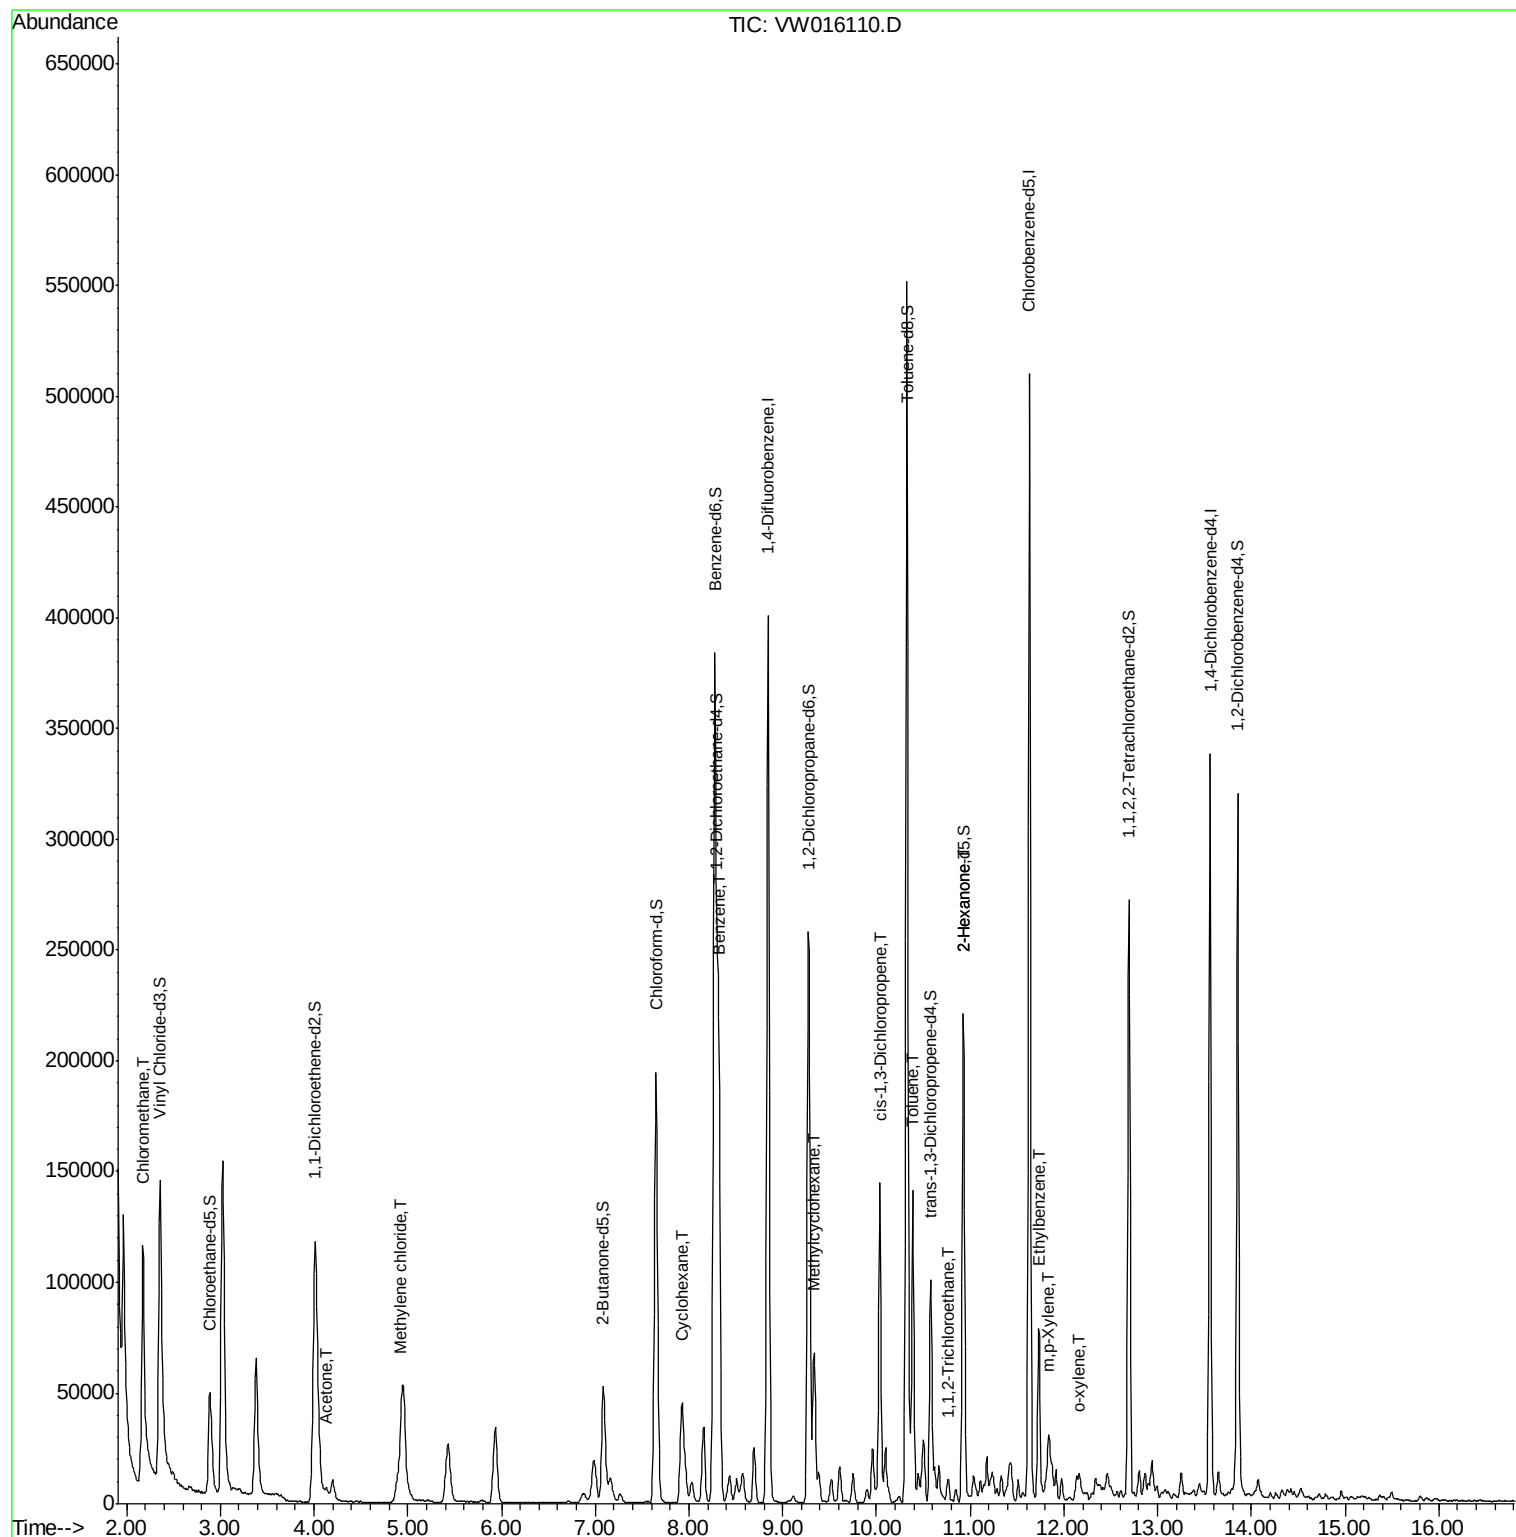



#3

Chloromethane

Concen: 0.394 ug/L

RT: 2.18 min Scan# 45

Delta R.T. -0.04 min

Lab File: VW016110.D

Acq: 10 Aug 2020 19:29

Instrument :

MSVOA_W





ClientSampled :

Tot Ion: 50 Resp: 1294

Ion Ratio Lower Upper

50 100

52 28.5 22.0 40.8

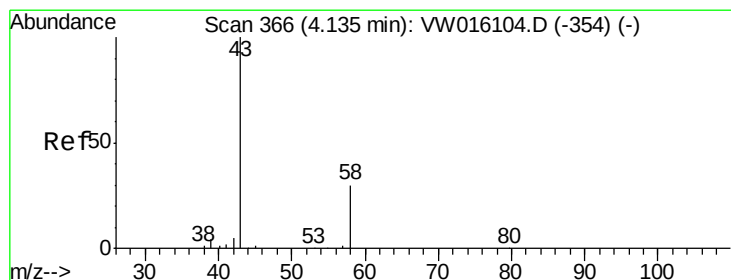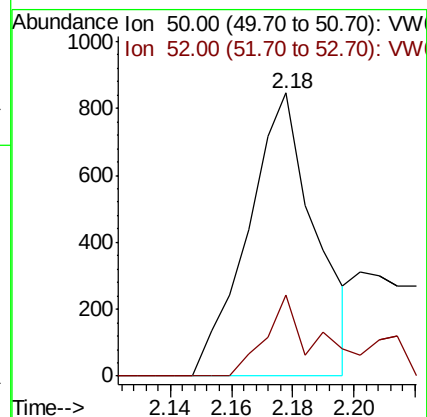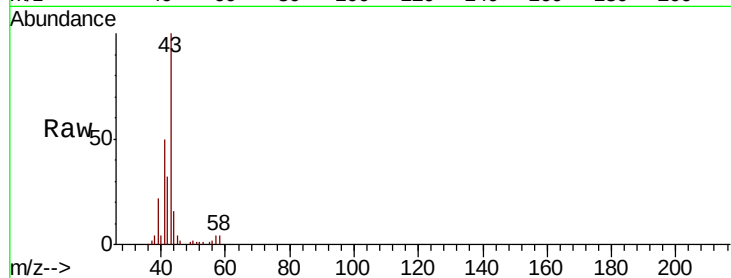

#13

Acetone

Concen: 12.953 ug/L

RT: 4.13 min Scan# 366

Delta R.T. -0.00 min

Lab File: VW016110.D




Acq: 10 Aug 2020 19:29


Tgt Ion: 43 Resp: 10472

Ion Ratio Lower Upper

43 100

58 24.6 0.0 59.4



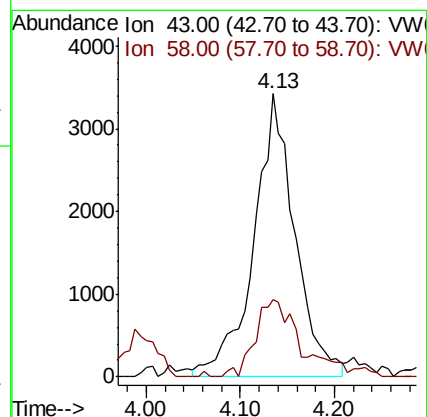
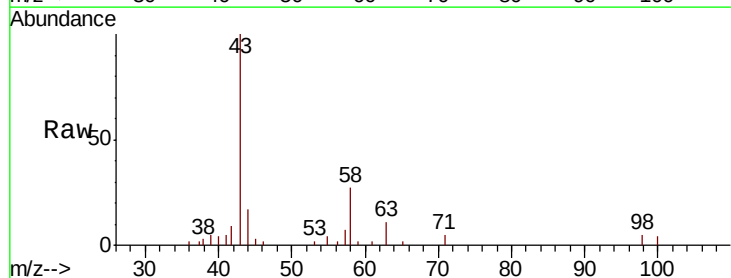


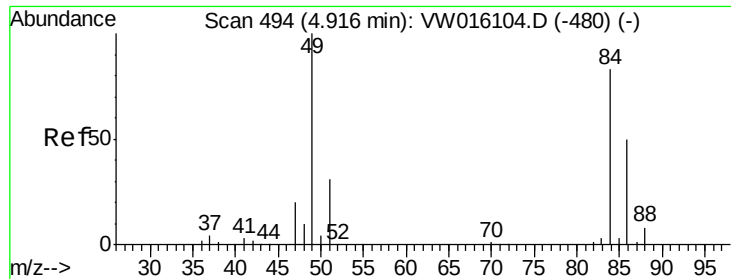

#16
Methylene chloride
Concen: 1.789 ug/L
RT: 4.92 min Scan# 495
Delta R.T. 0.01 min
Lab File: VW016110.D
Acq: 10 Aug 2020 19:29




Instrument :
MSVOA_W
ClientSampled :


Tot Ion: 84 Resp: 9256
Ion Ratio Lower Upper
84 100
49 95.0 80.4 149.4
86 60.2 43.8 81.3

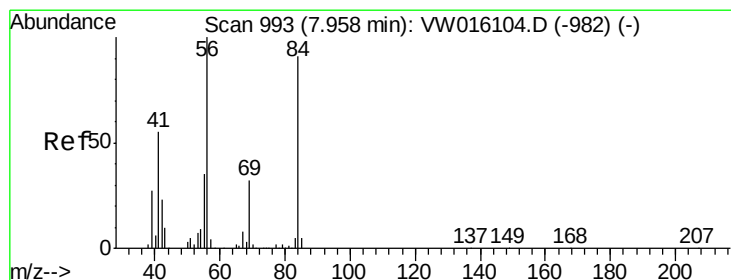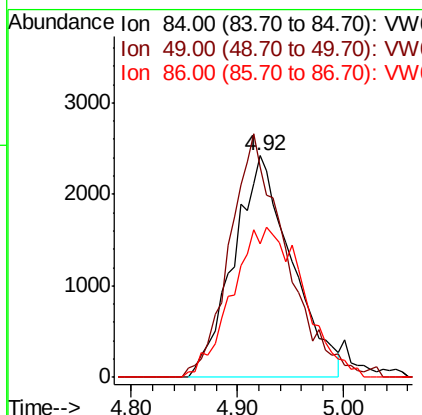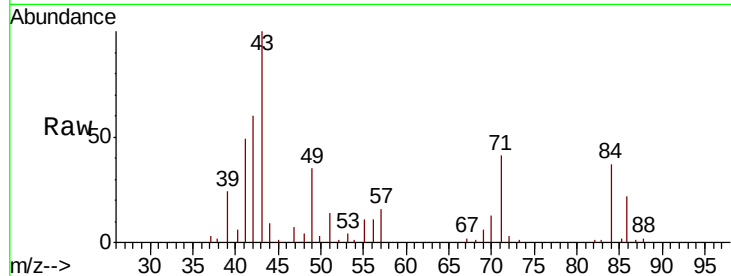

#30
Cyclohexane
Concen: 1.882 ug/L
RT: 7.93 min Scan# 989
Delta R.T. -0.02 min
Lab File: VW016110.D
Acq: 10 Aug 2020 19:29

Tgt Ion: 56 Resp: 11712
Ion Ratio Lower Upper
56 100
69 39.2 25.4 38.0#
84 89.5 73.0 109.6

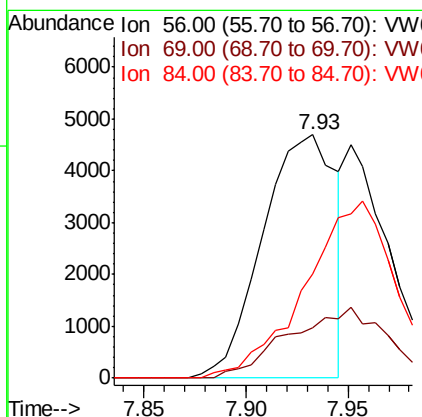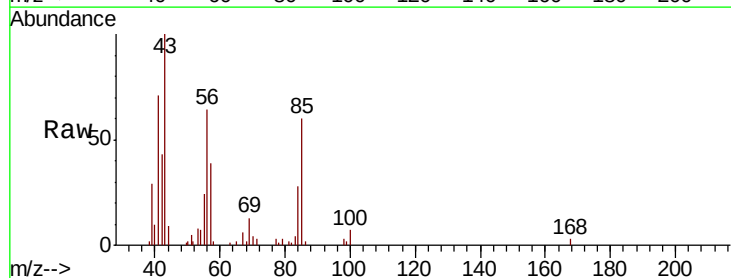

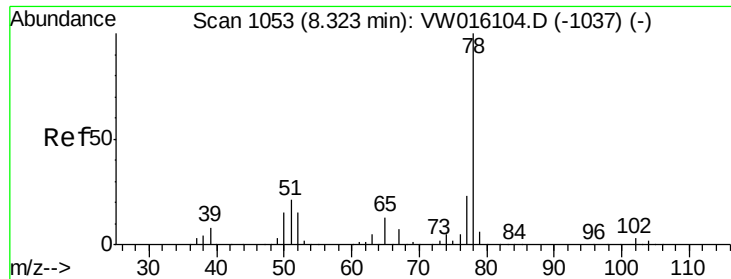

#34

Benzene

Concen: 5.931 ug/L

RT: 8.32 min Scan# 1053


Delta R.T. -0.00 min

Lab File: VW016110.D




Acq: 10 Aug 2020 19:29

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 78 Resp: 97811

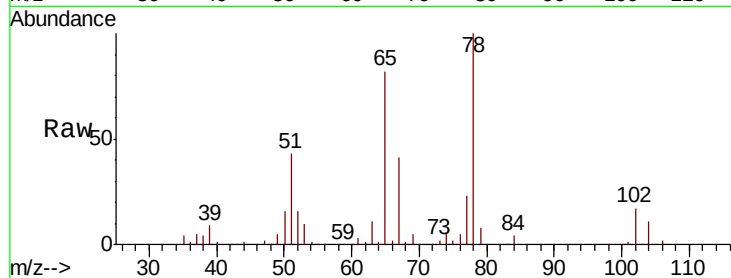

Abundance Ion 78.00 (77.70 to 78.70): VW

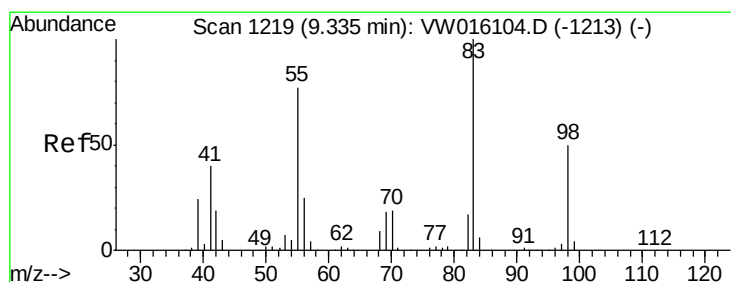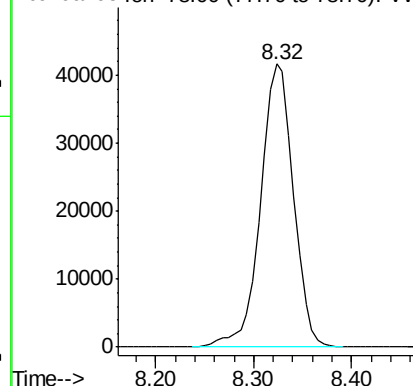

#36

Methylcyclohexane

Concen: 3.090 ug/L

RT: 9.34 min Scan# 1219

Delta R.T. -0.00 min

Lab File: VW016110.D


Acq: 10 Aug 2020 19:29

Tgt Ion: 83 Resp: 22568

Ion	Ratio	Lower	Upper
83	100		

55	89.6	60.7	91.1
----	------	------	------



98	49.2	39.4	59.0
----	------	------	------

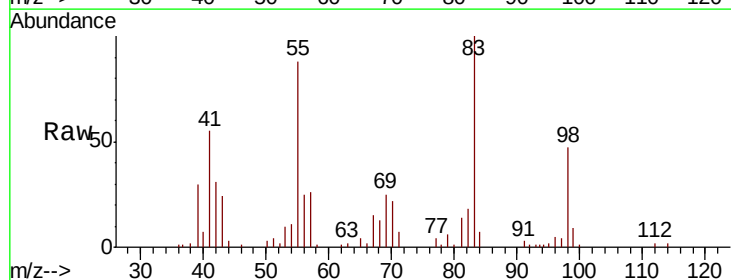


Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 55.00 (54.70 to 55.70): VW

Ion 98.00 (97.70 to 98.70): VW

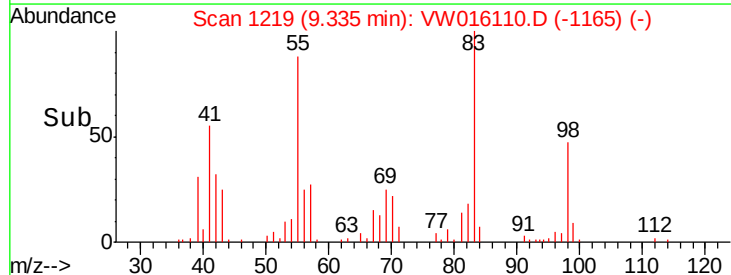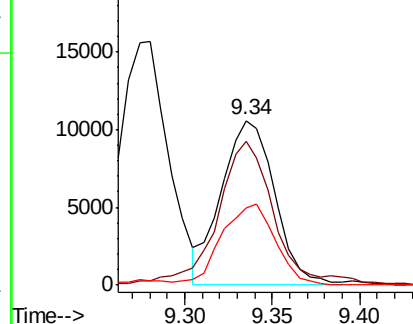

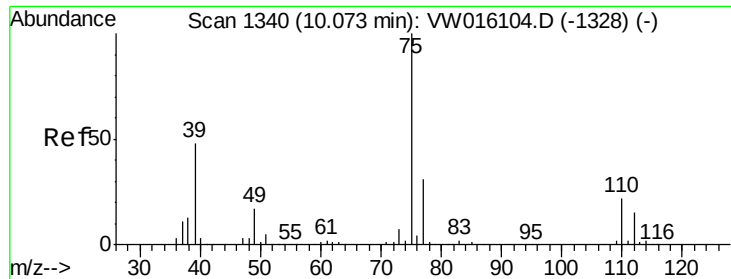

#42

cis-1,3-Dichloropropene

Concen: 0.618 ug/L

RT: 10.04 min Scan# 1334

Delta R.T. -0.04 min

Lab File: VW016110.D

Acq: 10 Aug 2020 19:29

Instrument :

MSVOA_W





ClientSampled :

Tot Ion: 75 Resp: 3810

Ion Ratio Lower Upper

75 100

77 47.7 22.9 42.5#

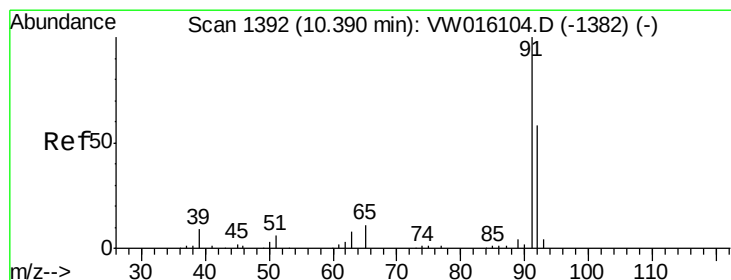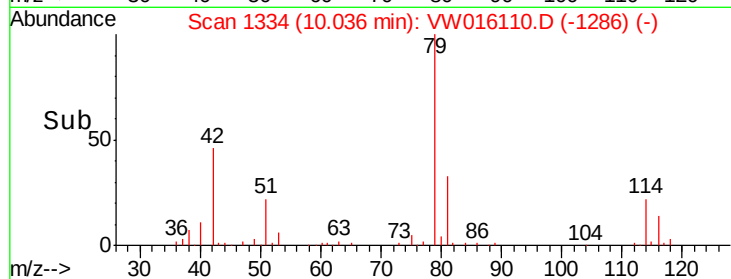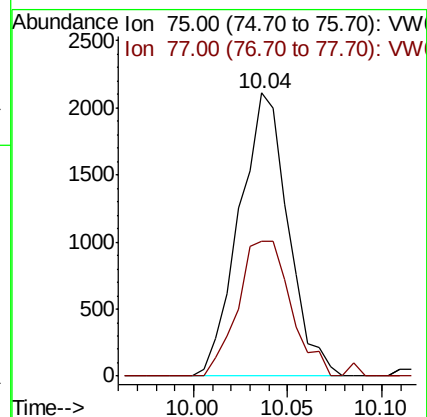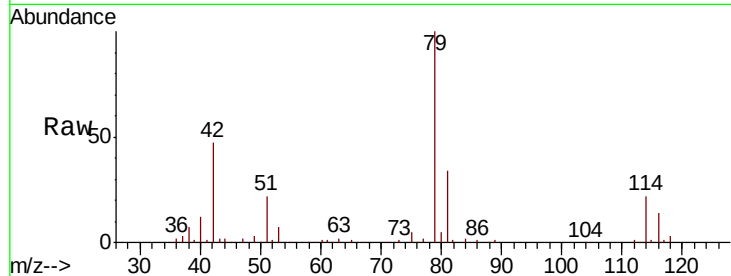

#44

Toluene

Concen: 5.581 ug/L

RT: 10.39 min Scan# 1392

Delta R.T. -0.00 min

Lab File: VW016110.D




Acq: 10 Aug 2020 19:29


Tgt Ion: 91 Resp: 97155

Ion Ratio Lower Upper

91 100

92 58.6 41.8 77.6



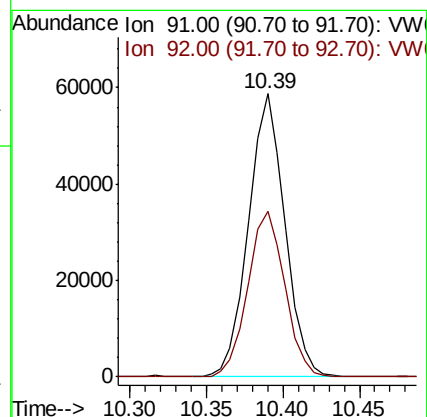
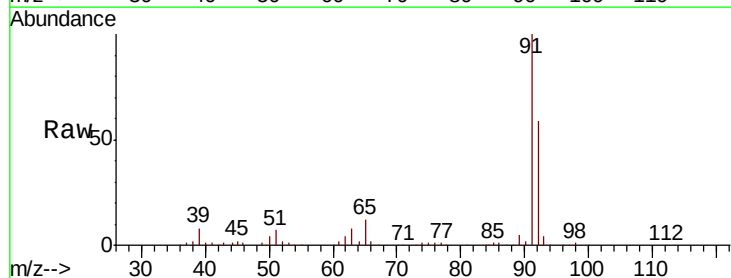




#46
 1,1,2-Trichloroethane
 Concen: 0.918 ug/L
 RT: 10.76 min Scan# 1453
 Delta R.T. -0.02 min
 Lab File: VW016110.D
 Acq: 10 Aug 2020 19:29




Instrument :
 MSVOA_W
 ClientSampleId :


Tot Ion: 97 Resp: 2925
 Ion Ratio Lower Upper
 97 100
 83 12.9 57.8 107.4#
 85 11.5 38.0 70.6#
 99 0.0 44.4 82.4#

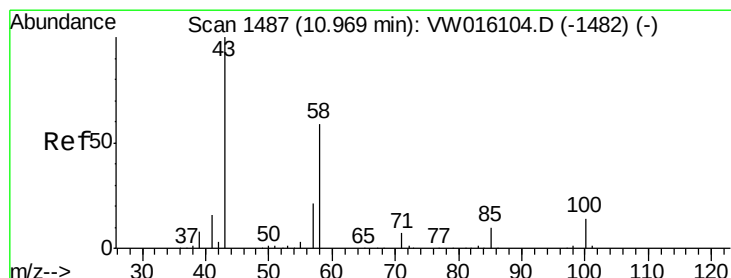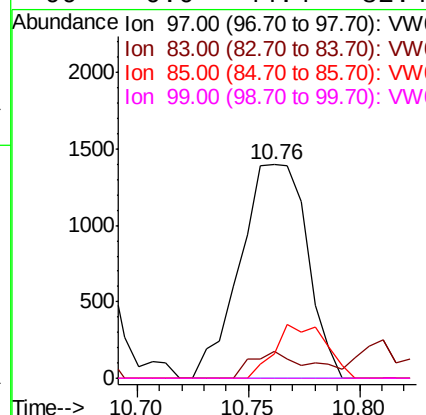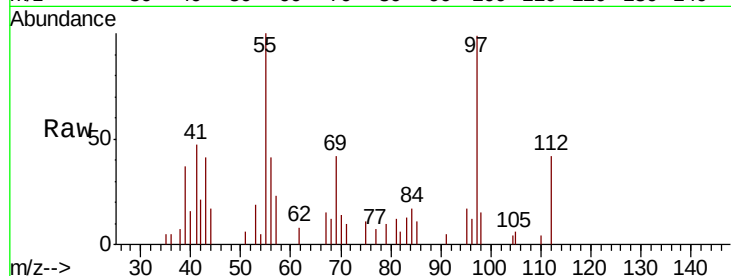

#49
 2-Hexanone
 Concen: 6.678 ug/L
 RT: 10.93 min Scan# 1480
 Delta R.T. -0.04 min
 Lab File: VW016110.D
 Acq: 10 Aug 2020 19:29

Tgt Ion: 43 Resp: 10976
 Ion Ratio Lower Upper
 43 100
 58 22.1 44.2 66.2#
 57 45.6 15.8 23.6#
 100 1.7 10.8 16.2#



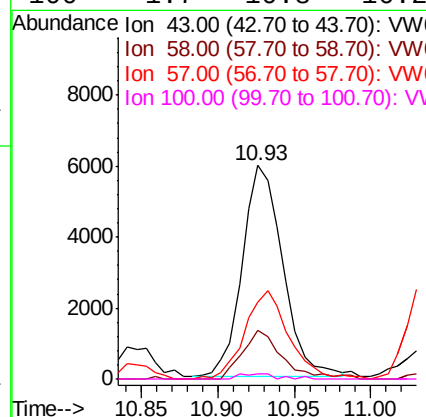
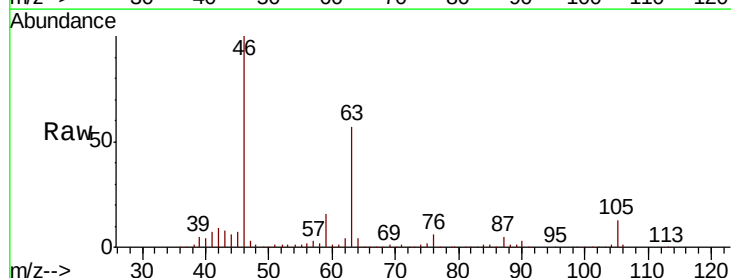


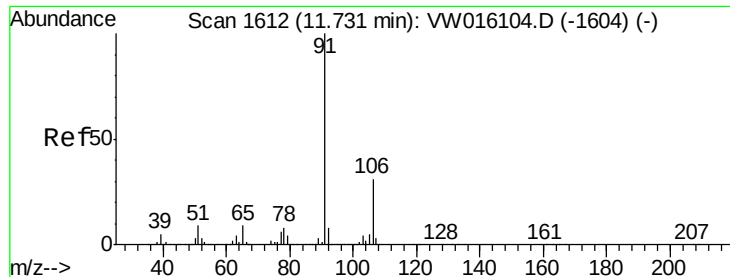

#53
Ethylbenzene
Concen: 2.668 ug/L
RT: 11.73 min Scan# 1612
Delta R.T. -0.00 min
Lab File: VW016110.D
Acq: 10 Aug 2020 19:29




Instrument :
MSVOA_W
ClientSampleId :


Tot Ion: 91 Resp: 52691
Ion Ratio Lower Upper
91 100
106 31.0 21.8 40.4

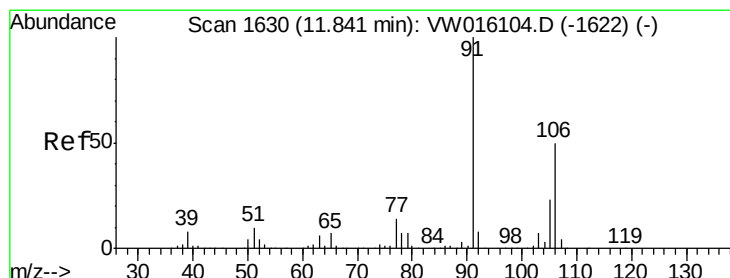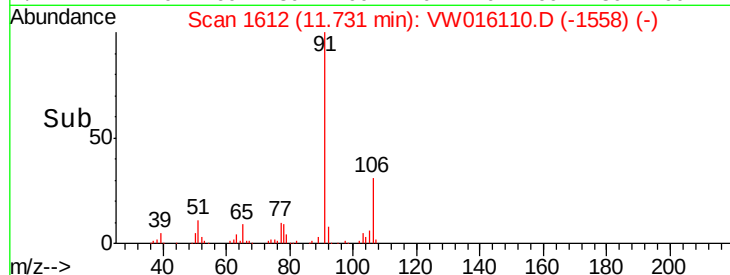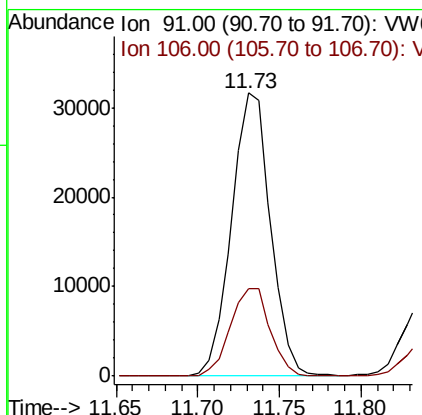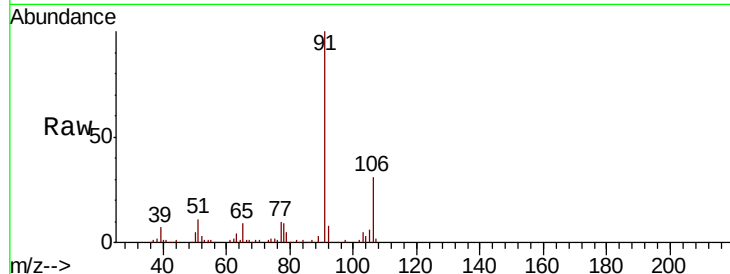

#54
m,p-Xylene
Concen: 0.934 ug/L
RT: 11.83 min Scan# 1629
Delta R.T. -0.01 min
Lab File: VW016110.D
Acq: 10 Aug 2020 19:29

Tgt Ion: 106 Resp: 6942
Ion Ratio Lower Upper
106 100
91 213.2 136.4 253.2

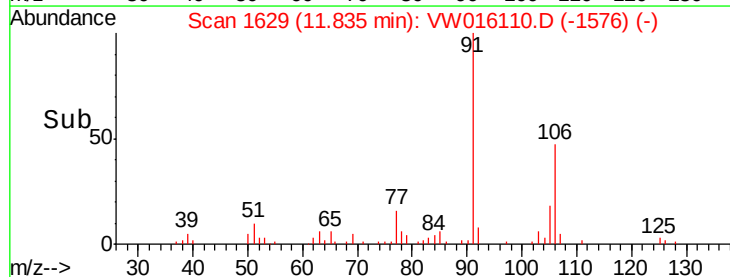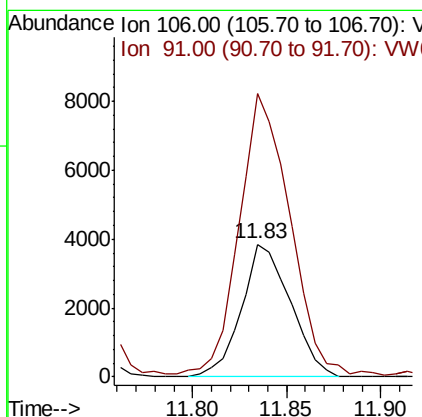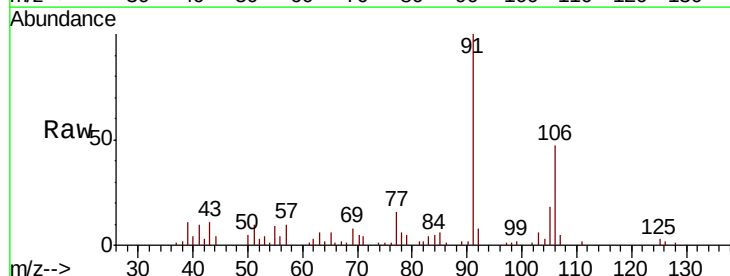

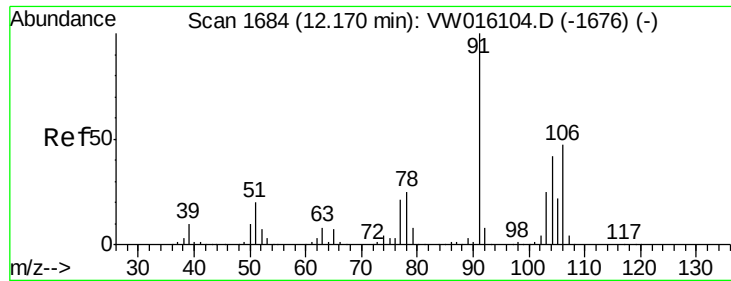

#55
o-xylene
Concen: 0.319 ug/L
RT: 12.16 min Scan# 1683
Delta R.T. -0.01 min
Lab File: VW016110.D
Acq: 10 Aug 2020 19:29

Instrument :
MSVOA_W
ClientSampleId :

Tot Ion:106 Resp: 2231
Ion Ratio Lower Upper
106 100
91 208.8 151.3 281.1

