


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW081420\
 Data File : VW016181.D
 Acq On : 14 Aug 2020 08:25
 Operator : SY/VA
 Sample : BFB10
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0814SBS01

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
 Title : SW846 8260
 Last Update : Fri Aug 14 11:36:08 2020

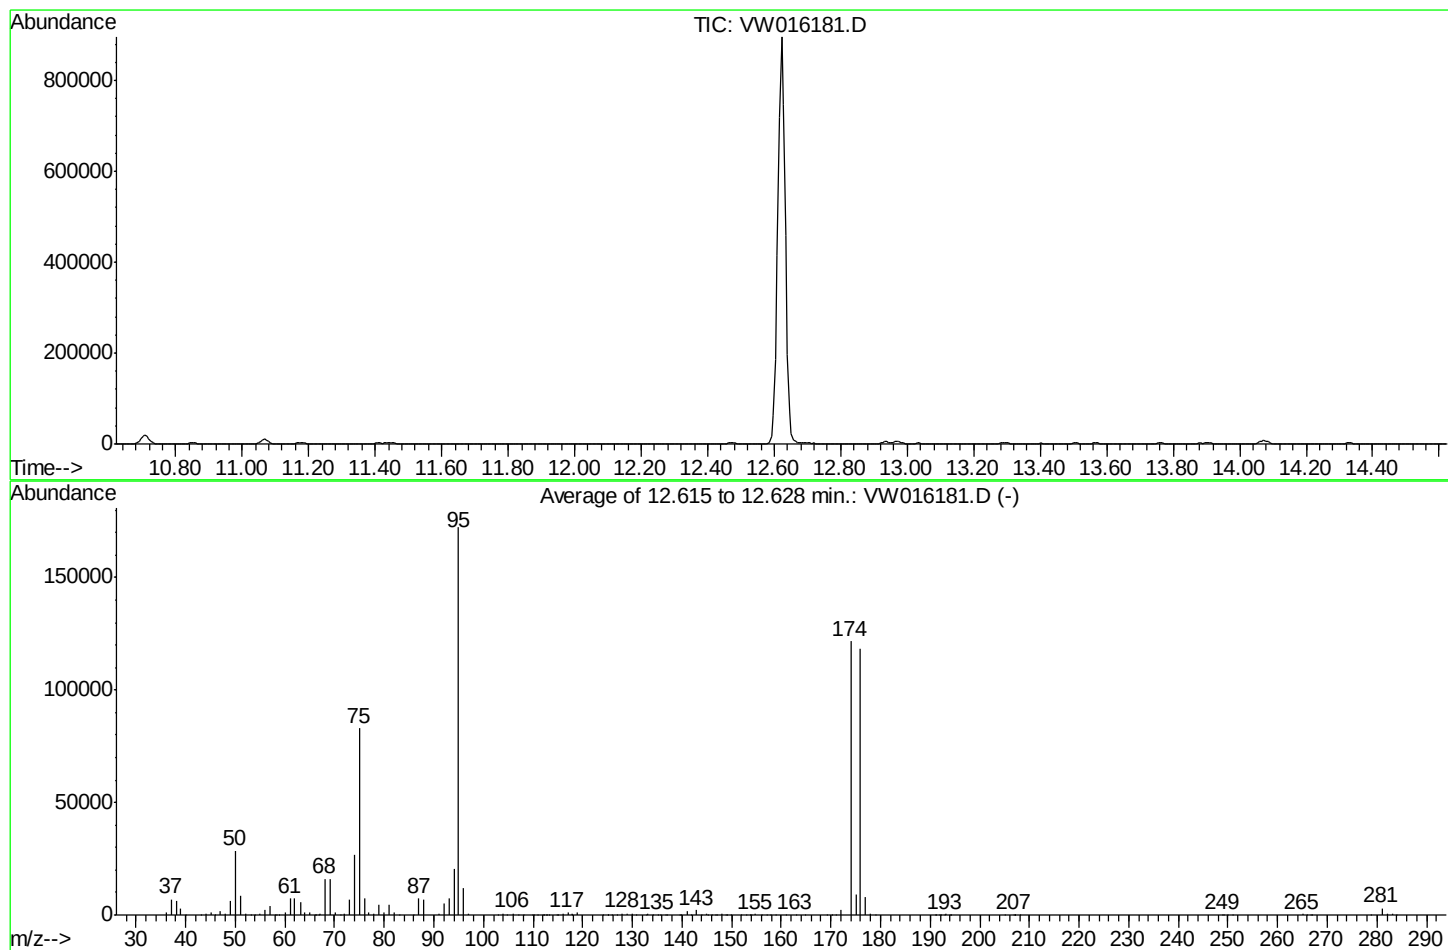

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	28712	PASS
75	95	30	60	48.1	82992	PASS
95	95	100	100	100.0	172373	PASS
96	95	5	9	6.9	11900	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.6	121669	PASS
175	174	5	9	7.5	9163	PASS
176	174	95	101	97.5	118573	PASS
177	176	5	9	6.5	7729	PASS