


Naphthalene

Response Ratio

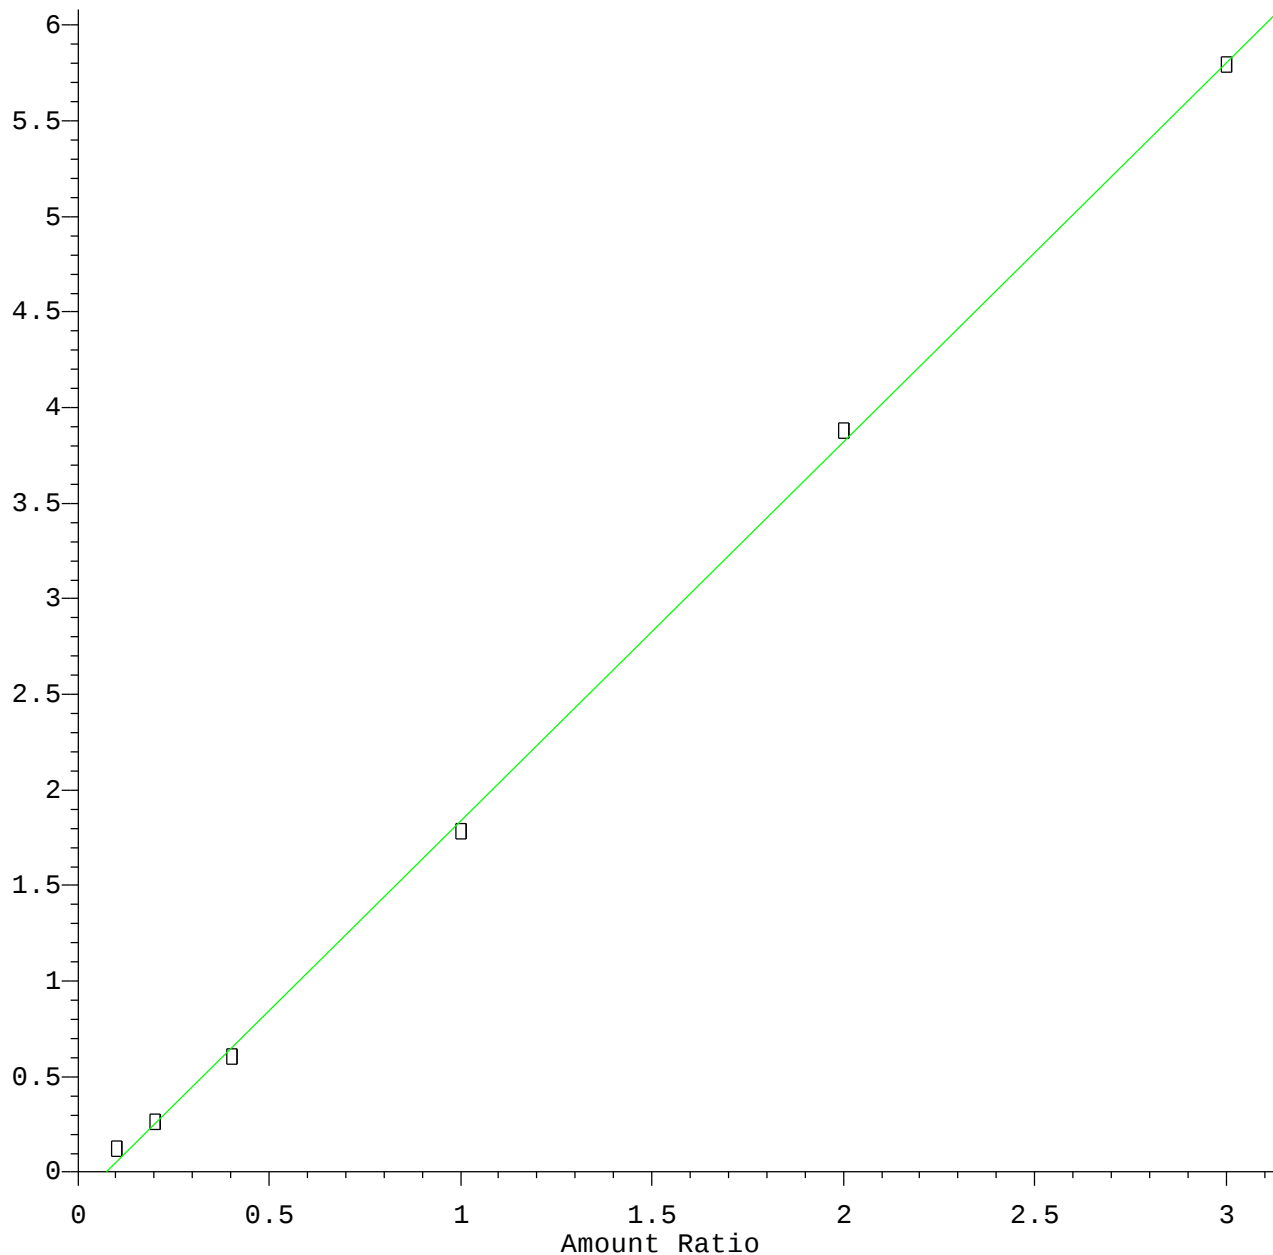


Resp Ratio = 1.98e+000 * Amt - 1.42e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
Calibration Table Last Updated: Mon Aug 17 08:01:41 2020

Methylene Chloride

Response Ratio

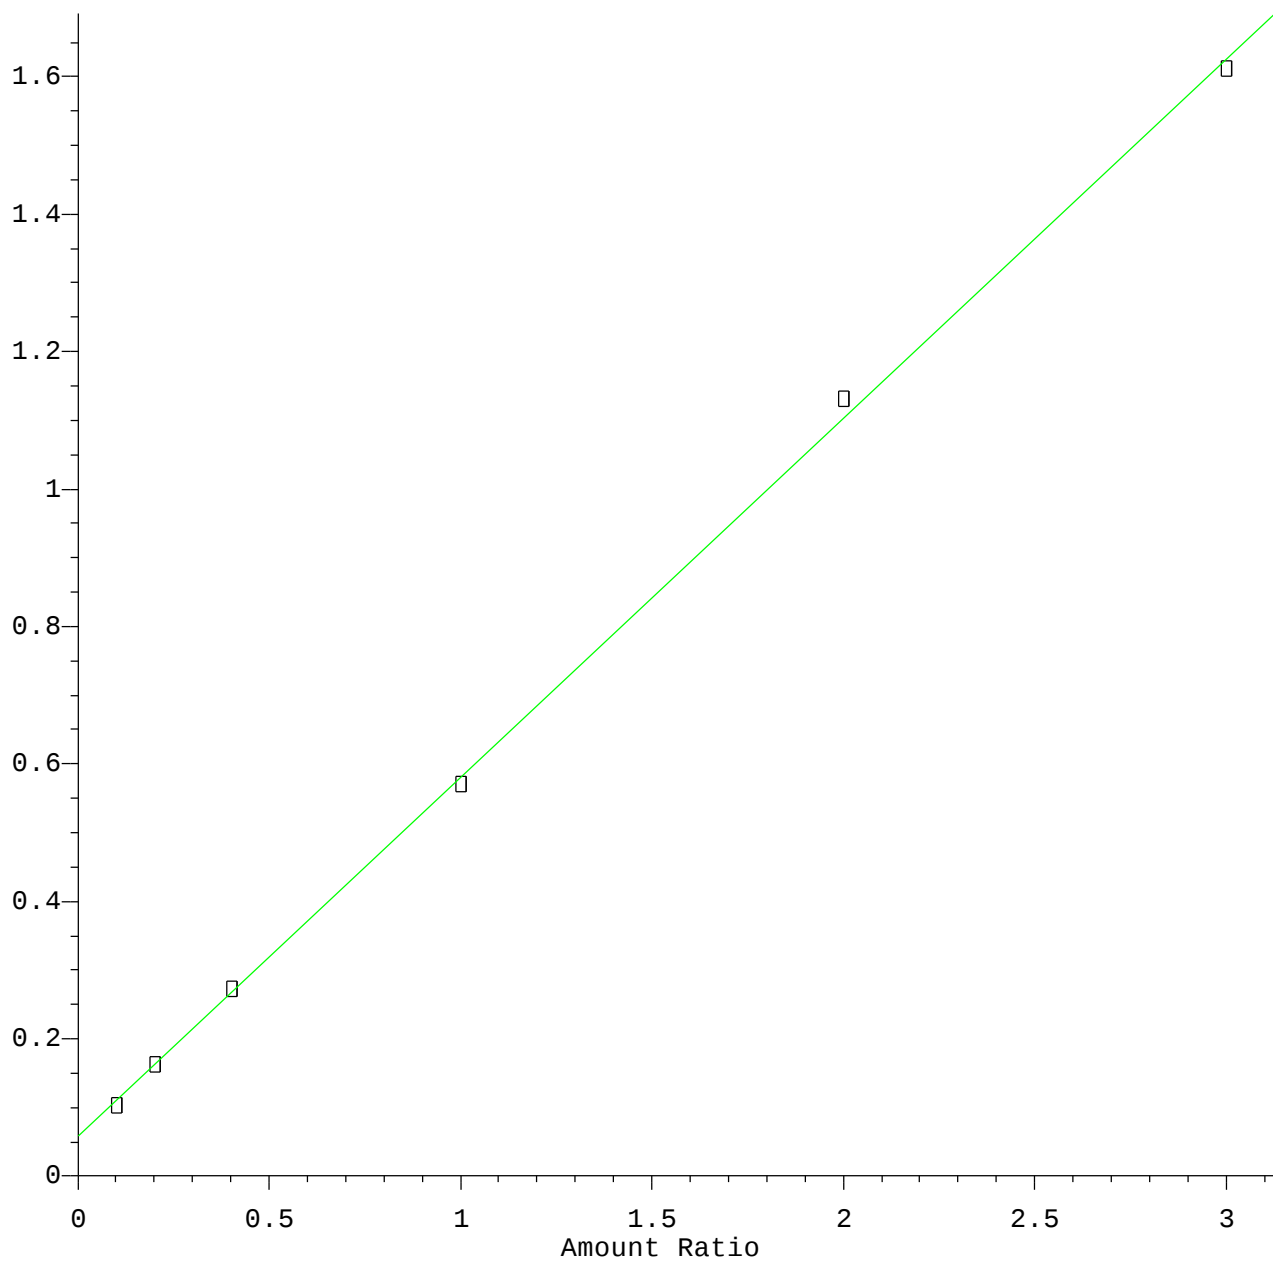

Resp Ratio = $5.23 \times 10^{-1} \times \text{Amt} + 5.73 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
Calibration Table Last Updated: Mon Aug 17 08:01:41 2020