

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081820\
 Data File : VW016230.D
 Acq On : 18 Aug 2020 10:23
 Operator : SY/VA
 Sample : VW0818SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK04

Quant Time: Aug 19 05:50:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 19 05:49:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	386674	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	364174	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	157661	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90544	18.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.56%
7) Chloroethane-d5	2.89	69	74857	20.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.28%
10) 1,1-Dichloroethene-d2	4.01	63	160042	15.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.88%
20) 2-Butanone-d5	7.08	46	45417	36.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.00%
24) Chloroform-d	7.65	84	219265	21.13	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.52%
26) 1,2-Dichloroethane-d4	8.31	65	109736	19.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.64%
29) Benzene-d6	8.28	84	446504	22.54	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.16%
33) 1,2-Dichloropropane-d6	9.28	67	126830	21.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.08%
37) Toluene-d8	10.33	98	404220	22.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.00%
38) trans-1,3-Dichloropropene-	10.58	79	50622	19.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.32%
39) 2-Hexanone-d5	10.93	63	36966	36.78	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.56%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	98179	20.70	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.80%
61) 1,2-Dichlorobenzene-d4	13.85	152	136525	24.43	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.72%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	17685	4.928 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW081820\
Data File : VW016230.D
Acq On : 18 Aug 2020 10:23
Operator : SY/VA
Sample : VW0818SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK04

Quant Time: Aug 19 05:50:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 19 05:49:31 2020
Response via : Initial Calibration

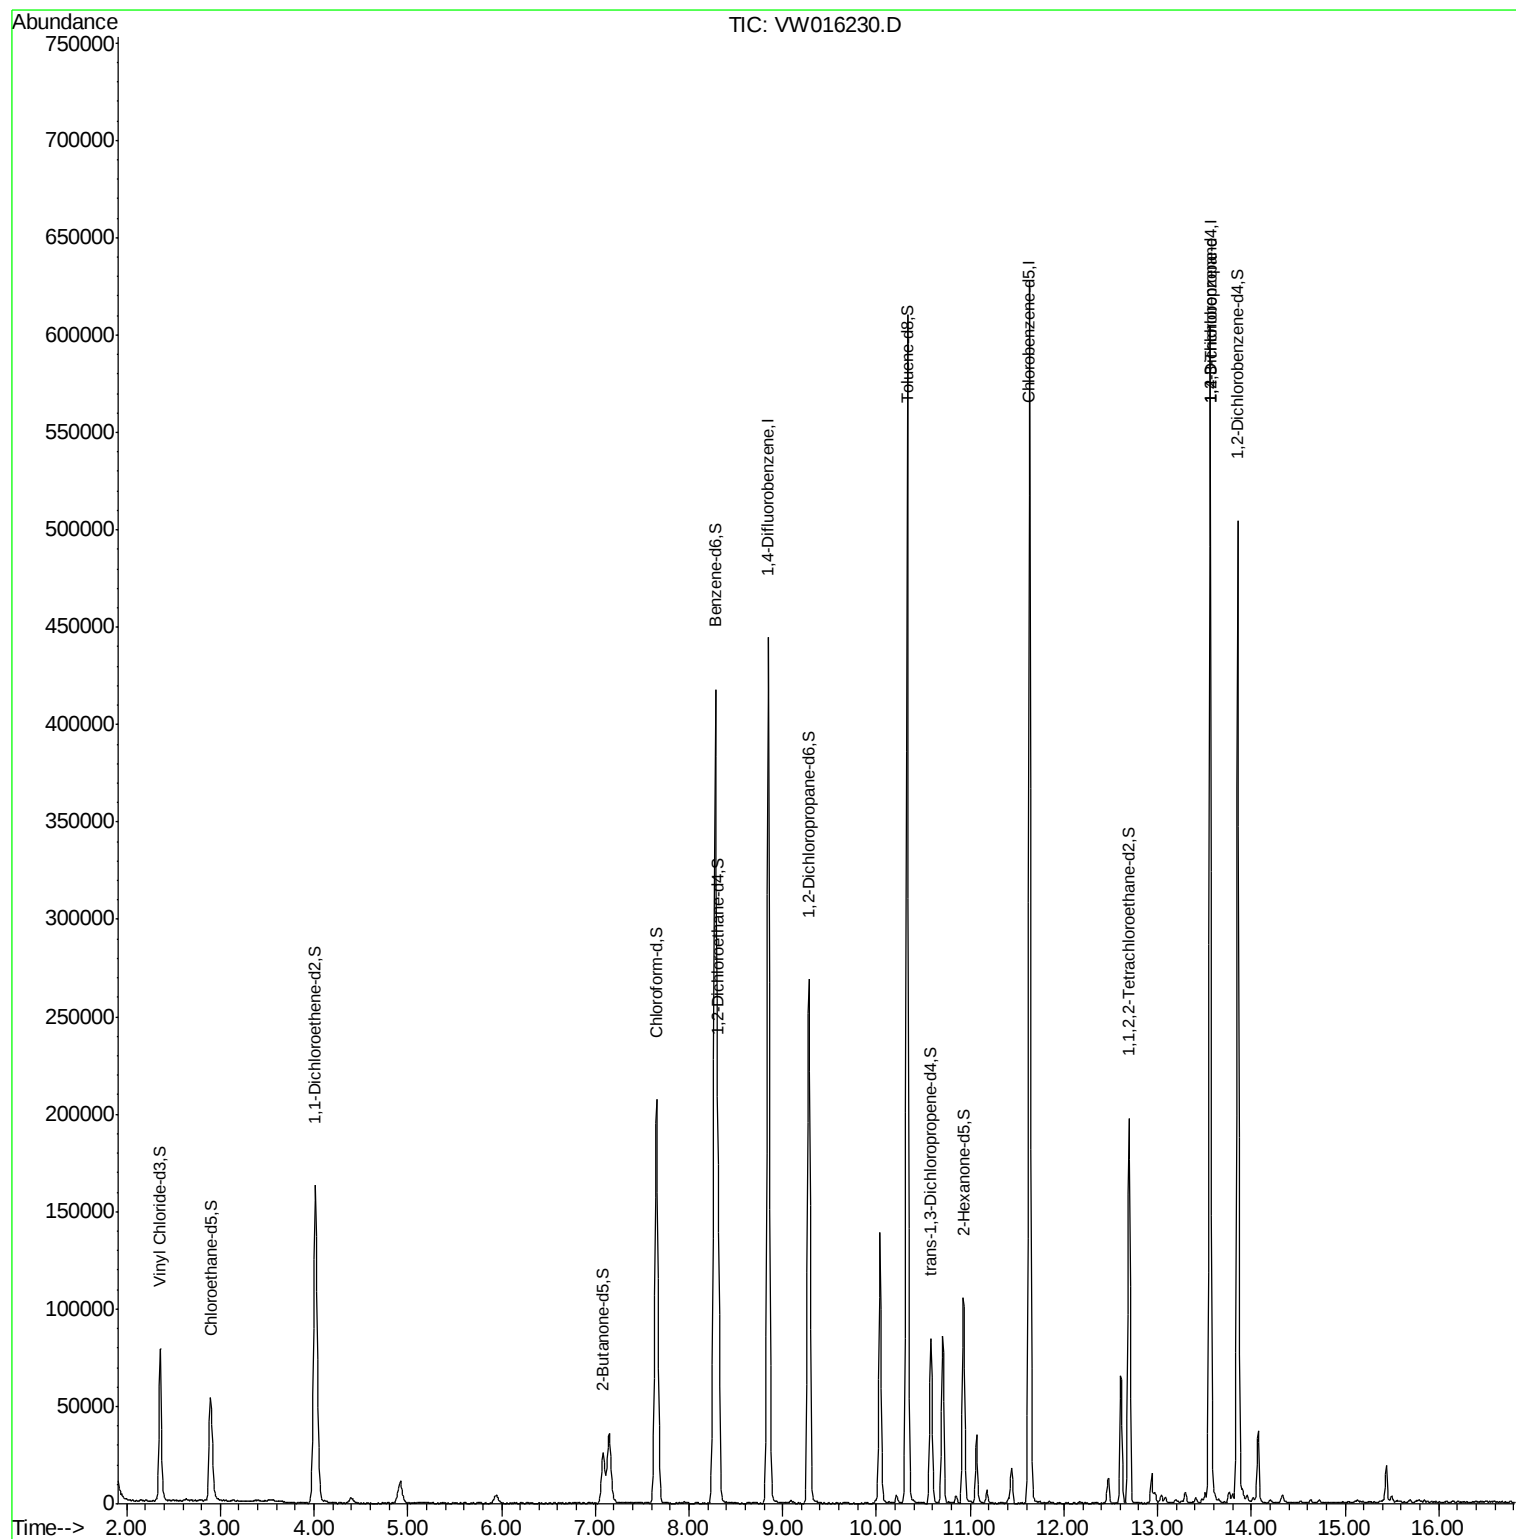

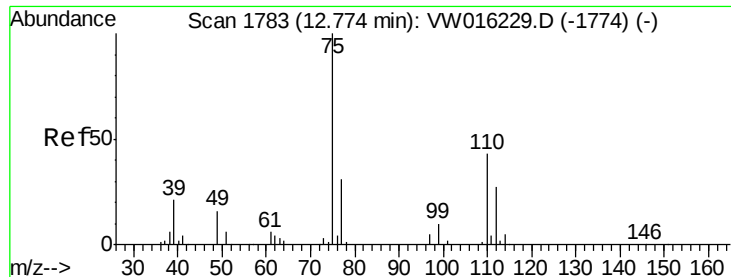

#59

1,2,3-Trichloropropane

Concen: 4.928 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW016230.D

Acq: 18 Aug 2020 10:23

Instrument :

MSVOA_W

ClientSampleId :

VBLK04

Tot Ion: 75 Resp: 17685

Ion Ratio Lower Upper

75 100

77 38.7 25.9 38.9

