

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081820\

Data File : VW016232.D

Acq On : 18 Aug 2020 11:29

Operator : SY/VA

Sample : L3709-02

Misc : 6.13G/10ML/MSVOA W/SOIL

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 19 06:17:53 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M

Quant Title : VOC Analysis

QLast Update : Wed Aug 19 05:49:31 2020

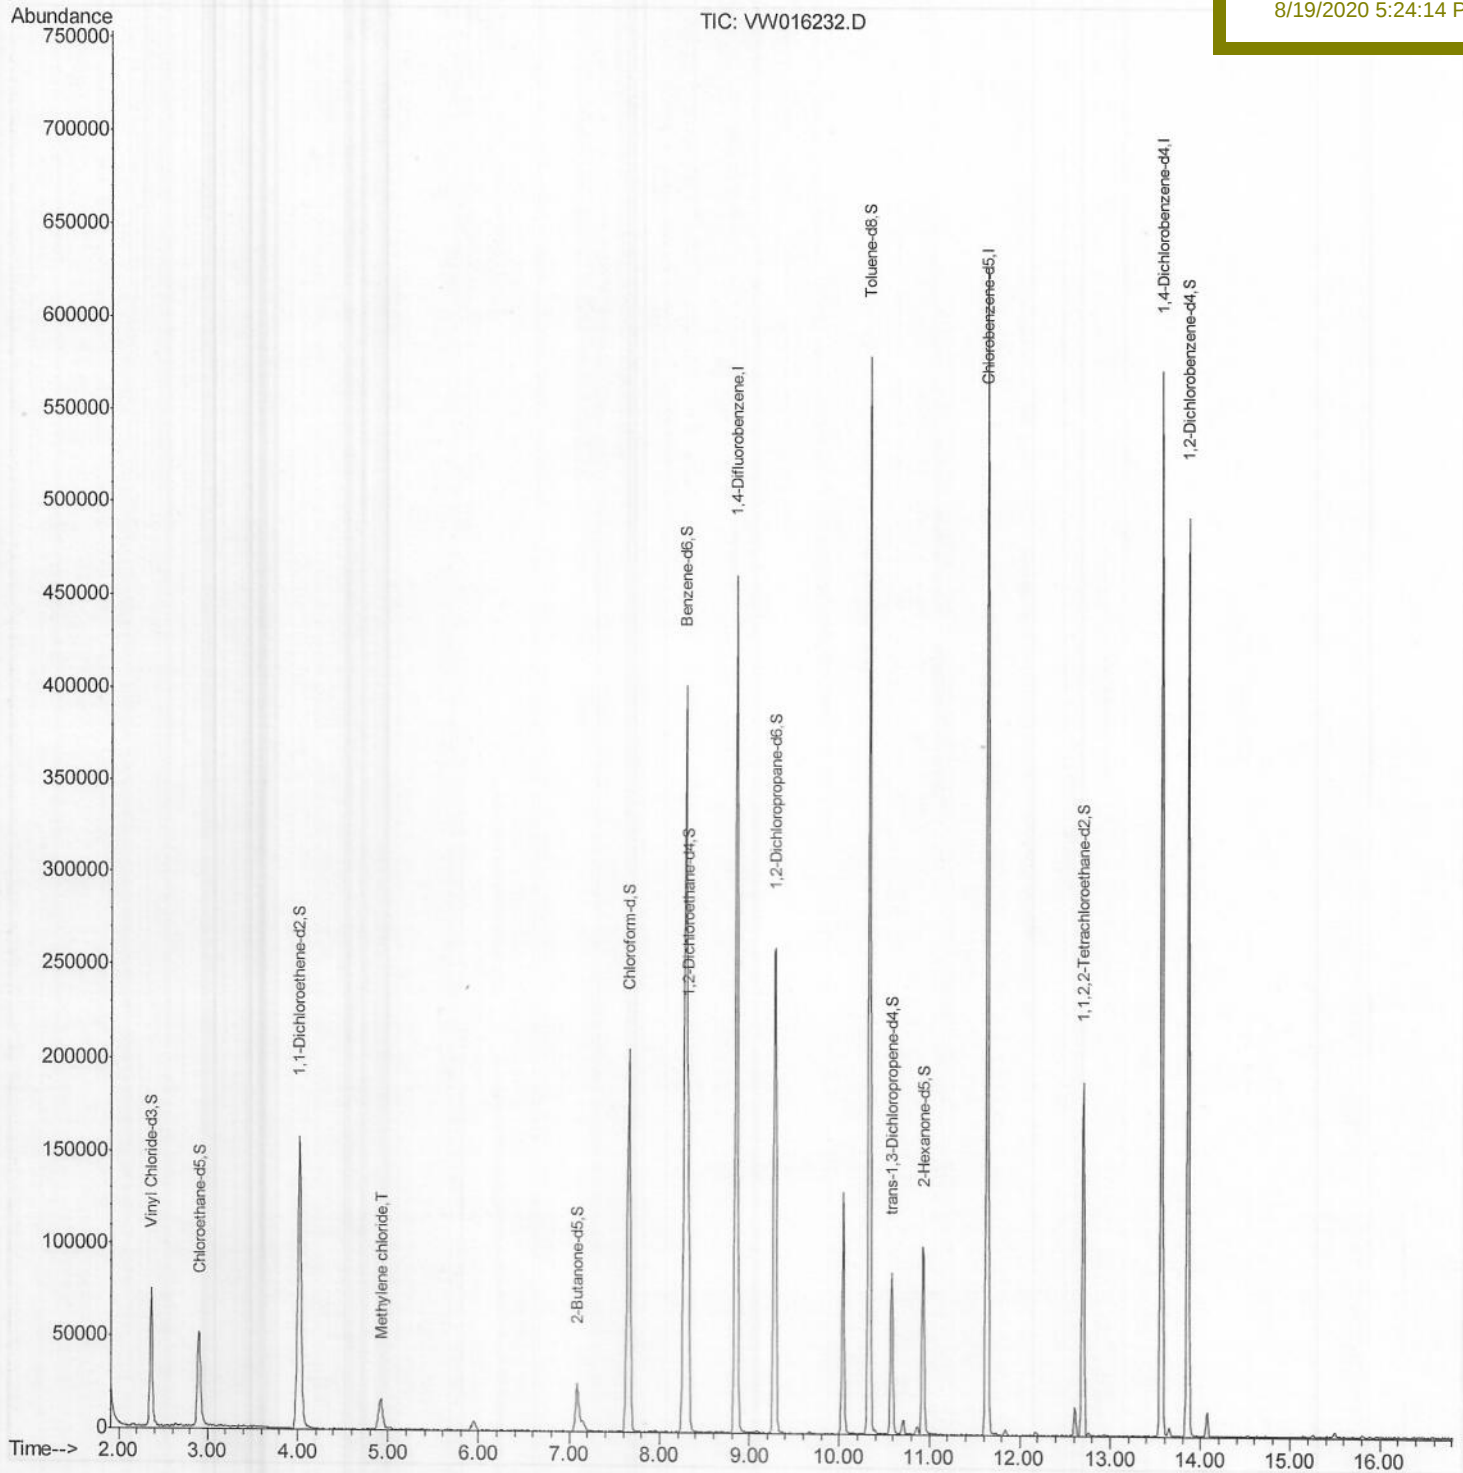
Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :

BFSQ5

Manual Integrations
APPROVEDMMDadoda
8/19/2020 5:24:14 PM

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081820\

Data File : VW016232.D

Acq On : 18 Aug 2020 11:29

Operator : SY/VA

Sample : L3709-02

Misc : 6.13G/10ML/MSVOA W/SOIL

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 19 05:51:08 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M

Quant Title : VOC Analysis

QLast Update : Wed Aug 19 05:49:31 2020

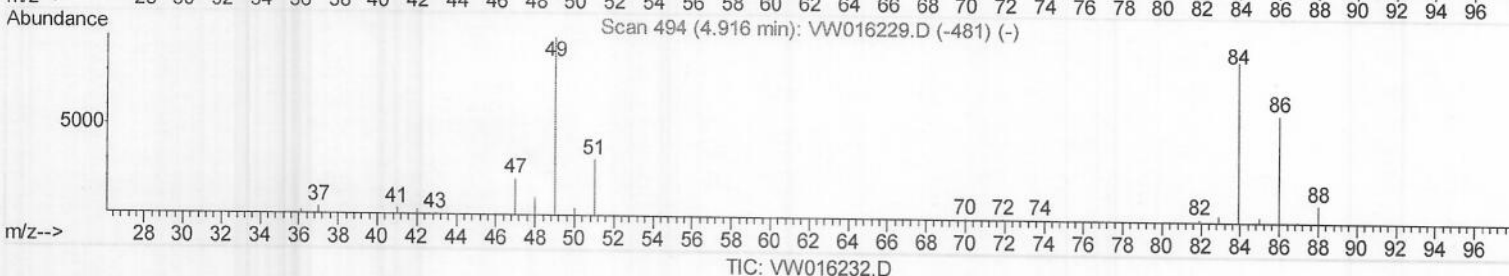
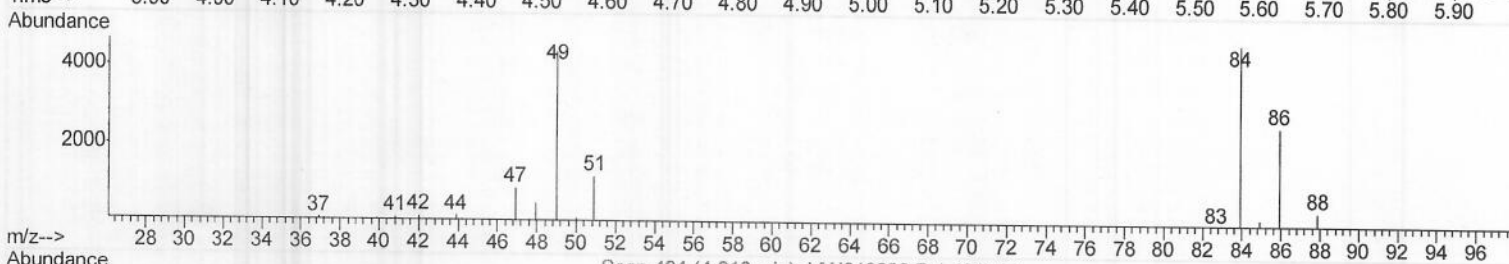
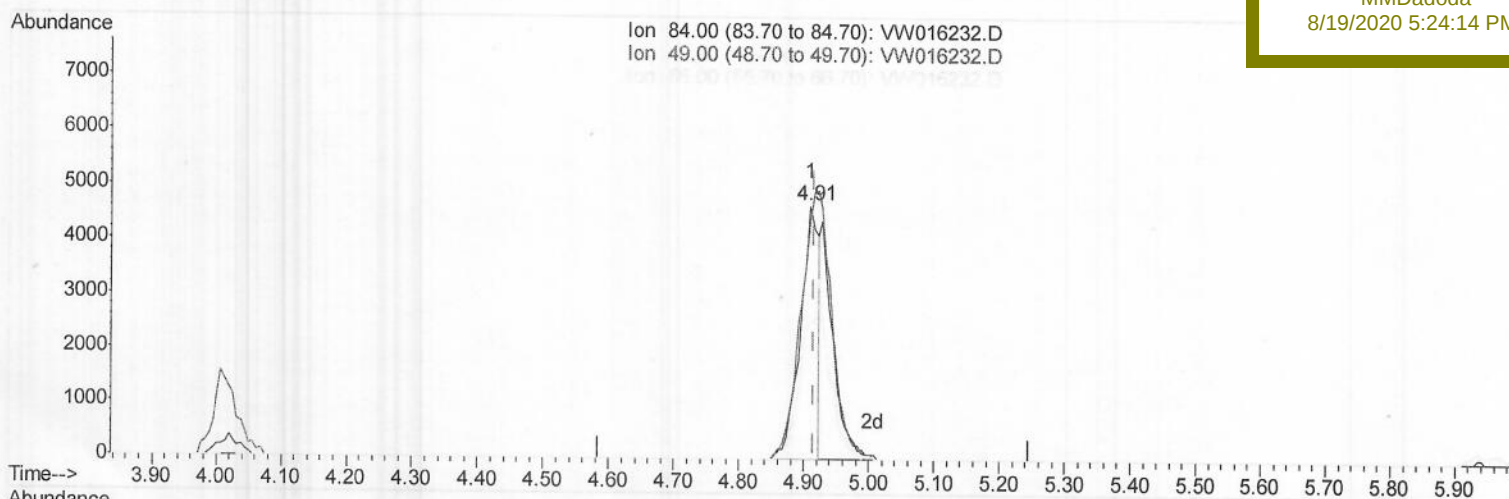
Response via : Initial Calibration

Instrument :

MSVOA_W

Client Sampled :

BFSQ5

Manual Integrations
APPROVEDMMDadoda
8/19/2020 5:24:14 PM

(16) Methylene chloride (T)

4.910min (-0.006) 1.44ug/L

response 8967

Ion	Exp%	Act%
84.00	100	100
49.00	114.90	93.78
86.00	62.50	55.10
0.00	0.00	0.00

Quantitation Report (Qedit)

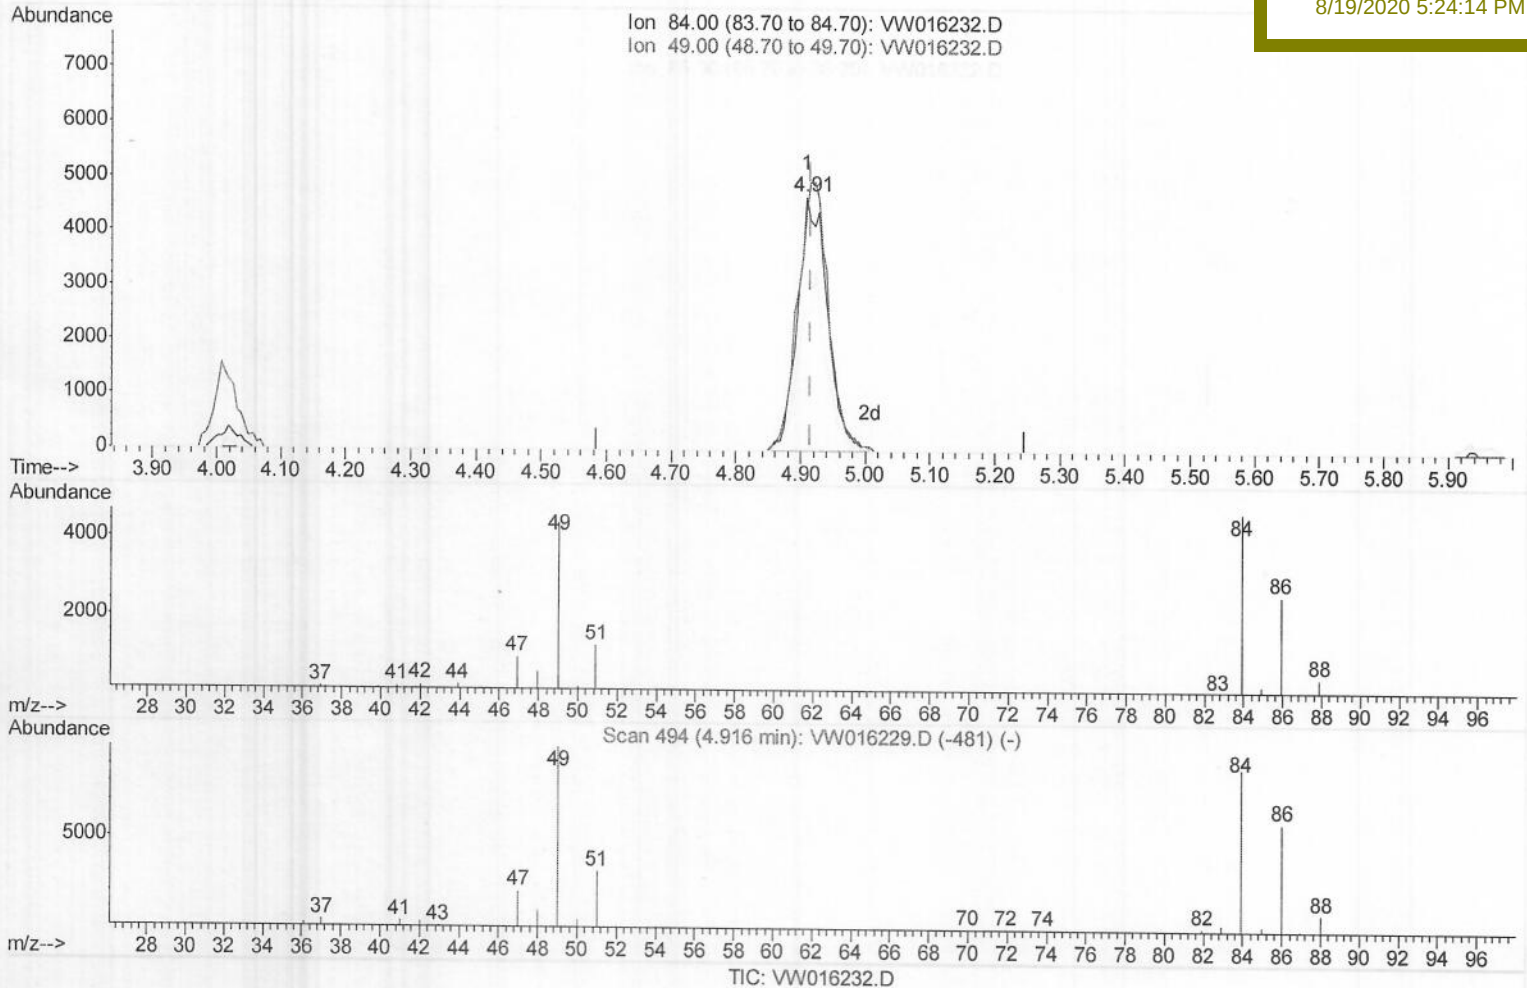
Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081820\
 Data File : VW016232.D
 Acq On : 18 Aug 2020 11:29
 Operator : SY/VA
 Sample : L3709-02
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Aug 19 05:51:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 19 05:49:31 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 ClientSampleId :
 BFSQ5

Manual Integrations
 APPROVED

MMDadoda
 8/19/2020 5:24:14 PM



(16) Methylene chloride (T)

4.910min (-0.006) 2.42ug/L m

response 15080

Ion Exp% Act%

84.00 100 100

49.00 114.90 93.78

86.00 62.50 55.10

0.00 0.00 0.00

> MD
 08/19/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW081820\
 Data File : VW016232.D
 Acq On : 18 Aug 2020 11:29
 Operator : SY/VA
 Sample : L3709-02
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BFSQ5

Quant Time: Aug 19 06:17:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM081020S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 19 05:49:31 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/19/2020 5:24:14 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	394345	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	357605	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	153079	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	91789	18.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.08%
7) Chloroethane-d5	2.90	69	74836	20.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.68%
10) 1,1-Dichloroethene-d2	4.01	63	157062	15.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.52%
20) 2-Butanone-d5	7.09	46	43034	33.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.90%
24) Chloroform-d	7.65	84	221467	20.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.72%
26) 1,2-Dichloroethane-d4	8.31	65	106501	18.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.80%
29) Benzene-d6	8.28	84	433557	22.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.16%
33) 1,2-Dichloropropane-d6	9.28	67	128183	22.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.64%
37) Toluene-d8	10.33	98	396425	22.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.88%
38) trans-1,3-Dichloropropene-	10.58	79	50181	19.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.08%
39) 2-Hexanone-d5	10.93	63	35475	35.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.90%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	95662	20.54	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	130852	24.11	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.44%

Target Compounds

16) Methylene chloride	4.91	84	15080m	2.422	ug/L	Ovalue
------------------------	------	----	--------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> MD
 08/19/20