

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW082120\
 Data File : VW016288.D
 Acq On : 21 Aug 2020 03:17
 Operator : SY/VA
 Sample : L3504-07
 Misc : 8.08G/5ML/MSVOA W/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EO-01-081920

Quant Time: Aug 21 04:39:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 17 08:01:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.63
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.56

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		12.65	95	80	0.00	ug/l	0.03
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW082120\
Data File : VW016288.D
Acq On : 21 Aug 2020 03:17
Operator : SY/VA
Sample : L3504-07
Misc : 8.08G/5ML/MSVOA W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EO-01-081920

Quant Time: Aug 21 04:39:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W081420S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 17 08:01:41 2020
Response via : Initial Calibration

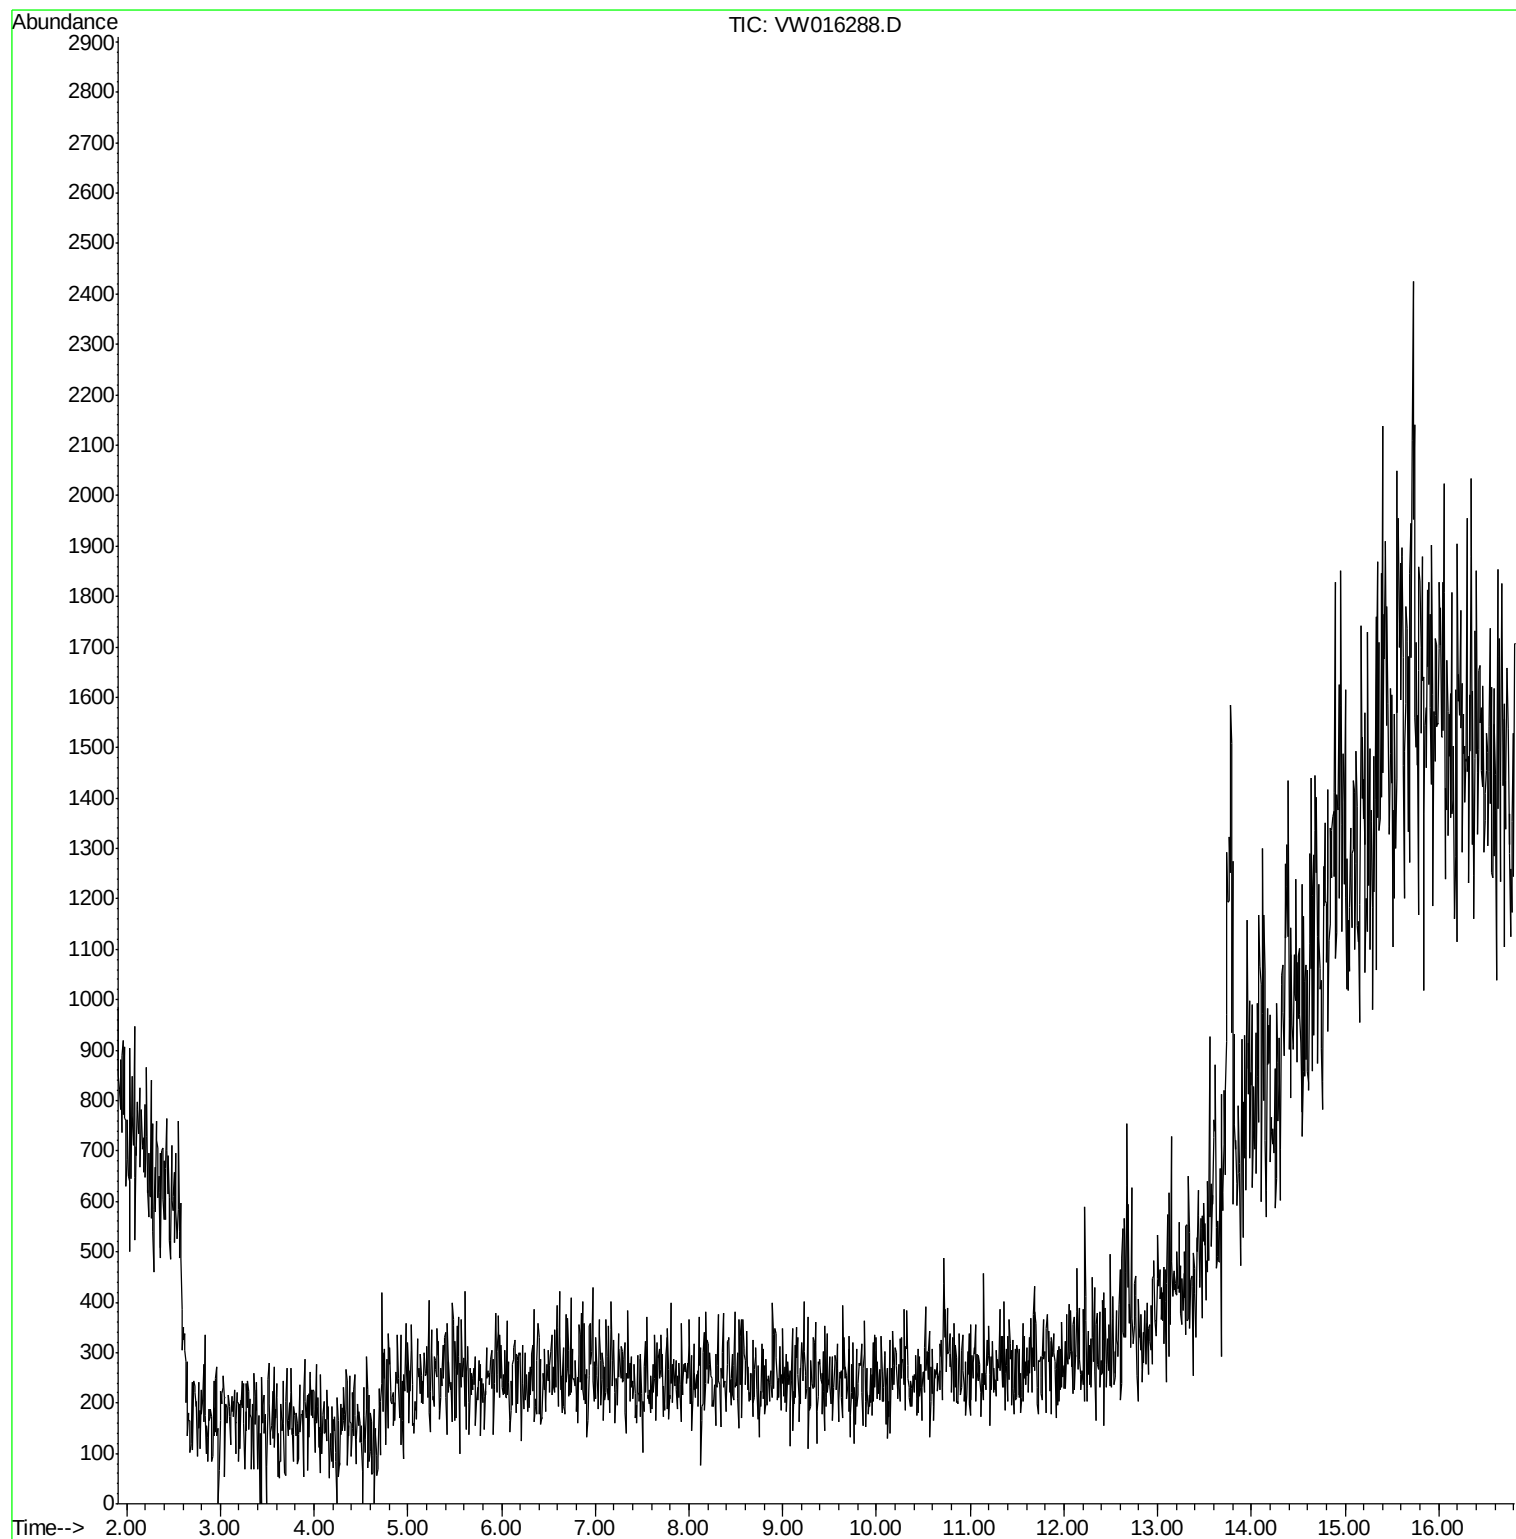

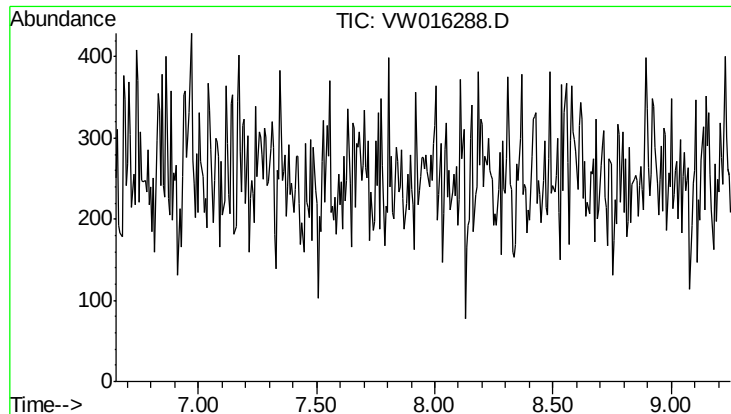

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.95 min

Lab File: VW016288.D

Acq: 21 Aug 2020 03:17

Tot Ion: 168

Sig Exp Ratio

168 100



99 60.4

Instrument :

MSVOA_W

ClientSampleId :

EO-01-081920

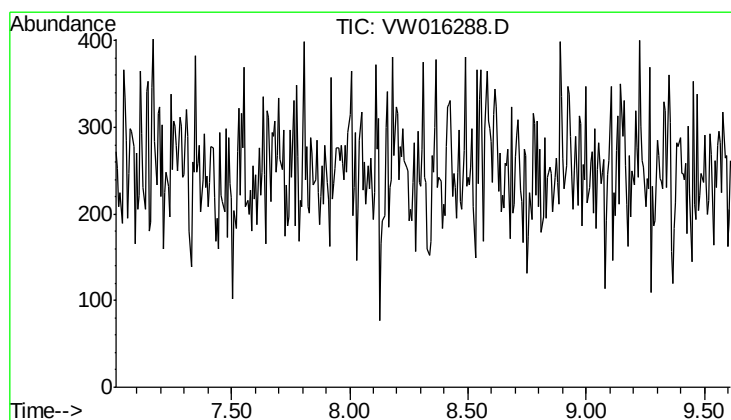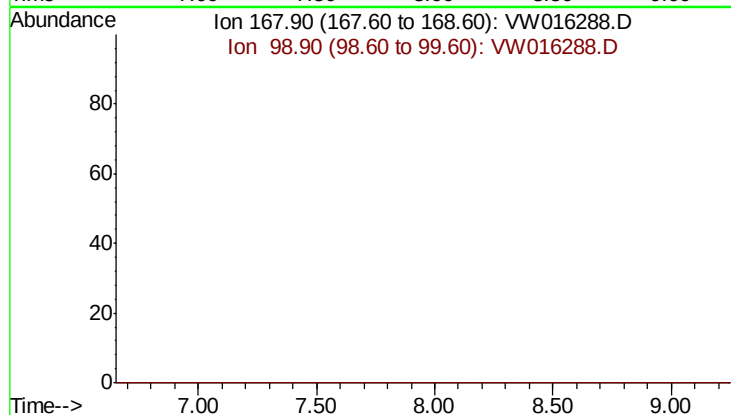

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.31 min

Lab File: VW016288.D


Acq: 21 Aug 2020 03:17


Tgt Ion: 65

Sig Exp Ratio

65 100

67 52.8

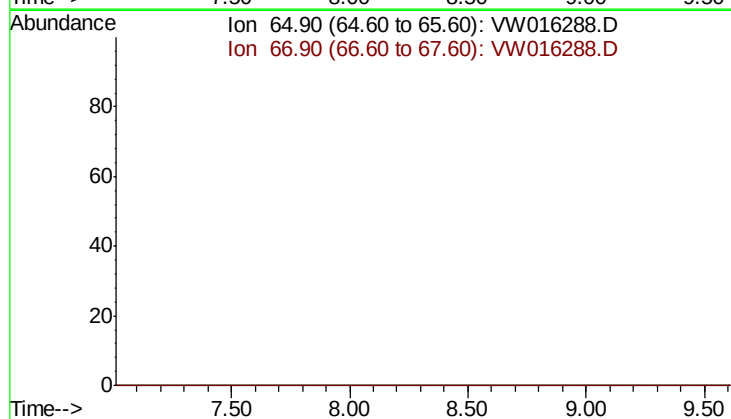

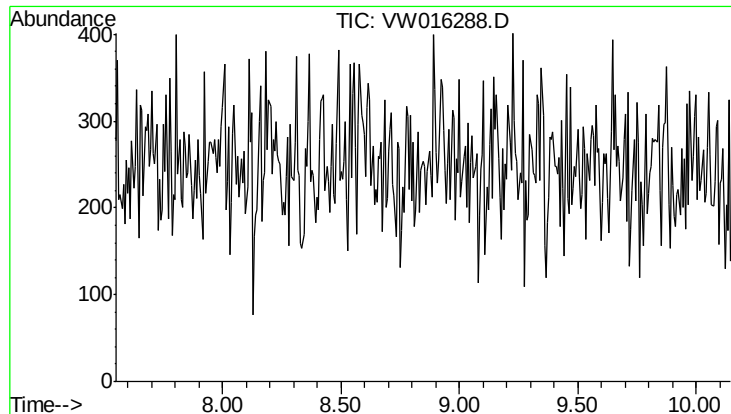

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 8.85 min

Lab File: VW016288.D

Acq: 21 Aug 2020 03:17

Tot Ion: 114



Sig	Exp Ratio
114	100
63	19.2
88	16.4

Instrument :

MSVOA_W

ClientSampleId :

EO-01-081920

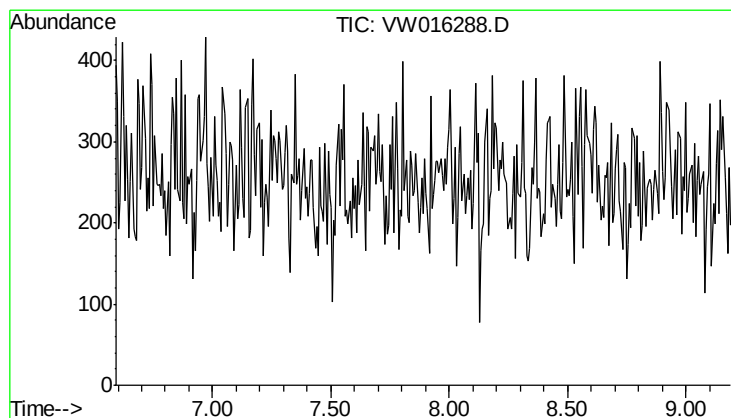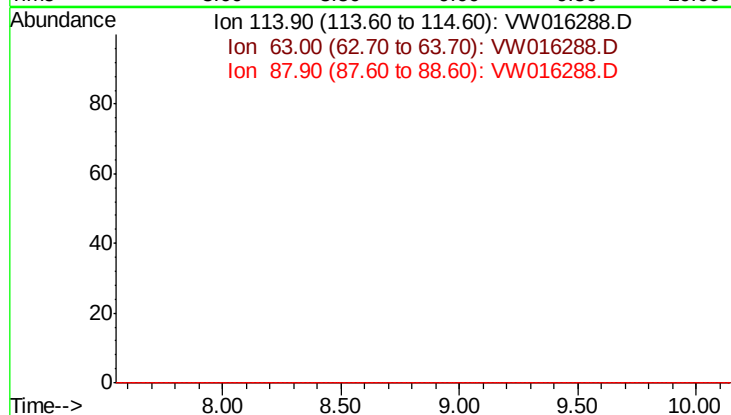

#35

Dibromofluoromethane

Concen: 0.000 ug/l


Expected RT: 7.89 min


Lab File: VW016288.D

Acq: 21 Aug 2020 03:17

Tgt Ion: 113

Sig	Exp Ratio
113	100
111	104.4
192	17.9

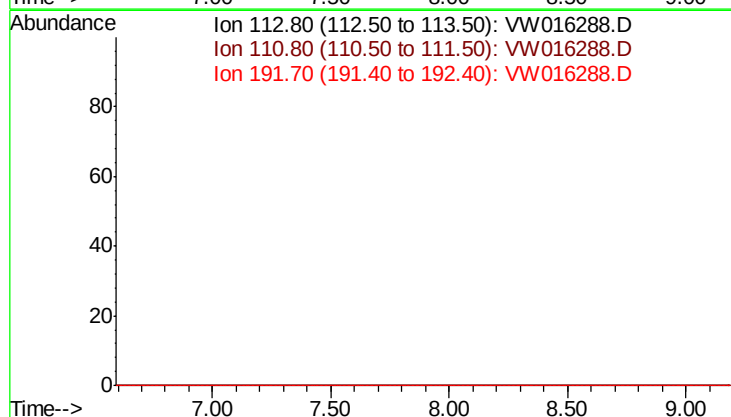


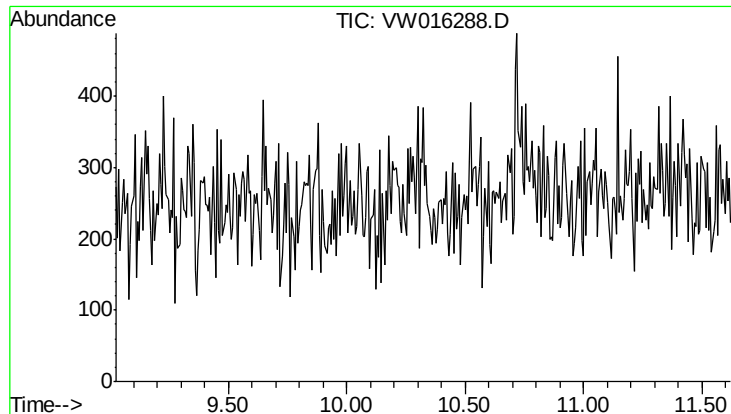


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.32 min

Lab File: VW016288.D
Acq: 21 Aug 2020 03:17




Instrument :
MSVOA_W
ClientSampleId :
EO-01-081920


Tot Ion: 98
Sig Exp Ratio
98 100
100 66.9

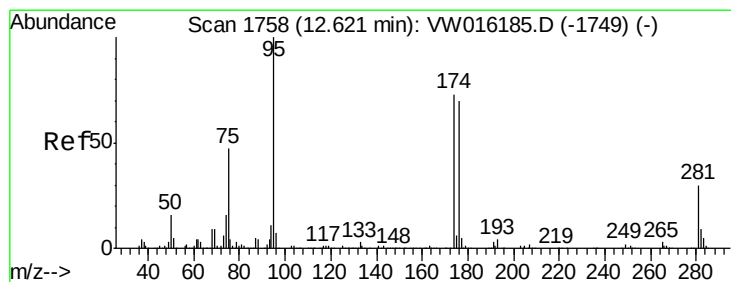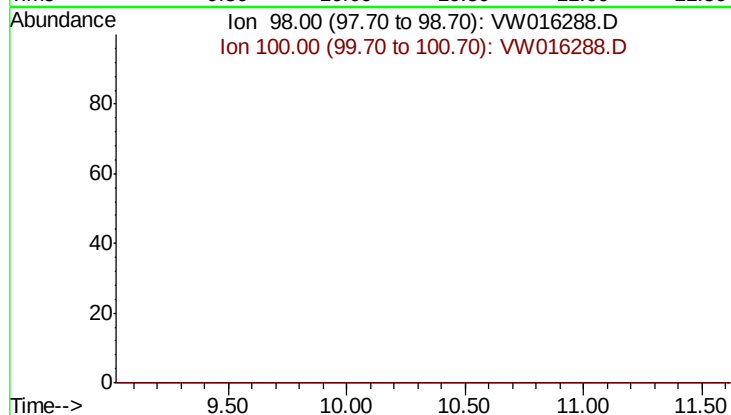

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 12.65 min Scan# 1763
Delta R.T. 0.03 min
Lab File: VW016288.D
Acq: 21 Aug 2020 03:17

Tgt Ion: 95 Resp: 80
Ion Ratio Lower Upper
95 100
174 0.0 0.0 145.6
176 0.0 0.0 137.8

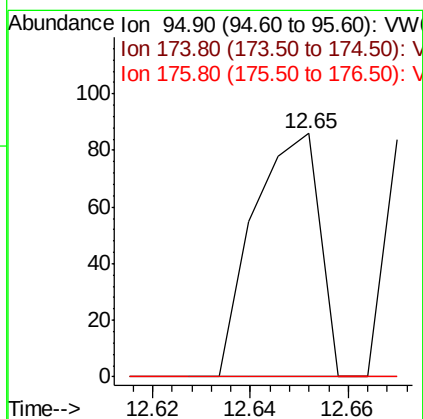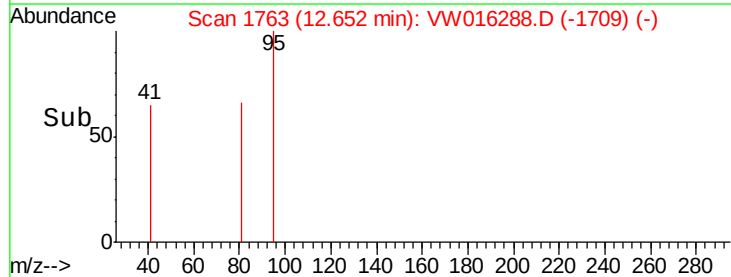
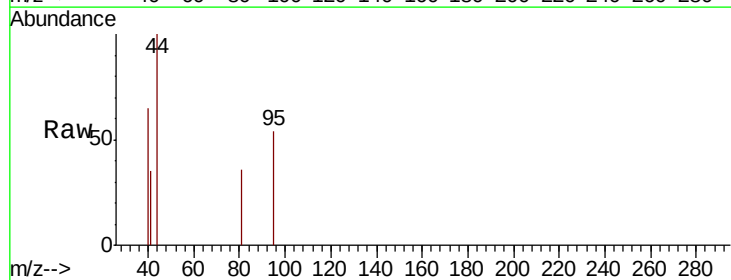


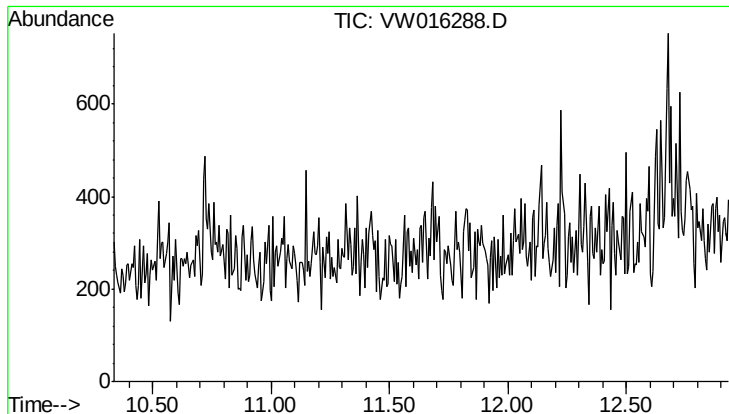

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.63 min
 Lab File: VW016288.D
 Acq: 21 Aug 2020 03:17

Instrument :
 MSVOA_W
 ClientSampleId :
 EO-01-081920

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 54.5
 119 31.7

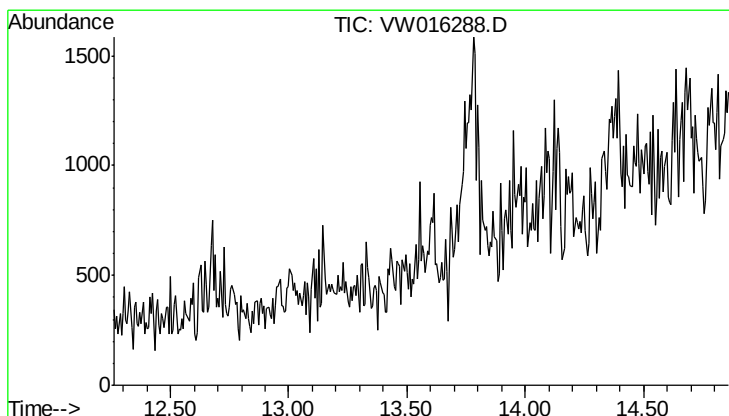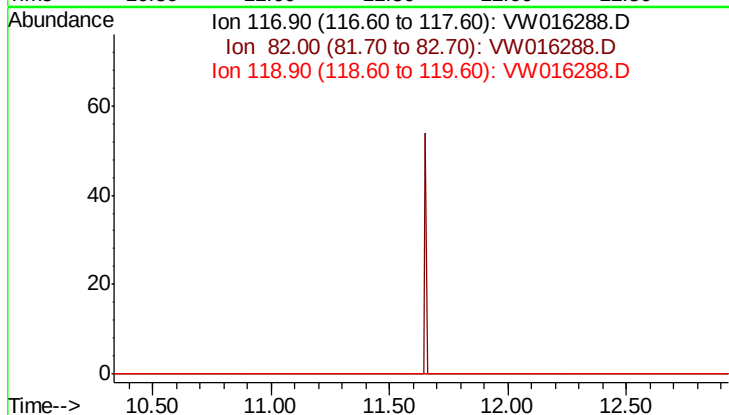

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.56 min
 Lab File: VW016288.D
 Acq: 21 Aug 2020 03:17

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 61.7
 150 168.9

