


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090120\
Data File : VW016429.D
Acq On : 01 Sep 2020 09:28
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082820S.M
Title : SW846 8260
Last Update : Fri Aug 28 15:01:43 2020

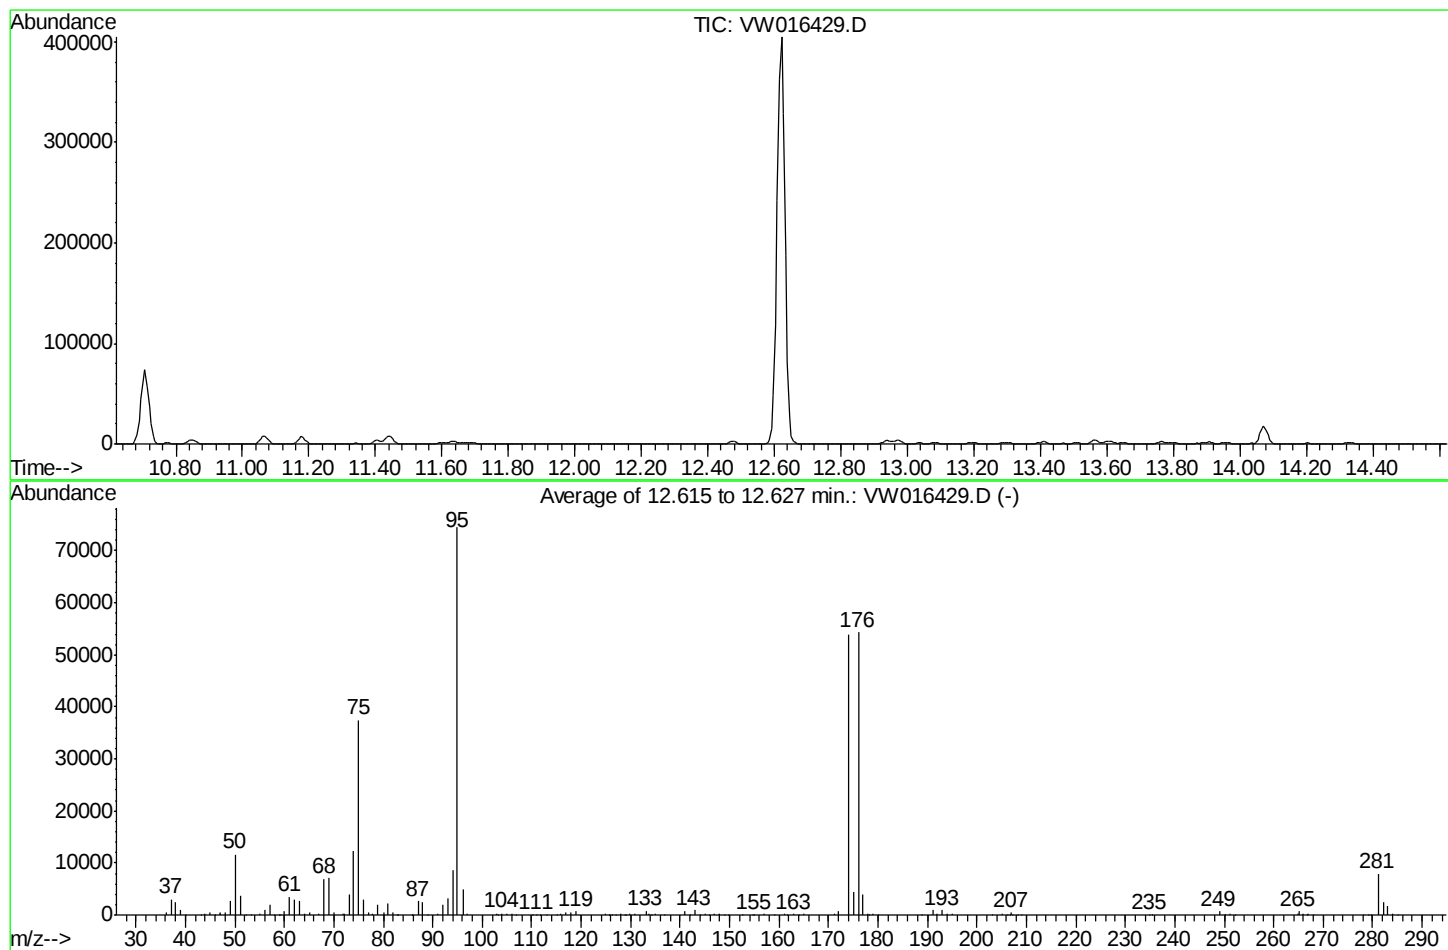

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	11653	PASS
75	95	30	60	50.3	37474	PASS
95	95	100	100	100.0	74509	PASS
96	95	5	9	6.7	4989	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.4	53981	PASS
175	174	5	9	8.2	4424	PASS
176	174	95	101	100.6	54312	PASS
177	176	5	9	7.3	3960	PASS