

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
 Data File : VW019971.D
 Acq On : 01 Sep 2021 10:30
 Operator : SY/VA
 Sample : M3526-10
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

SAM
 9/3/2021 5:33:44 PM

Quant Time: Sep 02 03:56:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 02 03:54:23 2021
 Response via : Initial Calibration

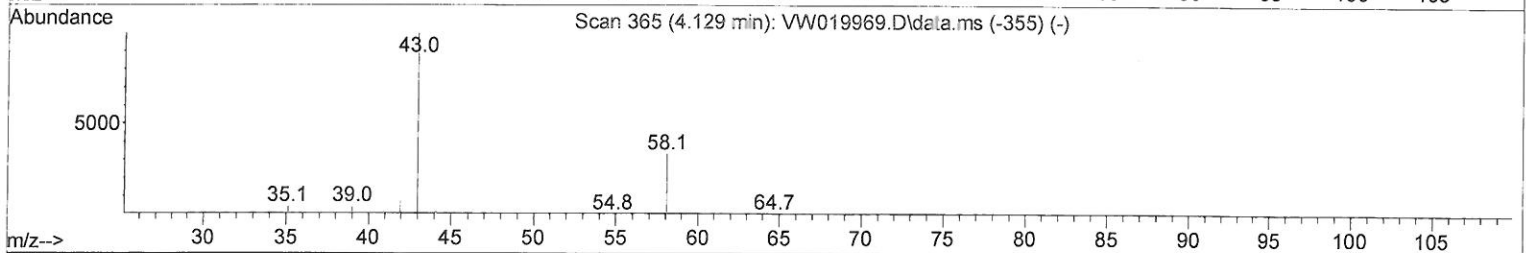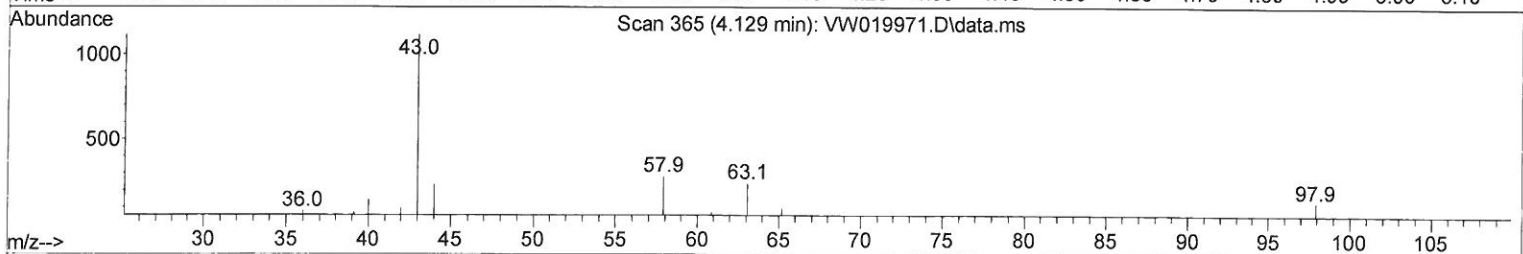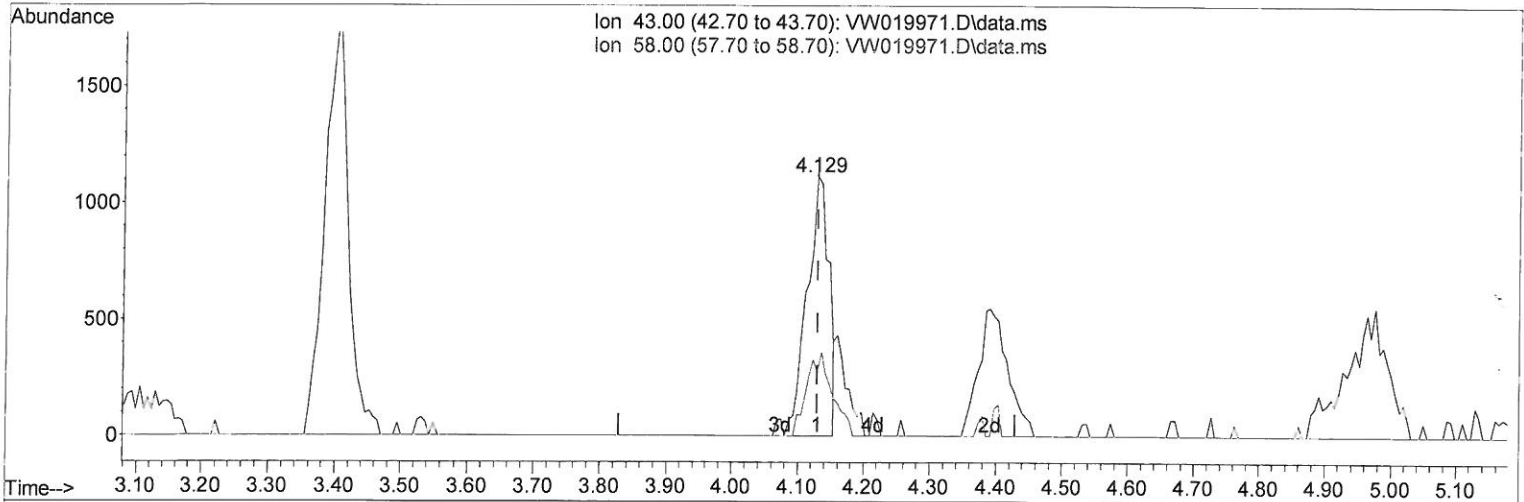

TIC: VW019971.D\data.ms

(13) Acetone (T)

4.129min (+ 0.000) 3.23 ug/L

response 2553

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	17.59
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
 Data File : VW019971.D
 Acq On : 01 Sep 2021 10:30
 Operator : SY/VA
 Sample : M3526-10
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

SAM
 9/3/2021 5:33:44 PM

Quant Time: Sep 02 03:56:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 02 03:54:23 2021
 Response via : Initial Calibration

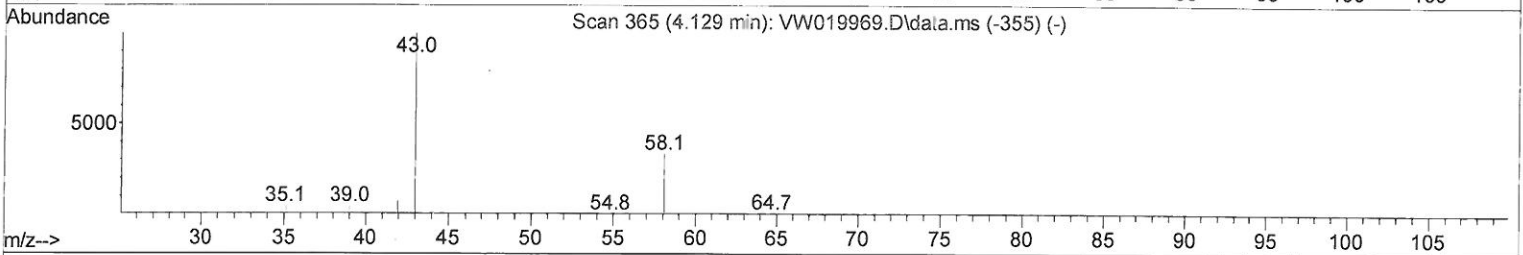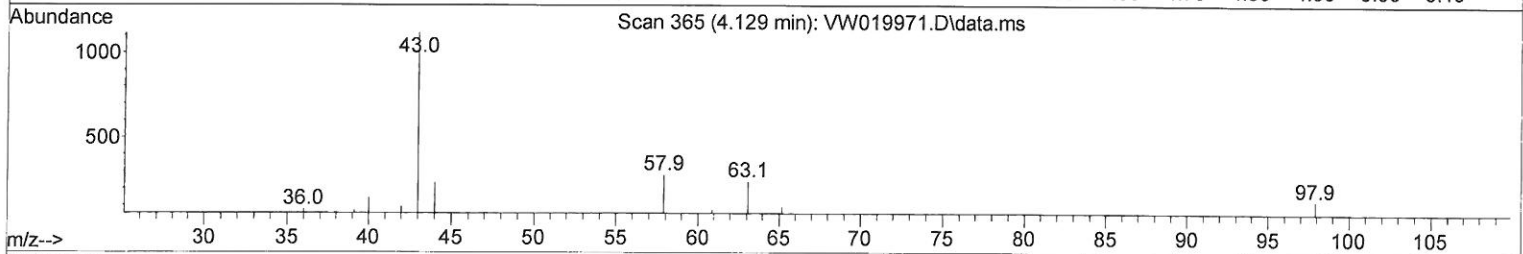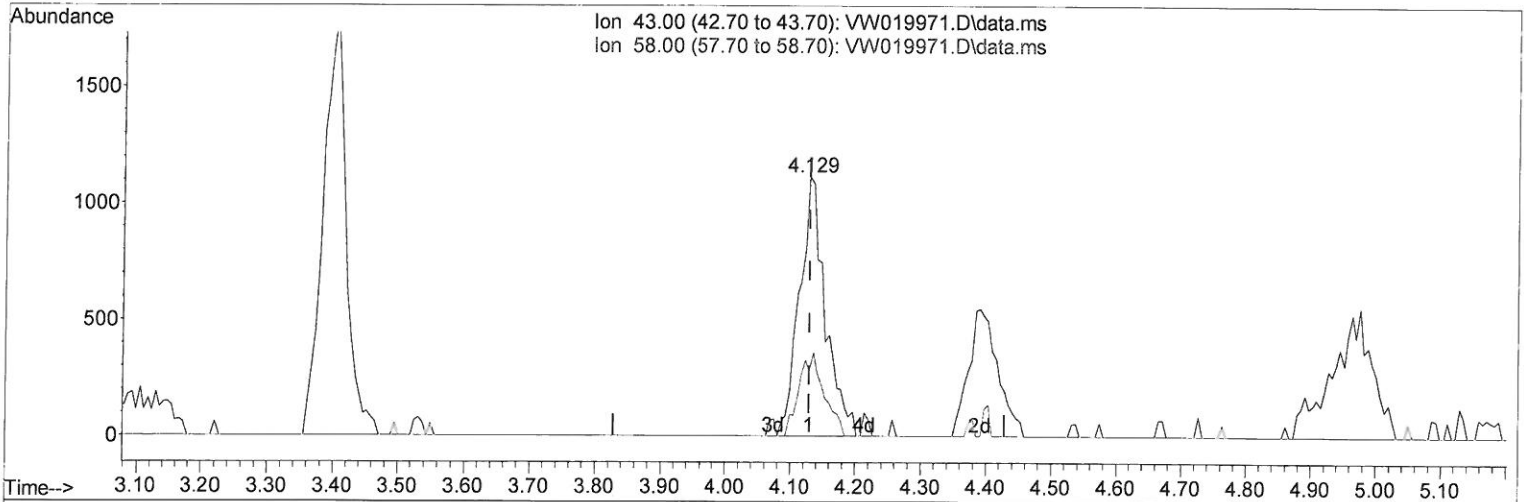

TIC: VW019971.D\data.ms

(13) Acetone (T)

4.129min (+ 0.000) 3.93 ug/L m

response 3099

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	14.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
 Data File : VW019971.D
 Acq On : 01 Sep 2021 10:30
 Operator : SY/VA
 Sample : M3526-10
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

SAM
 9/3/2021 5:33:44 PM

Quant Time: Sep 02 03:56:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 02 03:54:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	293875	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	291819	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	137190	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	98296	21.59	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.36%		
7) Chloroethane-d5	2.904	69	90109	22.55	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.20%		
11) 1,1-Dichloroethene-d2	4.025	63	115047	14.56	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	58.24%		
21) 2-Butanone-d5	7.080	46	45315	49.00	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.00%		
24) Chloroform-d	7.653	84	186766	23.11	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.44%		
26) 1,2-Dichloroethane-d4	8.305	65	102053	23.43	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.72%		
32) Benzene-d6	8.281	84	361585	21.73	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.92%		
36) 1,2-Dichloropropane-d6	9.281	67	111965	22.22	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.88%		
41) Toluene-d8	10.323	98	314310	20.61	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.44%		
43) trans-1,3-Dichloroprop...	10.579	79	42495	20.41	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.64%		
47) 2-Hexanone-d5	10.927	63	28864	41.12	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.24%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	95464	23.28	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.12%		
66) 1,2-Dichlorobenzene-d4	13.853	152	115450	24.53	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.12%		
Target Compounds						
13) Acetone	4.129	43	3099m	3.93	ug/L	Qvalue 88
16) Methylene chloride	4.915	84	16394	3.25	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
Data File : VW019971.D
Acq On : 01 Sep 2021 10:30
Operator : SY/VA
Sample : M3526-10
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual Integrations
APPROVED

SAM
9/3/2021 5:33:44 PM

Quant Time: Sep 02 03:56:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 02 03:54:23 2021
Response via : Initial Calibration

