

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
Data File : VW019973.D
Acq On : 01 Sep 2021 13:56
Operator : SY/VA
Sample : VIBLK430
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK430

Manual Integrations
APPROVED

MMDadoda
9/3/2021 5:24:24 PM

Quant Time: Sep 02 03:58:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 02 03:54:23 2021
Response via : Initial Calibration

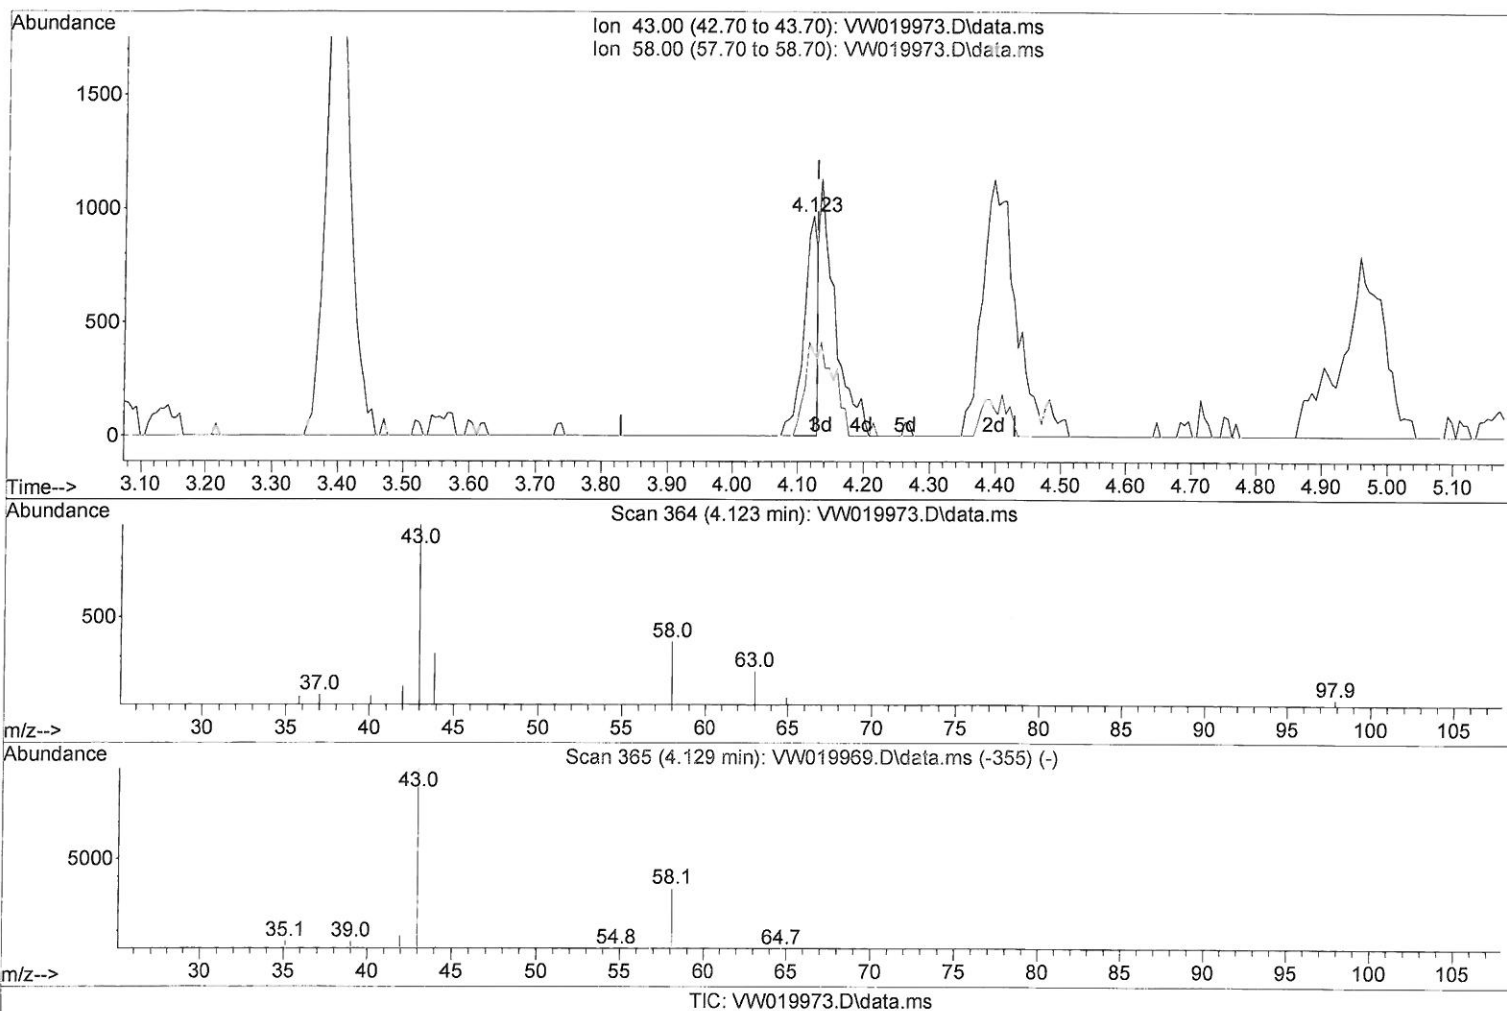

(13) Acetone (T)

4.123min (-0.006) 1.85 ug/L

response 1449

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	38.72
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
 Data File : VW019973.D
 Acq On : 01 Sep 2021 13:56
 Operator : SY/VA
 Sample : VIBLK430
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK430

Manual Integrations
 APPROVED

MMDadoda
 9/3/2021 5:24:24 PM

Quant Time: Sep 02 03:58:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 02 03:54:23 2021
 Response via : Initial Calibration

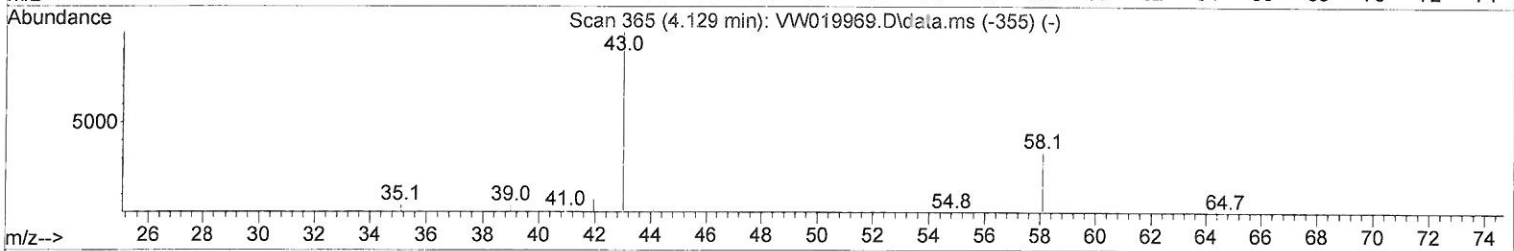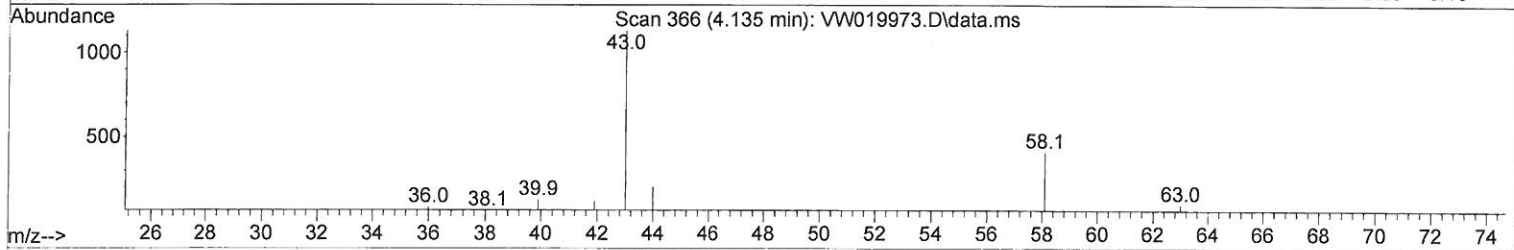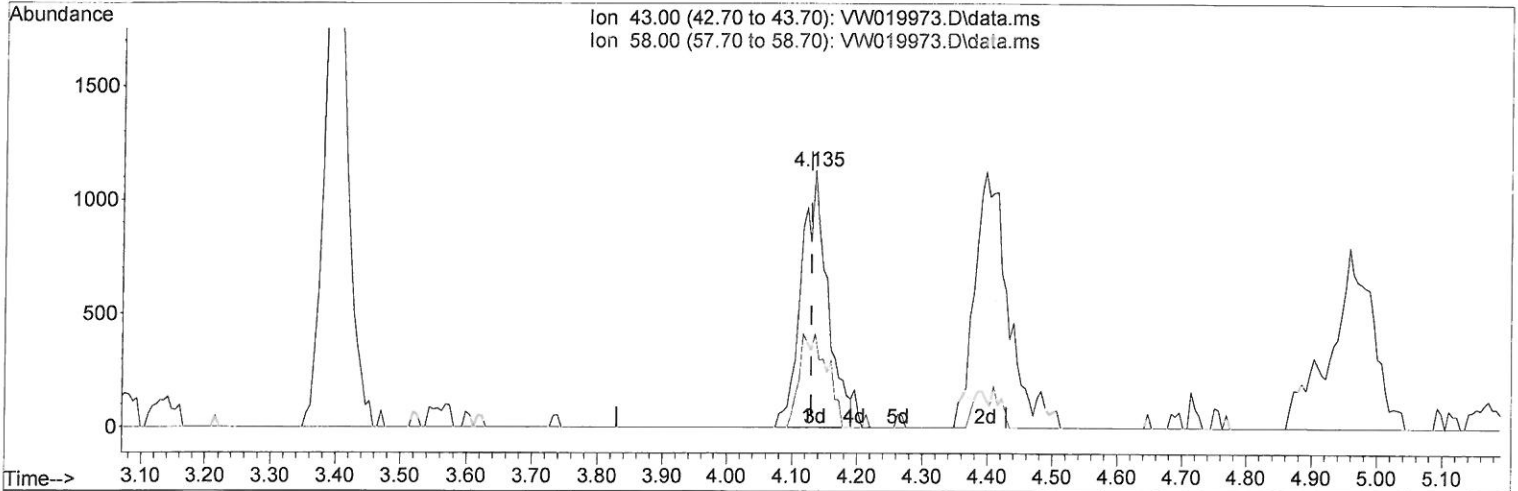

TIC: VW019973.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 4.05 ug/L m

response 3169

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	17.70
0.00	0.00	0.00
0.00	0.00	0.00

09/09/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
 Data File : VW019973.D
 Acq On : 01 Sep 2021 13:56
 Operator : SY/VA
 Sample : VIBLK430
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK430

Manual Integrations
 APPROVED

MMDadoda
 9/3/2021 5:24:24 PM

Quant Time: Sep 02 03:58:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 02 03:54:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	291074	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	286732	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	133646	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	98118	21.76	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.04%		
7) Chloroethane-d5	2.898	69	90141	22.77	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.08%		
11) 1,1-Dichloroethene-d2	4.025	63	114903	14.68	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	58.72%		
21) 2-Butanone-d5	7.080	46	54701	59.71	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	119.42%		
24) Chloroform-d	7.653	84	188859	23.59	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.36%		
26) 1,2-Dichloroethane-d4	8.305	65	107881	25.01	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.04%		
32) Benzene-d6	8.275	84	371316	22.71	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.84%		
36) 1,2-Dichloropropane-d6	9.274	67	111382	22.50	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.00%		
41) Toluene-d8	10.323	98	310295	20.71	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.84%		
43) trans-1,3-Dichloroprop...	10.579	79	45924	22.45	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.80%		
47) 2-Hexanone-d5	10.927	63	36510	52.94	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.88%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	109077	27.07	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	108.28%		
66) 1,2-Dichlorobenzene-d4	13.853	152	113565	24.77	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.08%		
Target Compounds						
13) Acetone	4.135	43	3169m	4.05	ug/L	Qvalue 97
16) Methylene chloride	4.922	84	12726	2.55	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090121\
Data File : VW019973.D
Acq On : 01 Sep 2021 13:56
Operator : SY/VA
Sample : VIBLK430
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK430

Manual Integrations
APPROVED

MMDadoda
9/3/2021 5:24:24 PM

Quant Time: Sep 02 03:58:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWL081821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 02 03:54:23 2021
Response via : Initial Calibration

