


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090419\  
 Data File : VW012608.D  
 Acq On : 04 Sep 2019 22:47  
 Operator : SY/VA  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W082319S.M  
 Title : SW846 8260  
 Last Update : Mon Aug 26 07:18:31 2019

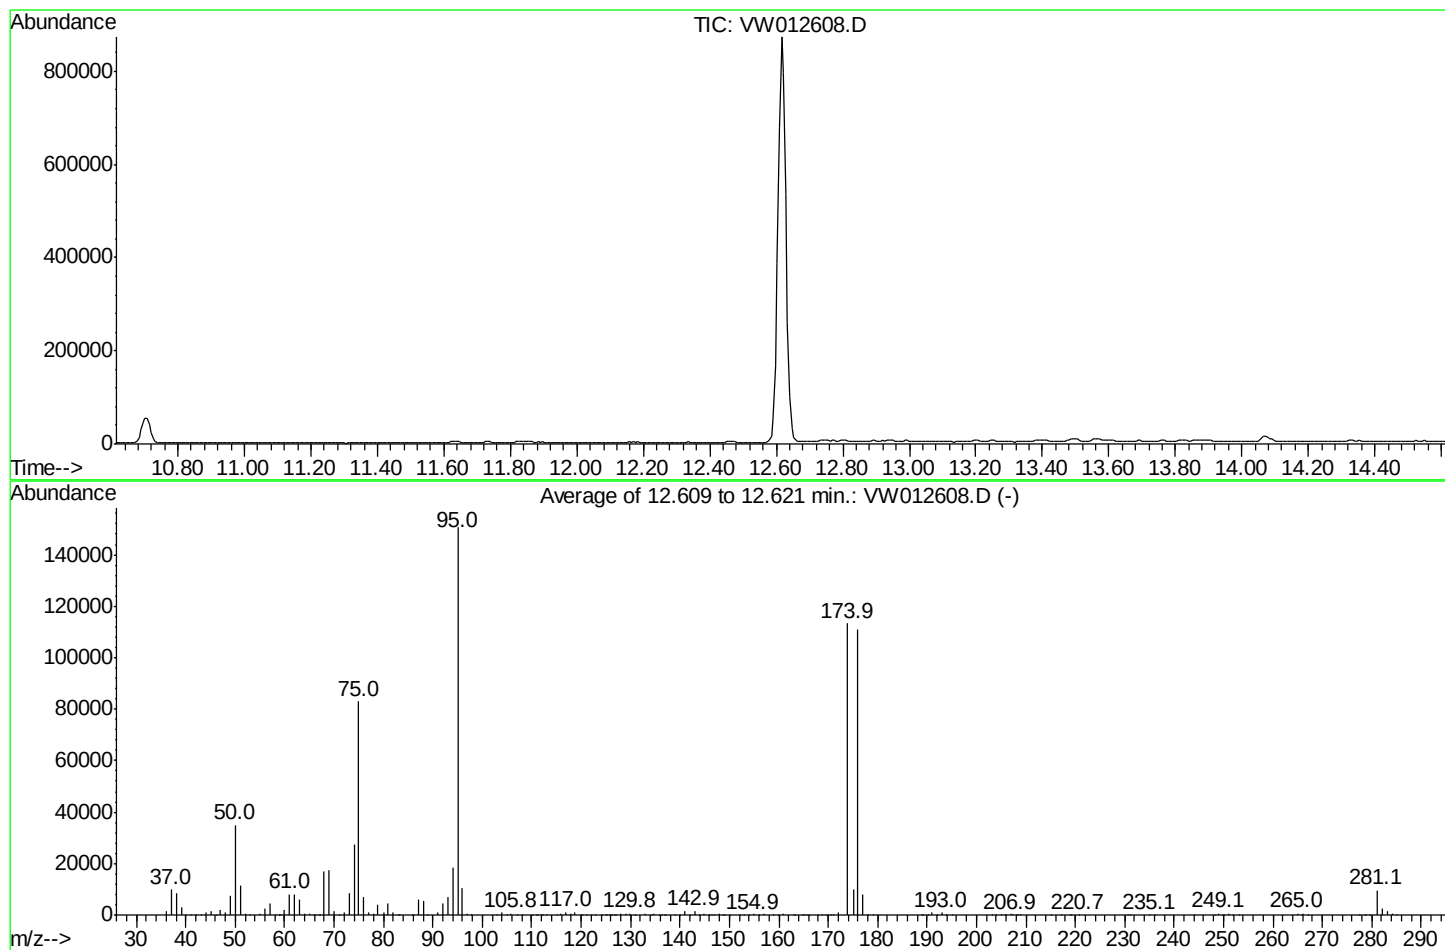

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 23.1      | 34832   | PASS             |
| 75          | 95           | 30           | 60           | 55.1      | 83013   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 150641  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 10396   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 75.2      | 113333  | PASS             |
| 175         | 174          | 5            | 9            | 8.6       | 9741    | PASS             |
| 176         | 174          | 95           | 101          | 97.8      | 110834  | PASS             |
| 177         | 176          | 5            | 9            | 7.1       | 7823    | PASS             |