

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090519\
 Data File : VW012665.D
 Acq On : 06 Sep 2019 02:39
 Operator : SY/VA
 Sample : K4579-10
 Misc : 2.50G/5ML/MSVOA W/SOIL
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 PAR-12-B2-(0)

Quant Time: Sep 06 08:41:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 26 07:18:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	246806	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	412820	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	335002	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	129824	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	156011	53.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.34%	
35) Dibromofluoromethane	7.88	113	119434	48.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.94%	
50) Toluene-d8	10.32	98	466006	46.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.28%	
62) 4-Bromofluorobenzene	12.62	95	143491	40.74	ug/l	0.00
Spiked Amount 50.000			Recovery	=	81.48%	
Target Compounds						
16) Acetone	4.15	43	5872	7.830	ug/l	95
20) Methylene Chloride	4.90	84	26579	9.375	ug/l	93
29) Tetrahydrofuran	7.54	42	6074	9.934	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090519\
Data File : VW012665.D
Acq On : 06 Sep 2019 02:39
Operator : SY/VA
Sample : K4579-10
Misc : 2.50G/5ML/MSVOA W/SOIL
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PAR-12-B2-(0)

Quant Time: Sep 06 08:41:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 26 07:18:31 2019
Response via : Initial Calibration

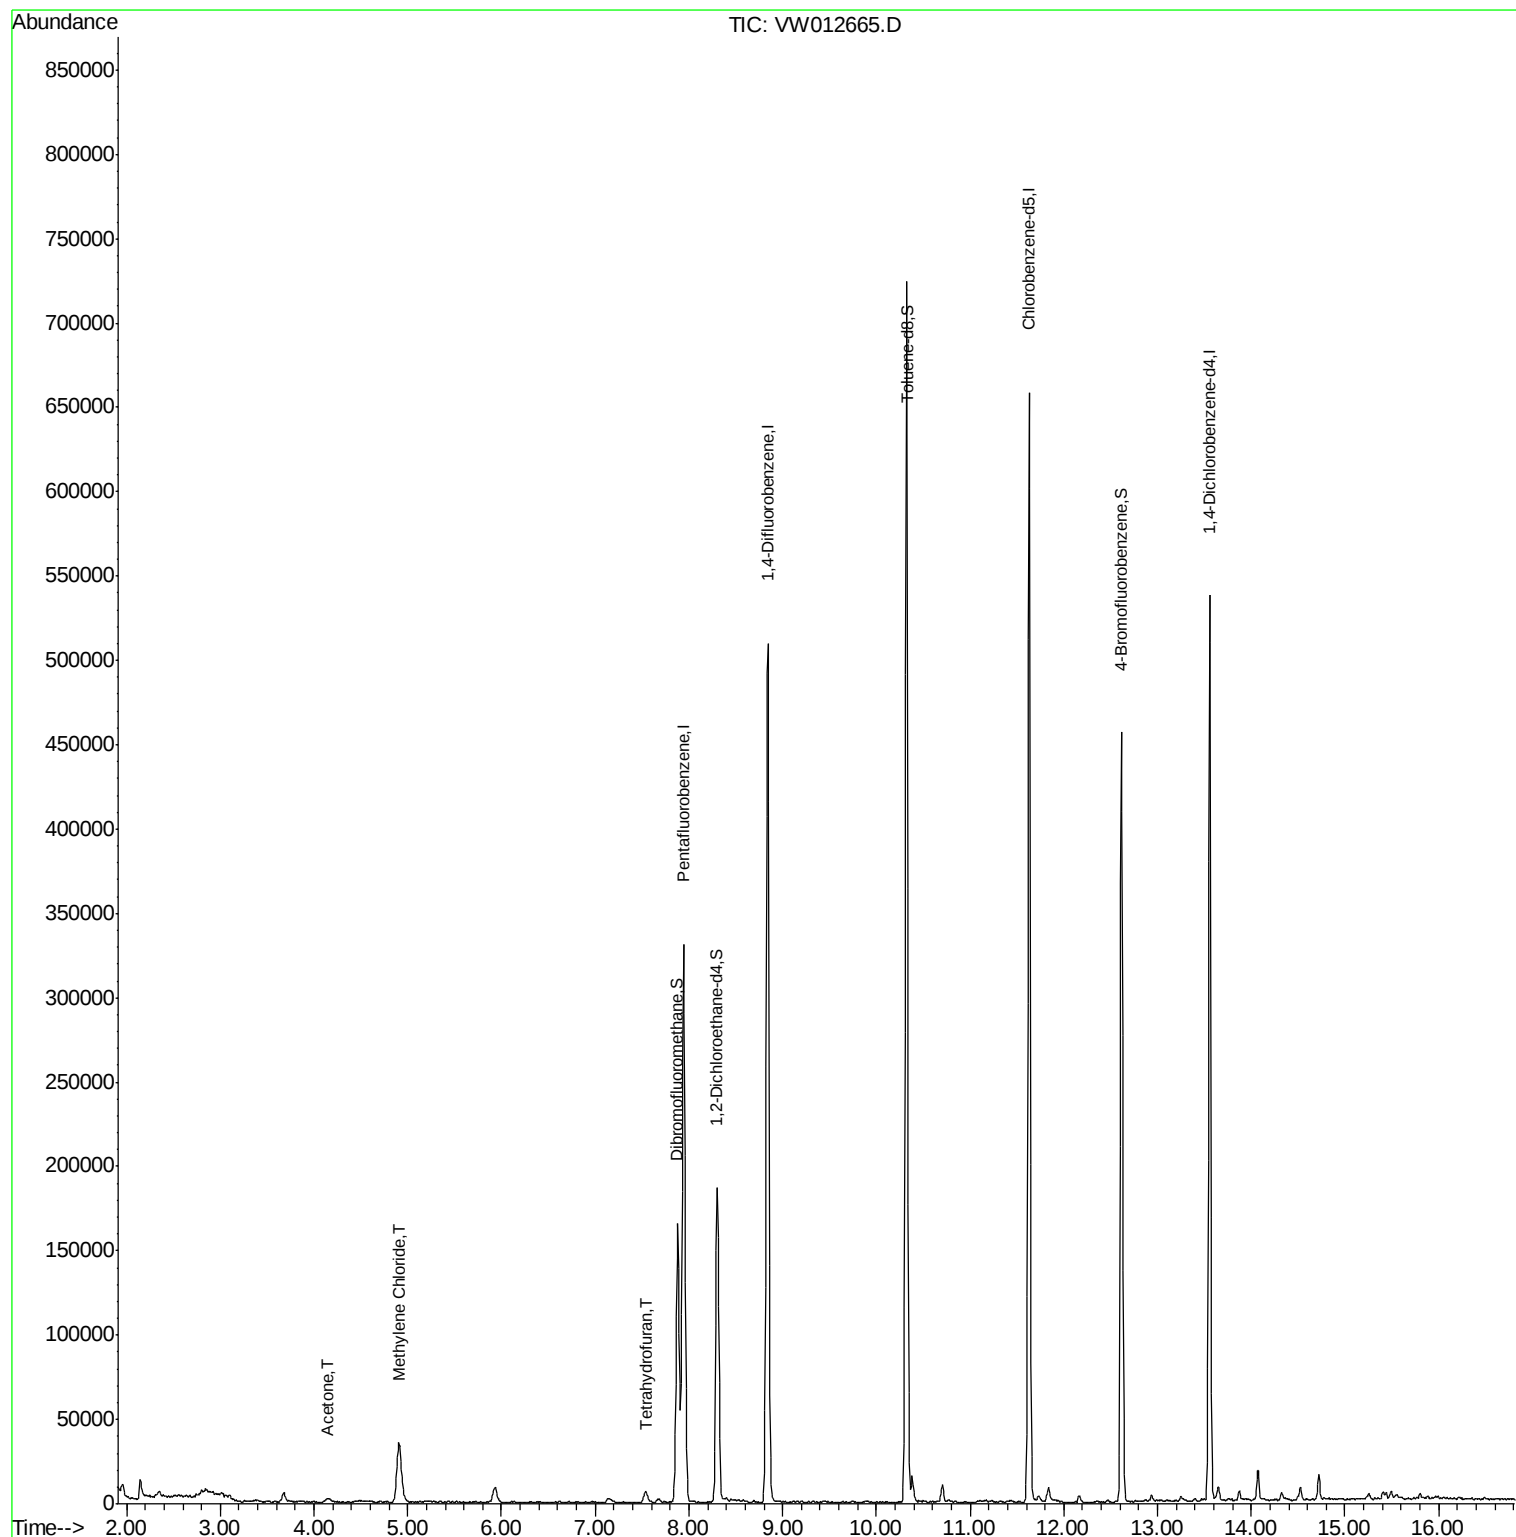



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39

Instrument :

MSVOA_W

ClientSampleId :


PAR-12-B2-(0)

Tot Ion:168 Resp: 246806

Ion Ratio Lower Upper

168 100

99 58.1 49.2 73.8

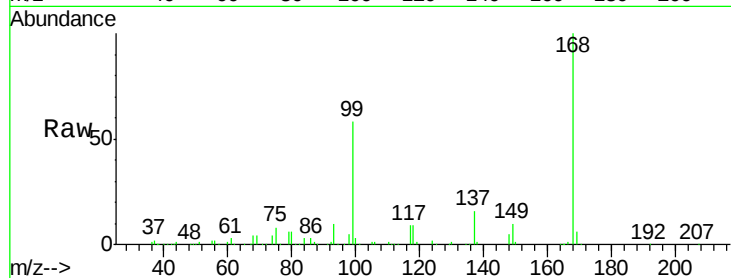

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

120000

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00

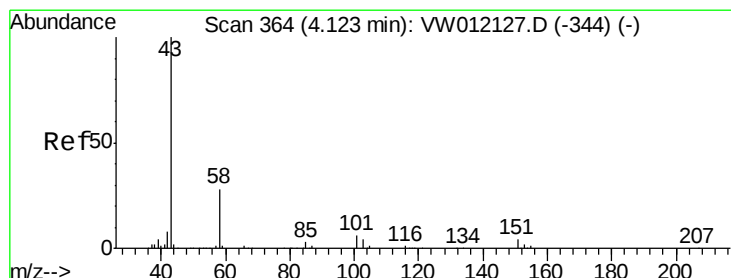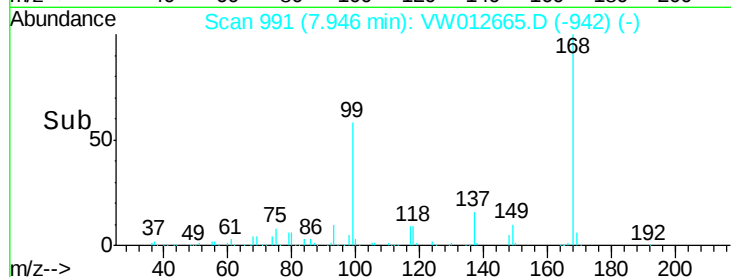

#16

Acetone

Concen: 7.830 ug/l

RT: 4.15 min Scan# 368

Delta R.T. 0.02 min

Lab File: VW012665.D


Acq: 06 Sep 2019 02:39

Tgt Ion: 43 Resp: 5872

Ion Ratio Lower Upper

43 100

58 25.4 22.4 33.6

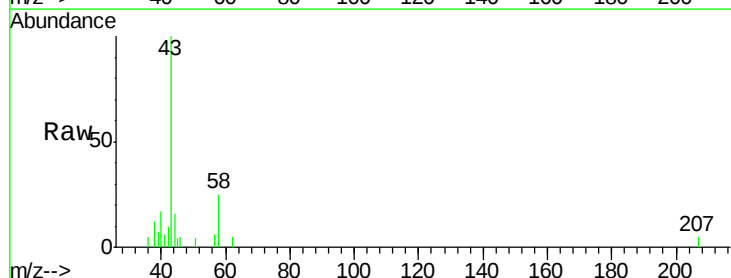

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.15


1500


1000

500

0

Time--> 4.00 4.10 4.20 4.30

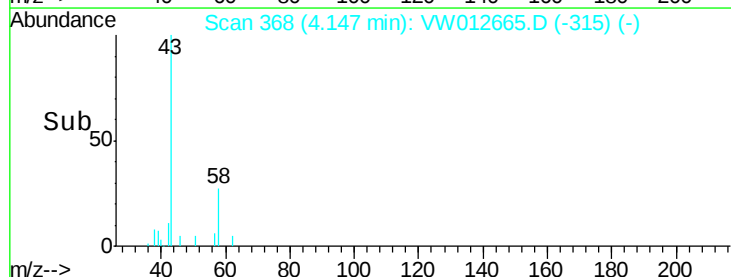

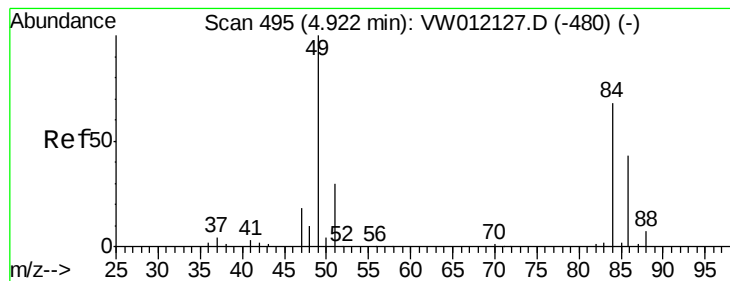

#20

Methvlene Chloride

Concen: 9.375 ug/l

RT: 4.90 min Scan# 492

Delta R.T. -0.02 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-B2-(0)

Tot Ion: 84 Resp: 26579



Ion Ratio Lower Upper

84 100

49 136.2 117.8 176.8

51 47.9 35.6 53.4

86 61.5 51.2 76.8

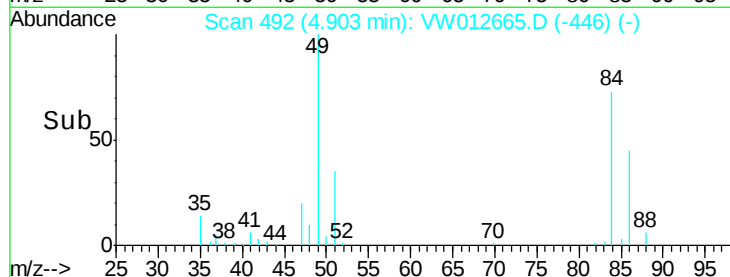
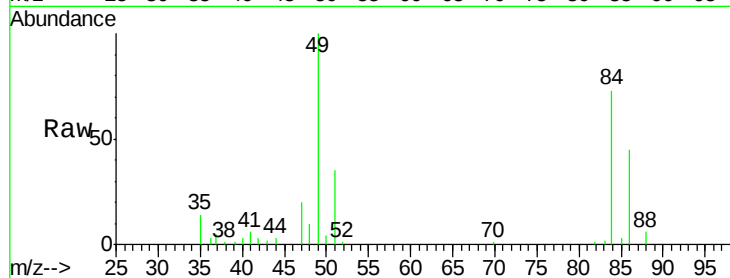


Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

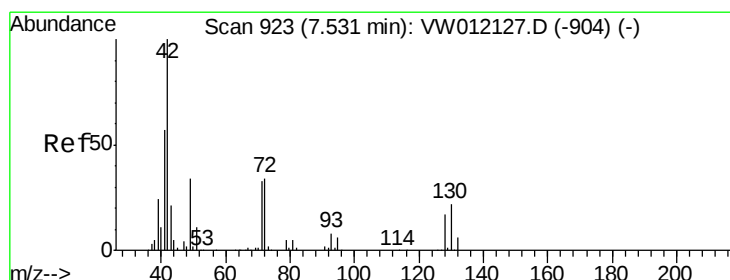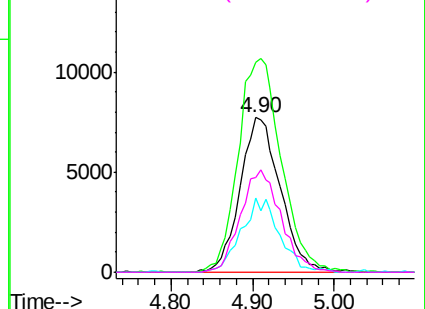

#29

Tetrahydrofuran

Concen: 9.934 ug/l

RT: 7.54 min Scan# 924

Delta R.T. 0.01 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39



Tgt Ion: 42 Resp: 6074

Ion Ratio Lower Upper

42 100

72 35.4 27.3 40.9


71 36.8 25.5 38.3

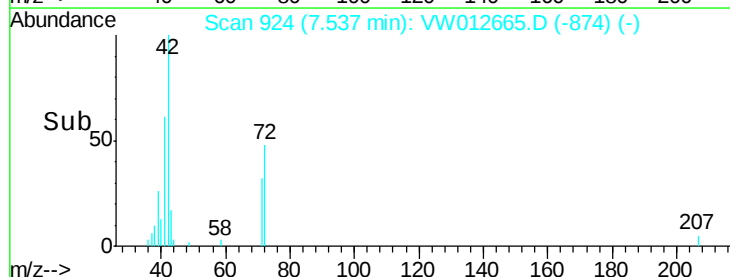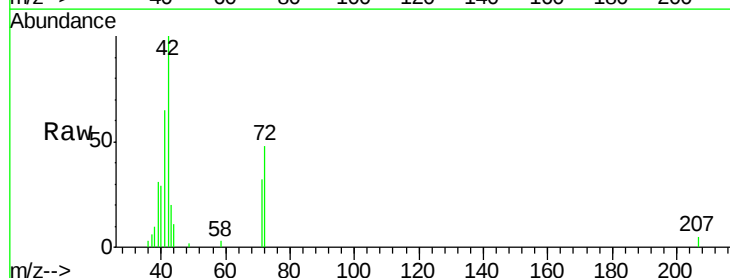


Abundance Ion 42.00 (41.70 to 42.70): VW

Ion 72.00 (71.70 to 72.70): VW

Ion 71.00 (70.70 to 71.70): VW




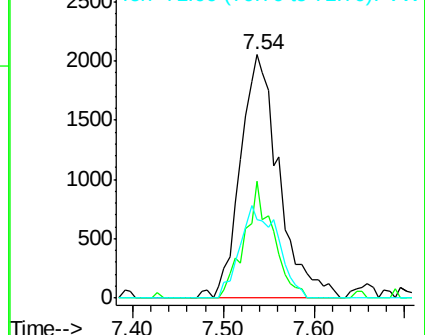


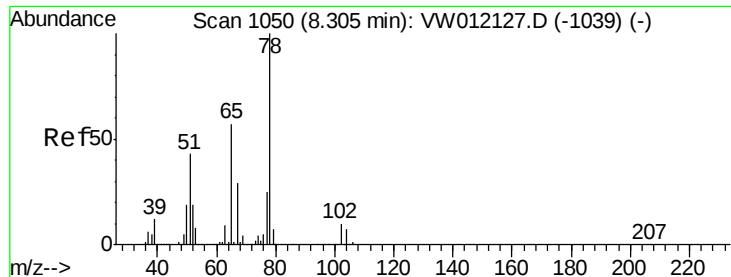

#33
 1,2-Dichloroethane-d4
 Concen: 53.175 ug/l
 RT: 8.30 min Scan# 1049
 Delta R.T. -0.01 min
 Lab File: VW012665.D
 Acq: 06 Sep 2019 02:39




Instrument :
 MSVOA_W
 ClientSampleId :
 PAR-12-B2-(0)


Tot Ion: 65 Resp: 156011
 Ion Ratio Lower Upper
 65 100
 67 50.8 0.0 102.6

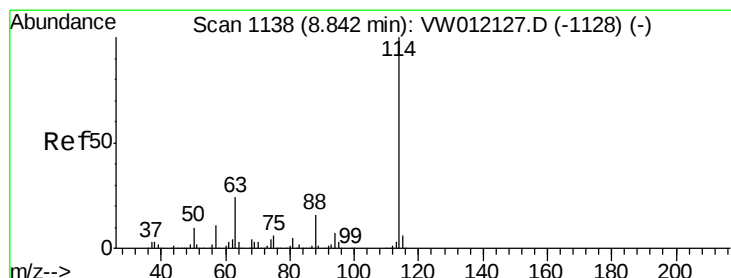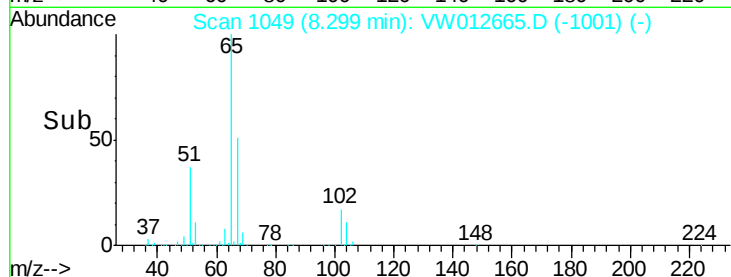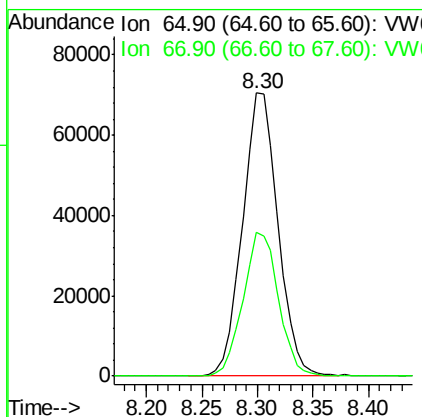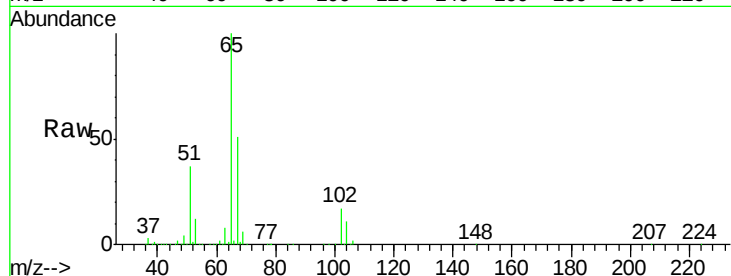

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW012665.D
 Acq: 06 Sep 2019 02:39

Tgt Ion: 114 Resp: 412820
 Ion Ratio Lower Upper
 114 100
 63 23.6 0.0 48.6
 88 15.6 0.0 32.2


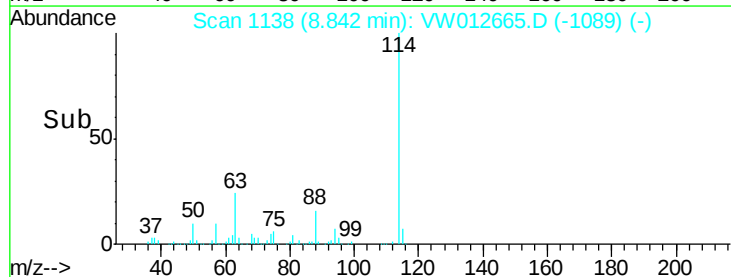
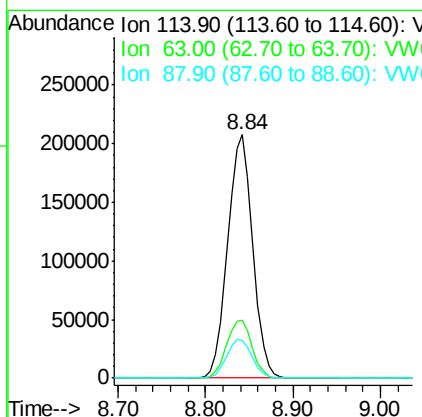
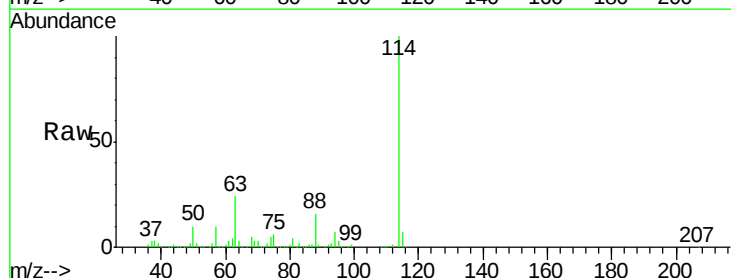


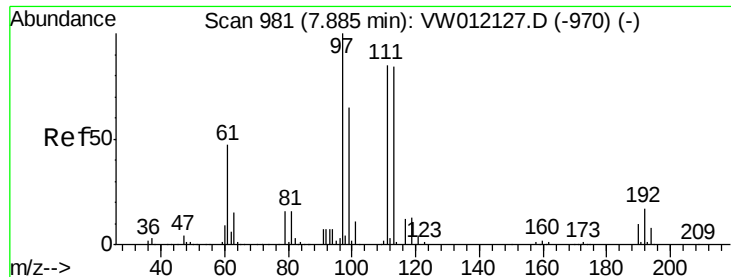

#35
 Dibromofluoromethane
 Concen: 48.469 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.01 min
 Lab File: VW012665.D
 Acq: 06 Sep 2019 02:39




Instrument :
 MSVOA_W
 ClientSampleId :
 PAR-12-B2-(0)


Tot Ion:113 Resp: 119434
 Ion Ratio Lower Upper
 113 100
 111 101.0 82.7 124.1
 192 22.1 16.2 24.2

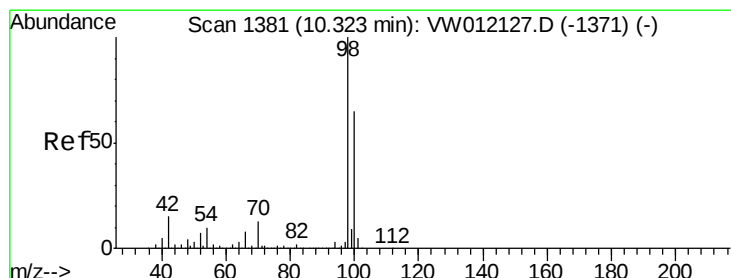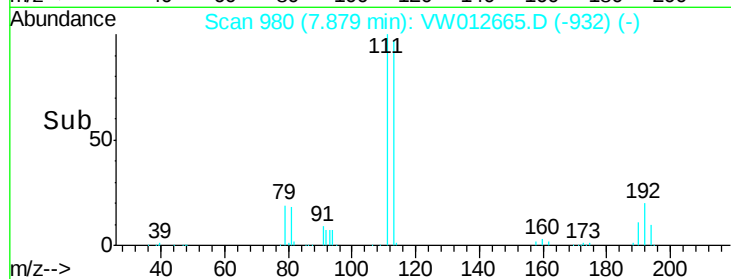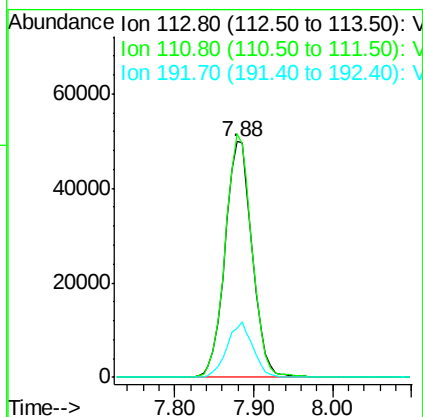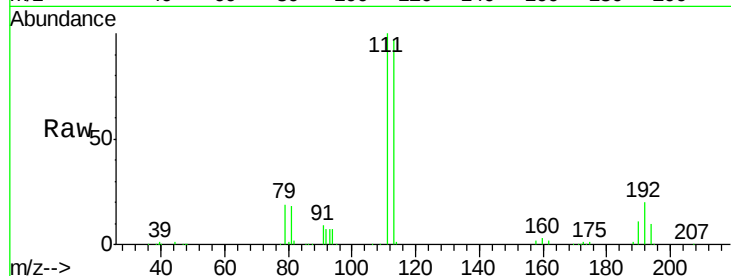

#50
 Toluene-d8
 Concen: 46.641 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. 0.00 min
 Lab File: VW012665.D
 Acq: 06 Sep 2019 02:39

Tgt Ion: 98 Resp: 466006
 Ion Ratio Lower Upper
 98 100
 100 64.9 52.4 78.6

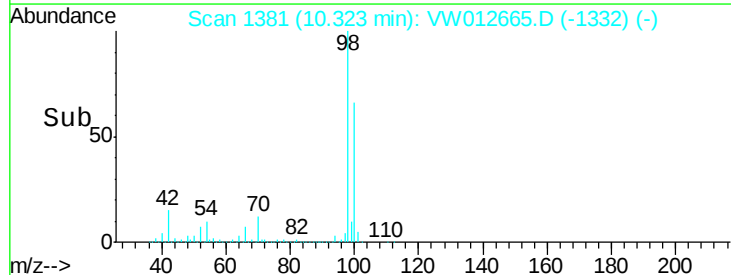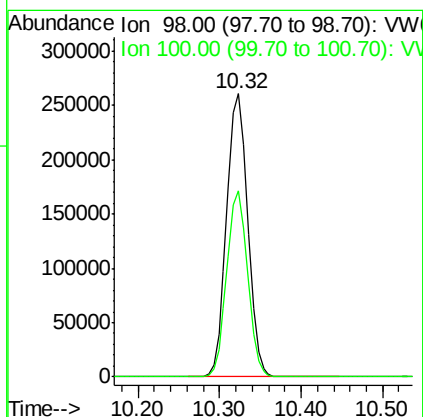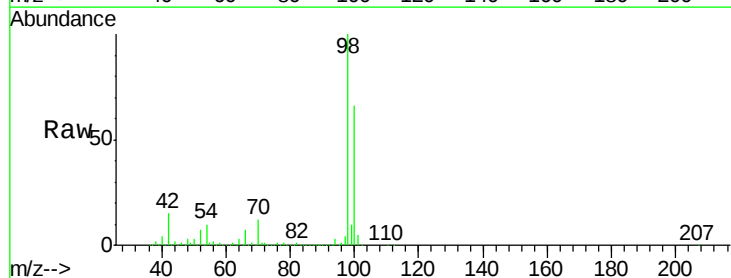

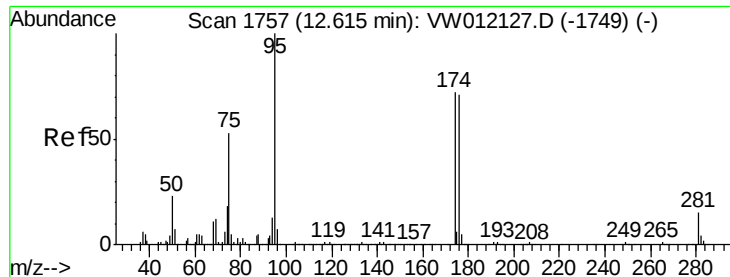

#62

4-Bromofluorobenzene

Concen: 40.742 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-B2-(0)


Tot Ion: 95 Resp: 143491

Ion Ratio Lower Upper

95 100

174 79.4 0.0 150.8




176 76.6 0.0 148.6

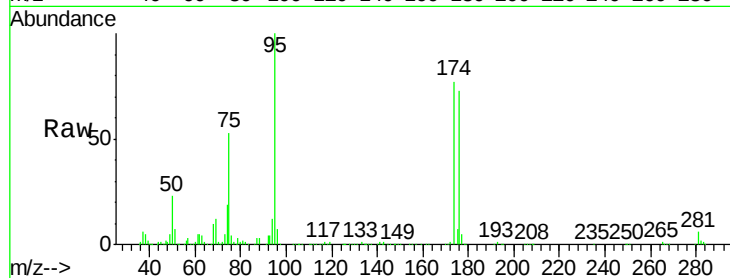

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

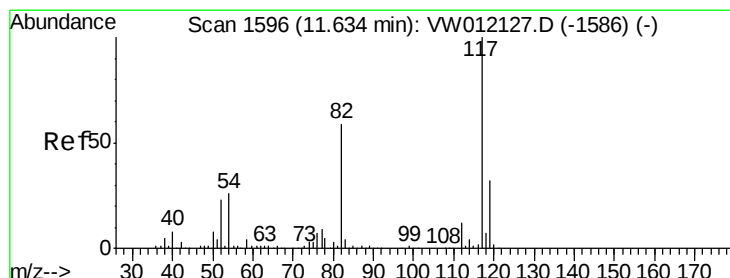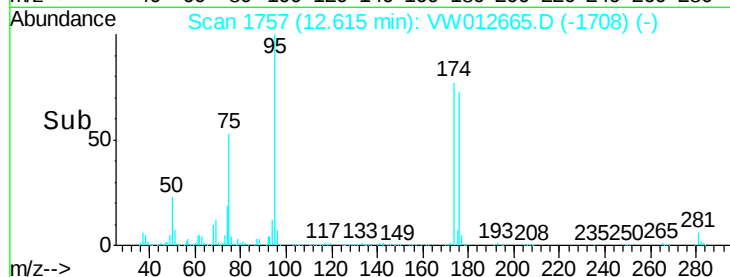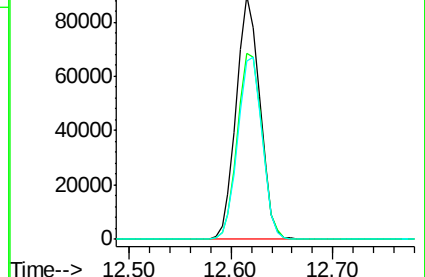

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1595

Delta R.T. -0.01 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39


Tgt Ion: 117 Resp: 335002

Ion Ratio Lower Upper

117 100

82 60.2 47.4 71.2



119 31.6 25.4 38.2

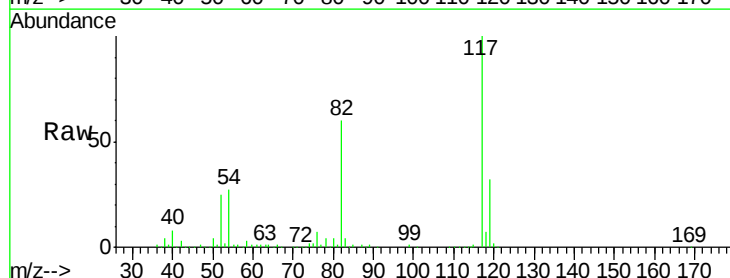


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

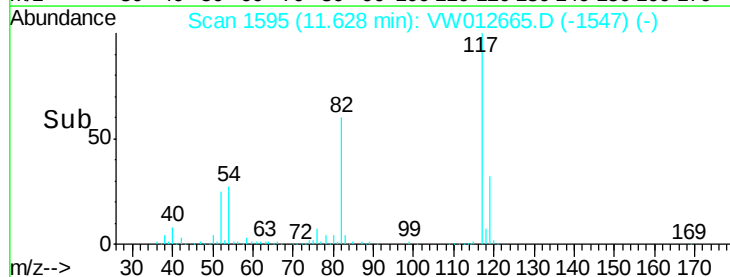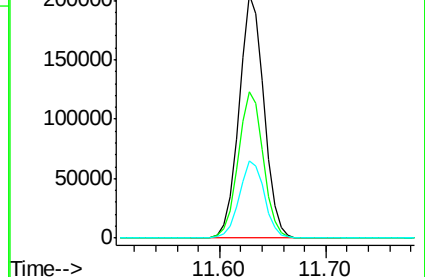

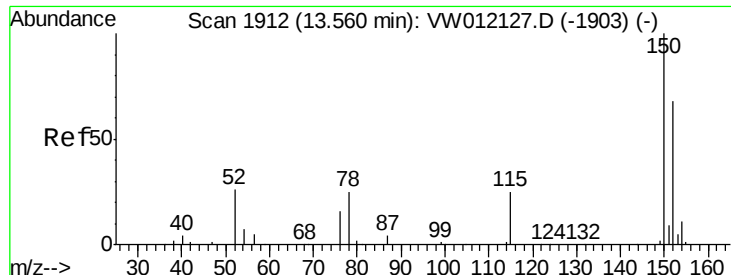

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.55 min Scan# 1911

Delta R.T. -0.01 min

Lab File: VW012665.D

Acq: 06 Sep 2019 02:39

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-B2-(0)


Tot Ion:152 Resp: 129824

Ion Ratio Lower Upper

152 100

115 59.8 30.1 90.3

150 158.6 0.0 345.8

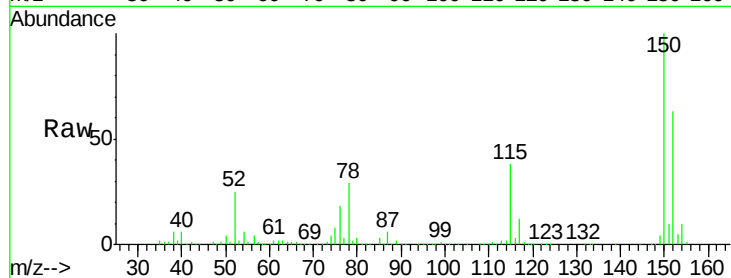

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

