
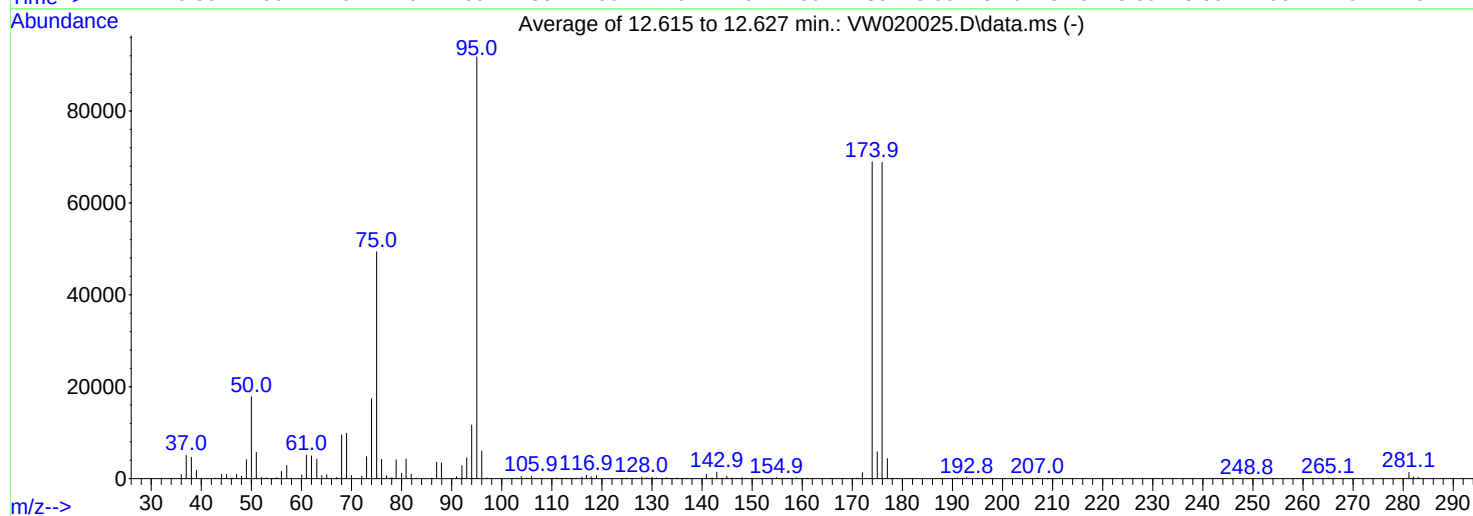


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091521\
 Data File : VW020025.D
 Acq On : 15 Sep 2021 08:28
 Operator : SY/VA
 Sample : BFB431
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB431

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Title : SFAM01.0
 Last Update : Thu Sep 16 00:47:26 2021

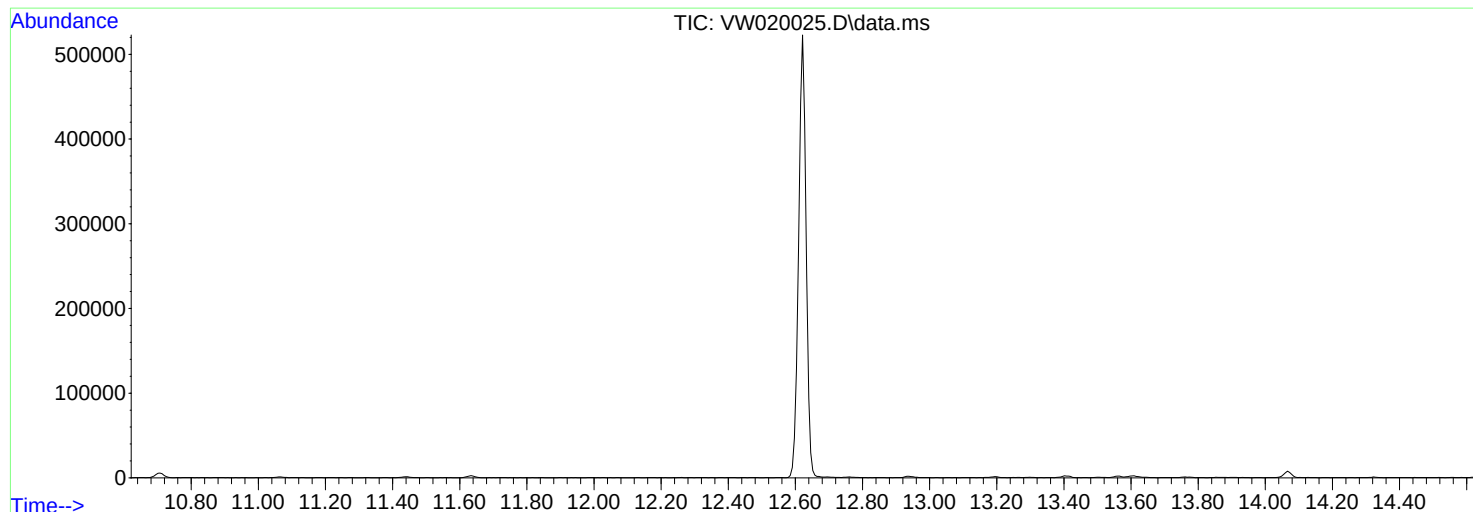

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	17815	PASS
75	95	30	80	53.8	49368	PASS
95	95	100	100	100.0	91781	PASS
96	95	5	9	6.5	5974	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	68952	PASS
175	174	5	9	8.5	5840	PASS
176	174	95	105	99.8	68795	PASS
177	176	5	10	6.3	4352	PASS