

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092920\
 Data File : VW016681.D
 Acq On : 29 Sep 2020 10:42
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 VBLK22

Manual Integrations
APPROVED

Sam
 10/1/2020 6:14:12 PM

Quant Time: Sep 30 09:11:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 30 07:14:58 2020
 Response via : Initial Calibration

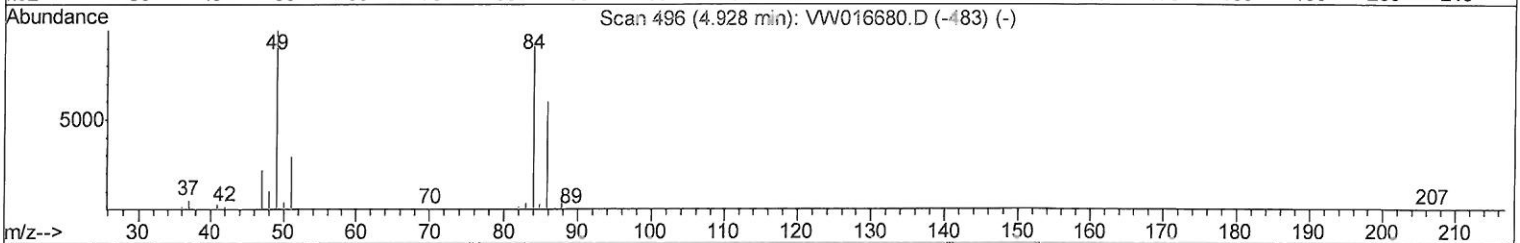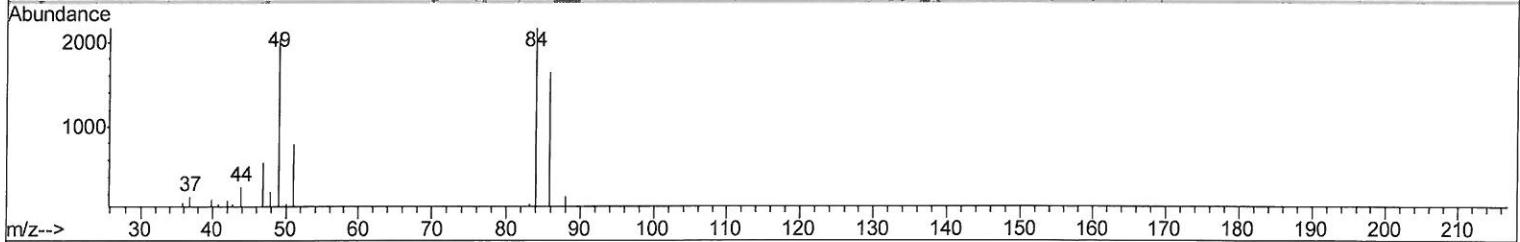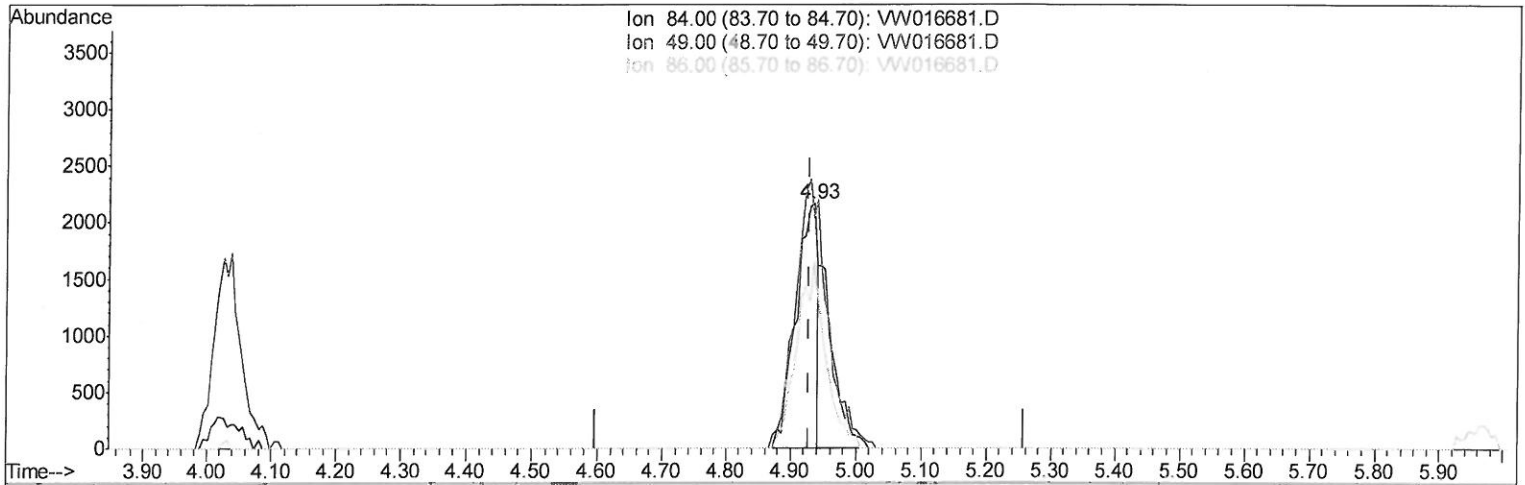

TIC: VW016681.D

(16) Methylene chloride (T)

4.934min (+0.006) 0.52ug/L

response 4927

Ion	Exp%	Act%
84.00	100	100
49.00	108.60	94.19
86.00	65.10	76.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092920\
 Data File : VW016681.D
 Acq On : 29 Sep 2020 10:42
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK22

Manual Integrations
 APPROVED

Sam
 10/1/2020 6:14:12 PM

Quant Time: Sep 30 09:11:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 30 07:14:58 2020
 Response via : Initial Calibration

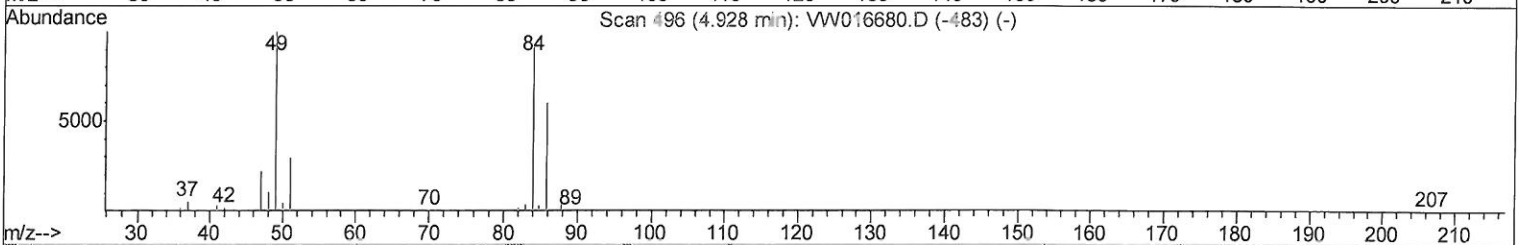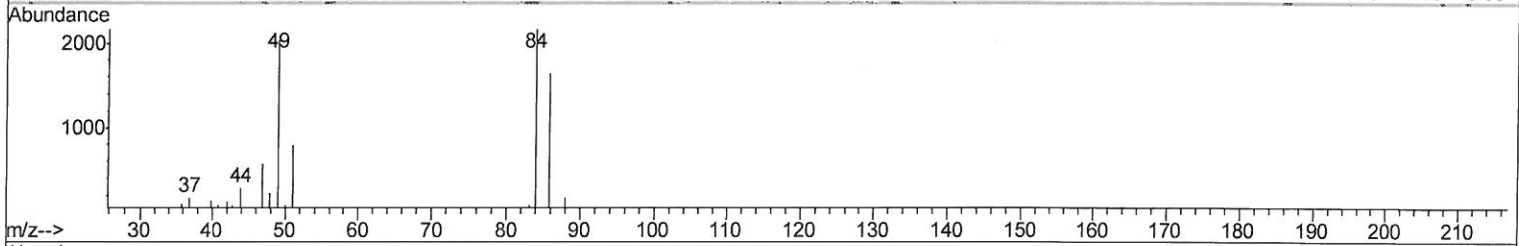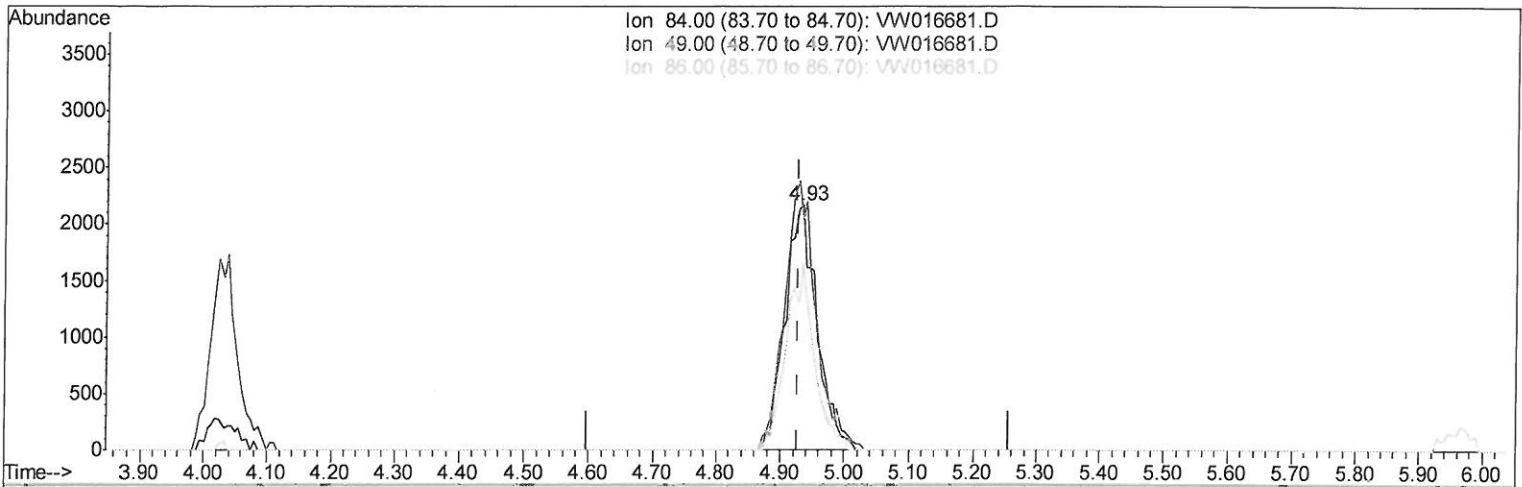

TIC: VW016681.D

(16) Methylene chloride (T)

4.934min (+0.006) 0.79ug/L m

> 16/16/2025

response 7492

Ion	Exp%	Act%
84.00	100	100
49.00	108.60	94.19
86.00	65.10	76.05
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092920\
 Data File : VW016681.D
 Acq On : 29 Sep 2020 10:42
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK22

Manual Integrations
 APPROVED

sam
 10/1/2020 6:14:12 PM

Quant Time: Sep 30 22:25:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 30 07:14:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	617696	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	539213	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	263048	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	98740	16.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.04%
7) Chloroethane-d5	2.90	69	92114	18.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.48%
10) 1,1-Dichloroethene-d2	4.03	63	168204	12.58	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.32%
20) 2-Butanone-d5	7.09	46	65111	39.94	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.88%
24) Chloroform-d	7.65	84	299138	23.15	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	8.31	65	150780	22.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.92%
29) Benzene-d6	8.28	84	529858	21.91	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.64%
33) 1,2-Dichloropropane-d6	9.28	67	155851	23.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.12%
37) Toluene-d8	10.33	98	481978	20.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.04%
38) trans-1,3-Dichloropropene-	10.59	79	67770	20.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.04%
39) 2-Hexanone-d5	10.93	63	53120	44.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.14%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128935	23.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	208508	24.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.24%

Target Compounds

16) Methylene chloride	4.93	84	7492m	0.786	ug/L	Ovalue
------------------------	------	----	-------	-------	------	--------

10/1/2020

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092920\
Data File : VW016681.D
Acq On : 29 Sep 2020 10:42
Operator : SY/VA
Sample : VW0929SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK22

Manual Integrations
APPROVED

sam
10/1/2020 6:14:12 PM

Quant Time: Sep 30 22:25:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 30 07:14:58 2020
Response via : Initial Calibration

