

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW092920\
 Data File : VW016692.D
 Acq On : 29 Sep 2020 17:27
 Operator : SY/VA
 Sample : L4184-03
 Misc : 5.60G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AK0

Quant Time: Sep 30 08:37:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 30 07:14:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	585163	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	514664	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	242545	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	109967	19.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.68%
7) Chloroethane-d5	2.90	69	100313	21.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.76%
10) 1,1-Dichloroethene-d2	4.03	63	187998	14.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.40%
20) 2-Butanone-d5	7.09	46	79517	51.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.98%
24) Chloroform-d	7.65	84	300210	24.52	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.08%
26) 1,2-Dichloroethane-d4	8.31	65	165113	26.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.12%
29) Benzene-d6	8.28	84	579569	25.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.44%
33) 1,2-Dichloropropane-d6	9.28	67	168336	26.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.64%
37) Toluene-d8	10.33	98	548656	24.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.64%
38) trans-1,3-Dichloropropene-	10.58	79	73124	23.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.76%
39) 2-Hexanone-d5	10.93	63	63190	55.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.08%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	144733	27.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	202481	26.13	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.52%


Target Compounds					Ovalue
13) Acetone	4.14	43	7887	6.520 ug/L	82
16) Methylene chloride	4.93	84	9819	1.088 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW092920\
Data File : VW016692.D
Acq On : 29 Sep 2020 17:27
Operator : SY/VA
Sample : L4184-03
Misc : 5.60G/10ML/MSVOA W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AK0

Quant Time: Sep 30 08:37:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 30 07:14:58 2020
Response via : Initial Calibration

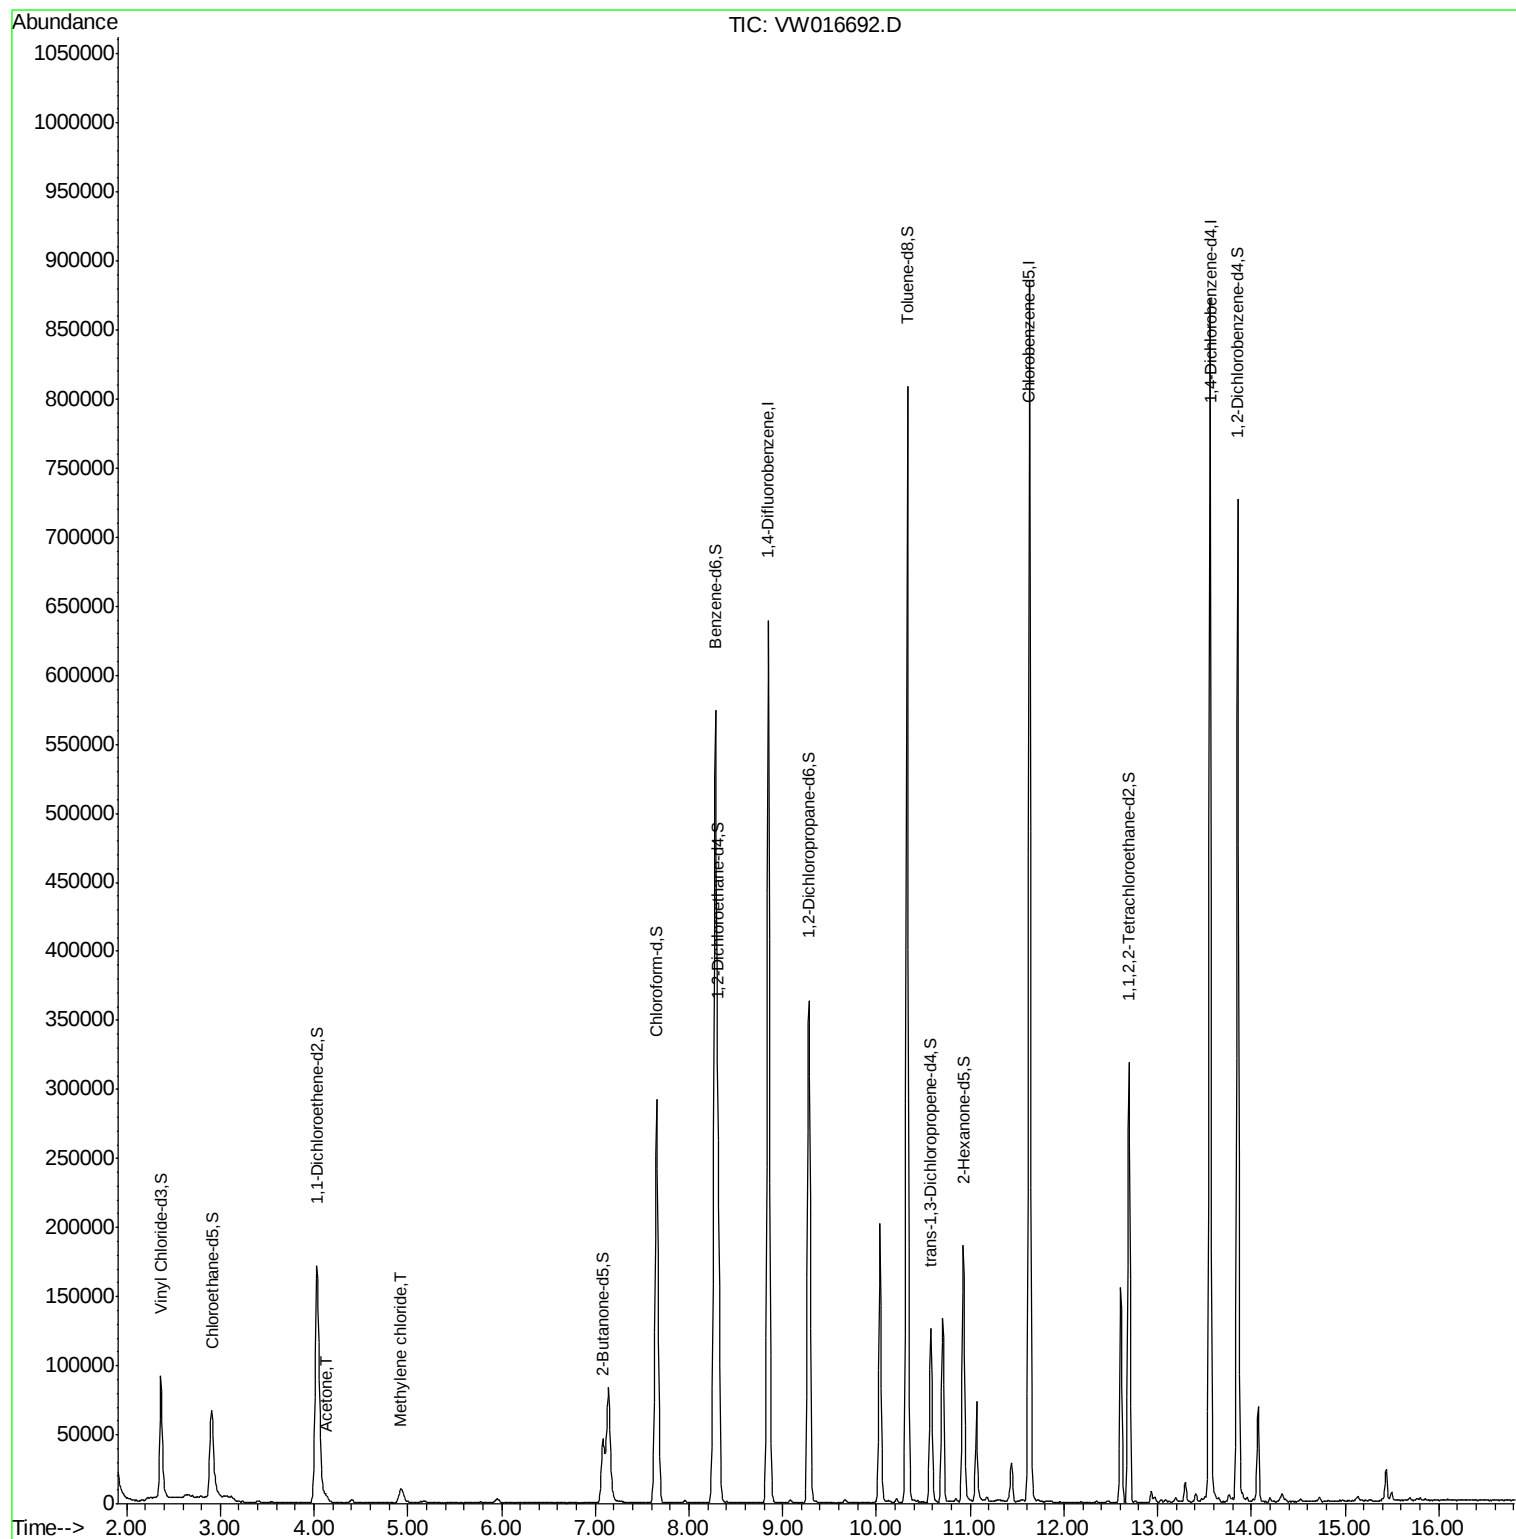

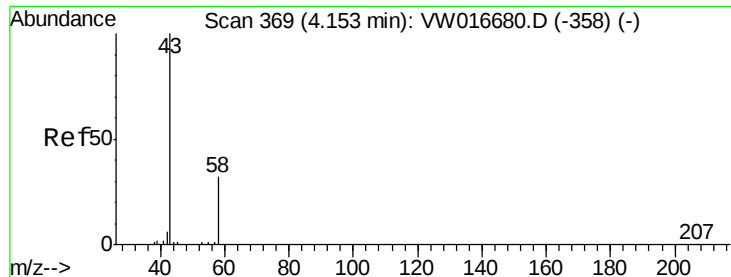

#13

Acetone

Concen: 6.520 ug/L

RT: 4.14 min Scan# 366

Delta R.T. -0.02 min

Lab File: VW016692.D

Acq: 29 Sep 2020 17:27

Instrument :

MSVOA_W

ClientSampleId :


C0AK0

Tot Ion: 43 Resp: 7887

Ion Ratio Lower Upper




43 100

58 20.4 0.0 60.2

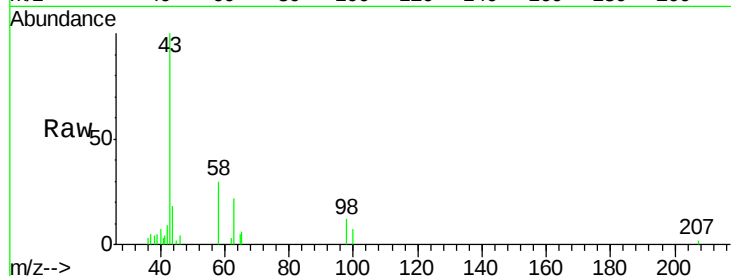

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

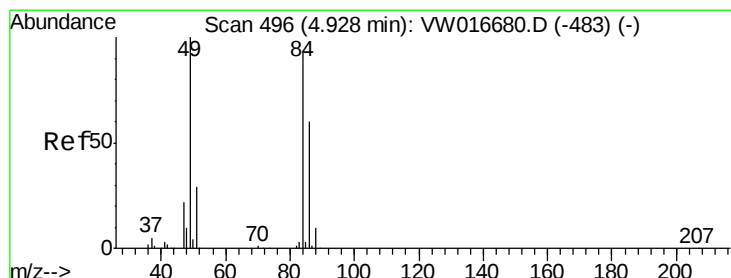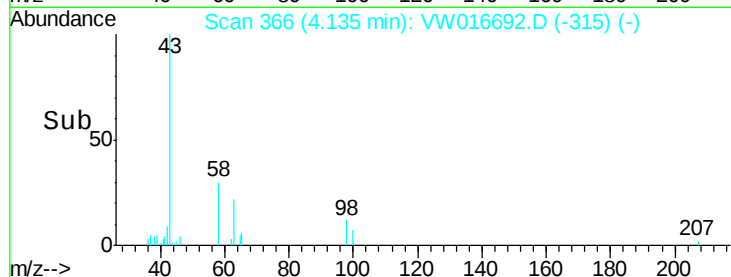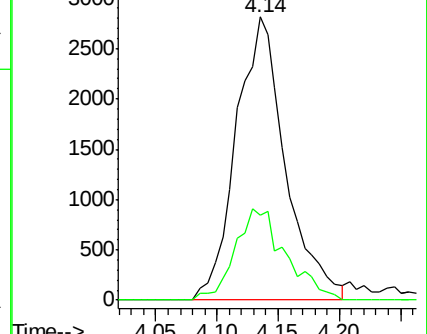

#16

Methylene chloride

Concen: 1.088 ug/L

RT: 4.93 min Scan# 496

Delta R.T. 0.00 min

Lab File: VW016692.D

Acq: 29 Sep 2020 17:27


Tgt Ion: 84 Resp: 9819

Ion Ratio Lower Upper

84 100

49 115.3 76.0 141.2

86 62.6 45.6 84.6

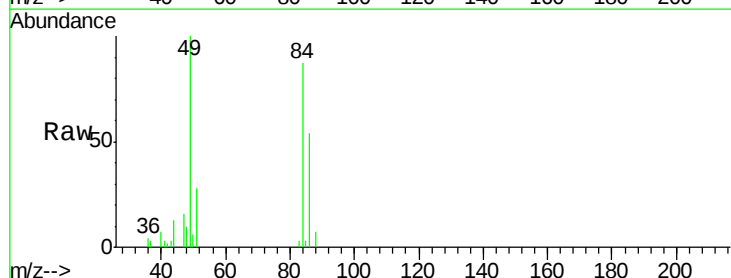

Abundance Ion 84.00 (83.70 to 84.70): VW

Ion 49.00 (48.70 to 49.70): VW

Ion 86.00 (85.70 to 86.70): VW

