


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW101320\  
Data File : VW016880.D  
Acq On : 12 Oct 2020 14:10  
Operator : SY/VA  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W101020S.M  
Title : SW846 8260  
Last Update : Sat Oct 10 05:14:48 2020

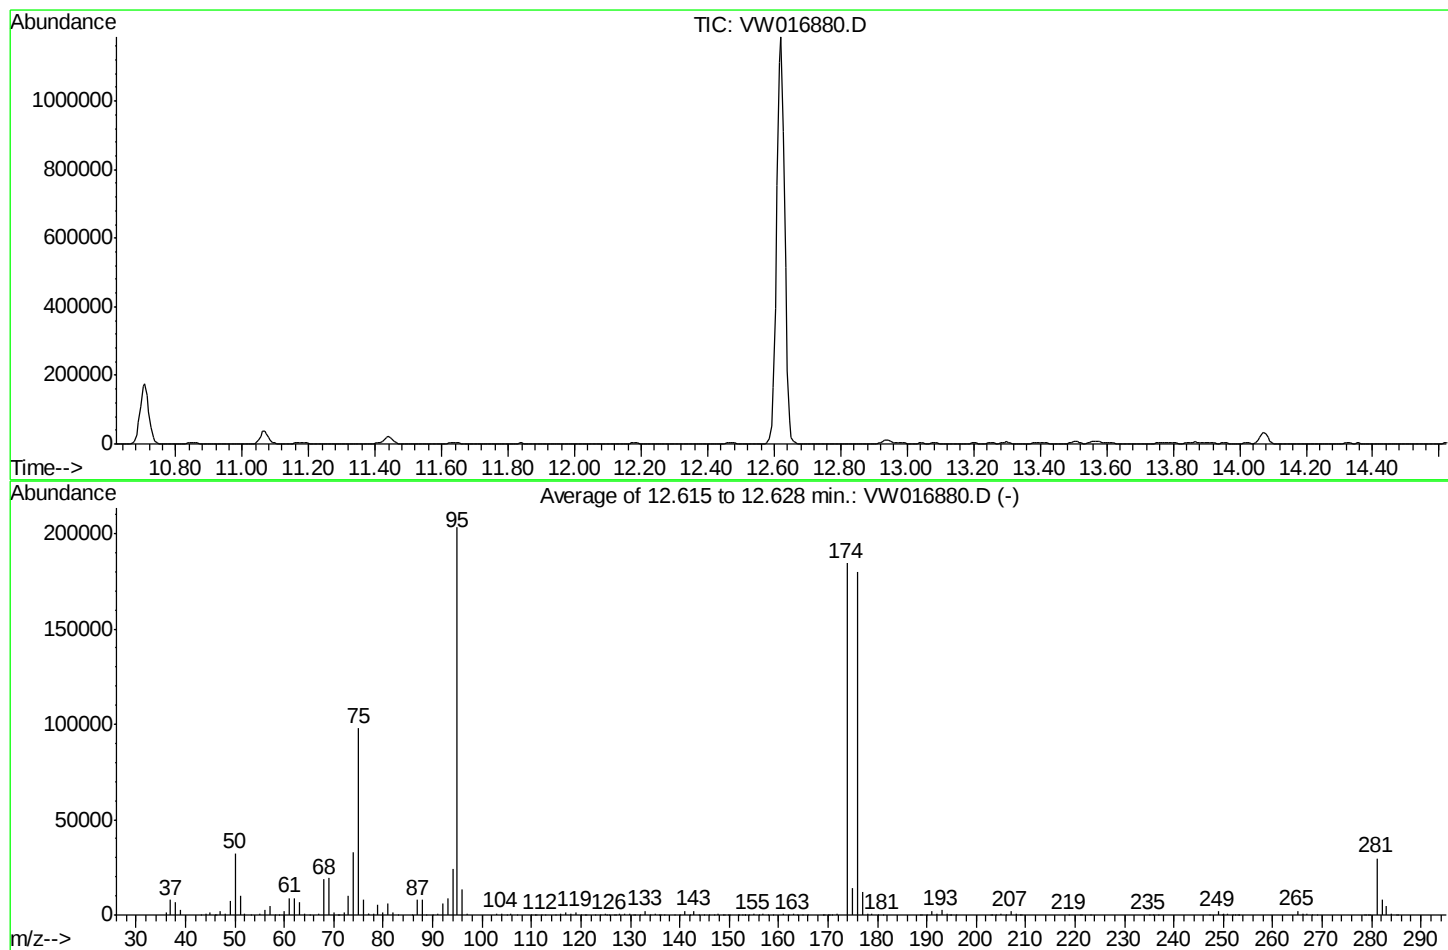

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.8      | 32082   | PASS             |
| 75          | 95           | 30           | 60           | 48.1      | 97754   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 203306  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 13169   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 184341  | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 13985   | PASS             |
| 176         | 174          | 95           | 101          | 97.7      | 180053  | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 12379   | PASS             |