

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
 Data File : VW020460.D
 Acq On : 13 Oct 2021 15:02
 Operator : SY/VA
 Sample : M4181-02
 Misc : 3.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0

Signal : TIC: VW020460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.904	158	164	172	rBV2	1807	3415	16.72%	3.146%
2	3.007	180	181	182	rBV	160	74	0.36%	0.068%
3	3.105	195	197	198	rBV	83	64	0.31%	0.059%
4	3.282	224	226	228	rVB2	99	80	0.39%	0.074%
5	3.306	228	230	232	rBV	124	129	0.63%	0.119%
6	3.385	241	243	247	rBV2	78	85	0.42%	0.078%
7	3.568	270	273	275	rVB	84	86	0.42%	0.079%
8	3.593	275	277	278	rBV	90	72	0.35%	0.066%
9	3.757	303	304	306	rBV2	71	49	0.24%	0.045%
10	3.794	308	310	311	rVB2	94	60	0.29%	0.055%
11	3.855	316	320	324	rBV2	76	132	0.65%	0.122%
12	3.922	330	331	334	rBV	89	105	0.51%	0.097%
13	3.971	338	339	341	rVV2	112	92	0.45%	0.085%
14	4.038	342	350	358	rVV2	3057	7827	38.33%	7.211%
15	4.117	362	363	366	rVB2	105	78	0.38%	0.072%
16	4.154	366	369	371	rBV2	97	133	0.65%	0.123%
17	4.184	373	374	376	rBV	115	86	0.42%	0.079%
18	4.233	379	382	383	rBV	79	76	0.37%	0.070%
19	4.275	385	389	392	rVB	95	91	0.45%	0.084%
20	4.318	393	396	399	rBV2	84	116	0.57%	0.107%
21	4.397	407	409	413	rBV	103	119	0.58%	0.110%
22	4.489	422	424	428	rBV2	108	111	0.54%	0.102%
23	4.538	430	432	435	rVB2	105	114	0.56%	0.105%
24	4.568	435	437	439	rBV2	66	70	0.34%	0.064%
25	4.623	441	446	447	rBV2	74	95	0.47%	0.088%
26	4.684	453	456	457	rBV	111	103	0.50%	0.095%
27	4.721	460	462	463	rBV	117	59	0.29%	0.054%
28	4.970	501	503	506	rBV2	87	95	0.47%	0.088%
29	5.288	553	555	556	rBV	82	60	0.29%	0.055%
30	5.757	631	632	635	rBV	147	153	0.75%	0.141%
31	5.824	641	643	644	rBV	103	60	0.29%	0.055%
32	5.861	647	649	653	rBV2	76	110	0.54%	0.101%
33	5.958	664	665	669	rBV	113	99	0.48%	0.091%
34	6.226	707	709	712	rVB2	92	81	0.40%	0.075%
35	6.257	712	714	715	rBV	103	63	0.31%	0.058%
36	6.293	718	720	722	rBV2	132	138	0.68%	0.127%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
 Data File : VW020460.D
 Acq On : 13 Oct 2021 15:02
 Operator : SY/VA
 Sample : M4181-02
 Misc : 3.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0

37	6.367	728	732	733	rBV2	89	98	0.48%	0.090%
38	6.415	739	740	742	rVB	91	57	0.28%	0.053%
39	6.519	755	757	758	rBV	97	88	0.43%	0.081%
40	6.964	828	830	833	rVV2	99	89	0.44%	0.082%
41	7.013	836	838	841	rBV2	91	82	0.40%	0.076%
42	7.244	874	876	878	rBV	131	66	0.32%	0.061%
43	7.348	889	893	895	rBV2	158	218	1.07%	0.201%
44	7.470	912	913	915	rBV2	130	76	0.37%	0.070%
45	7.507	918	919	920	rBV	91	56	0.27%	0.052%
46	7.659	935	944	952	rVB	3852	9698	47.49%	8.935%
47	7.824	968	971	972	rBV	159	136	0.67%	0.125%
48	8.110	1014	1018	1019	rVV	110	139	0.68%	0.128%
49	8.159	1022	1026	1028	rVB2	83	97	0.48%	0.089%
50	8.281	1039	1046	1055	rBV4	7235	20420	100.00%	18.813%
51	8.653	1105	1107	1108	rVB	116	58	0.28%	0.053%
52	8.848	1132	1139	1149	rBV	5721	10922	53.49%	10.062%
53	8.951	1154	1156	1157	rBV	81	66	0.32%	0.061%
54	9.055	1171	1173	1176	rVB2	101	115	0.56%	0.106%
55	9.147	1186	1188	1191	rVB	90	79	0.39%	0.073%
56	9.232	1200	1202	1203	rBV	78	76	0.37%	0.070%
57	9.281	1203	1210	1216	rVB2	4885	9345	45.76%	8.609%
58	9.397	1227	1229	1231	rVB2	94	59	0.29%	0.054%
59	9.421	1231	1233	1236	rBV	97	96	0.47%	0.088%
60	9.500	1244	1246	1248	rBV	91	79	0.39%	0.073%
61	9.628	1263	1267	1269	rBV2	117	130	0.64%	0.120%
62	9.768	1288	1290	1291	rVB	110	61	0.30%	0.056%
63	9.823	1297	1299	1300	rBV2	82	71	0.35%	0.065%
64	10.037	1330	1334	1341	rVB2	1568	2704	13.24%	2.491%
65	10.146	1350	1352	1354	rBV	168	122	0.60%	0.112%
66	10.195	1359	1360	1361	rBV	123	58	0.28%	0.053%
67	10.323	1375	1381	1389	rVB	6900	11964	58.59%	11.022%
68	10.457	1401	1403	1404	rBV2	83	63	0.31%	0.058%
69	10.469	1404	1405	1406	rVV	147	60	0.29%	0.055%
70	10.579	1419	1423	1428	rBV2	967	1353	6.63%	1.247%
71	10.652	1434	1435	1437	rBV	90	92	0.45%	0.085%
72	10.762	1451	1453	1454	rVB2	183	113	0.55%	0.104%
73	10.890	1472	1474	1475	rBV	88	49	0.24%	0.045%
74	10.927	1476	1480	1490	rVB3	415	865	4.24%	0.797%
75	11.000	1490	1492	1494	rBV	86	69	0.34%	0.064%
76	11.128	1511	1513	1515	rBV2	78	86	0.42%	0.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
 Data File : VW020460.D
 Acq On : 13 Oct 2021 15:02
 Operator : SY/VA
 Sample : M4181-02
 Misc : 3.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0

77	11.177	1519	1521	1522	rBV	91	52	0.25%	0.048%
78	11.305	1540	1542	1544	rVB2	97	90	0.44%	0.083%
79	11.421	1559	1561	1562	rVB	135	61	0.30%	0.056%
80	11.439	1562	1564	1565	rBV2	67	61	0.30%	0.056%
81	11.457	1565	1567	1569	rVV	130	113	0.55%	0.104%
82	11.634	1590	1596	1602	rBV	6454	10547	51.65%	9.717%
83	11.750	1614	1615	1616	rBV	149	66	0.32%	0.061%
84	12.122	1674	1676	1677	rBV	101	64	0.31%	0.059%
85	12.268	1698	1700	1701	rBV	102	59	0.29%	0.054%
86	12.439	1726	1728	1731	rBV2	91	117	0.57%	0.108%
87	12.689	1765	1769	1774	rVB	2288	3116	15.26%	2.871%
88	12.737	1774	1777	1778	rBV2	96	82	0.40%	0.076%
89	12.817	1788	1790	1794	rVB2	94	98	0.48%	0.090%
90	12.853	1794	1796	1799	rBV2	72	88	0.43%	0.081%
91	12.963	1812	1814	1816	rVB	177	100	0.49%	0.092%
92	12.993	1816	1819	1822	rBV2	114	207	1.01%	0.191%
93	13.329	1872	1874	1875	rBV2	134	74	0.36%	0.068%
94	13.524	1904	1906	1907	rVB2	149	83	0.41%	0.076%
95	13.560	1907	1912	1916	rBV	3079	4769	23.35%	4.394%
96	13.853	1956	1960	1965	rVB	2673	3779	18.51%	3.482%
97	13.975	1978	1980	1982	rBV2	147	149	0.73%	0.137%
98	13.999	1982	1984	1986	rVV	136	93	0.46%	0.086%
99	14.188	2013	2015	2019	rVB	122	107	0.52%	0.099%
100	14.463	2058	2060	2061	rBV	172	113	0.55%	0.104%




Sum of corrected areas: 108543

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
Data File : VW020460.D
Acq On : 13 Oct 2021 15:02
Operator : SY/VA
Sample : M4181-02
Misc : 3.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

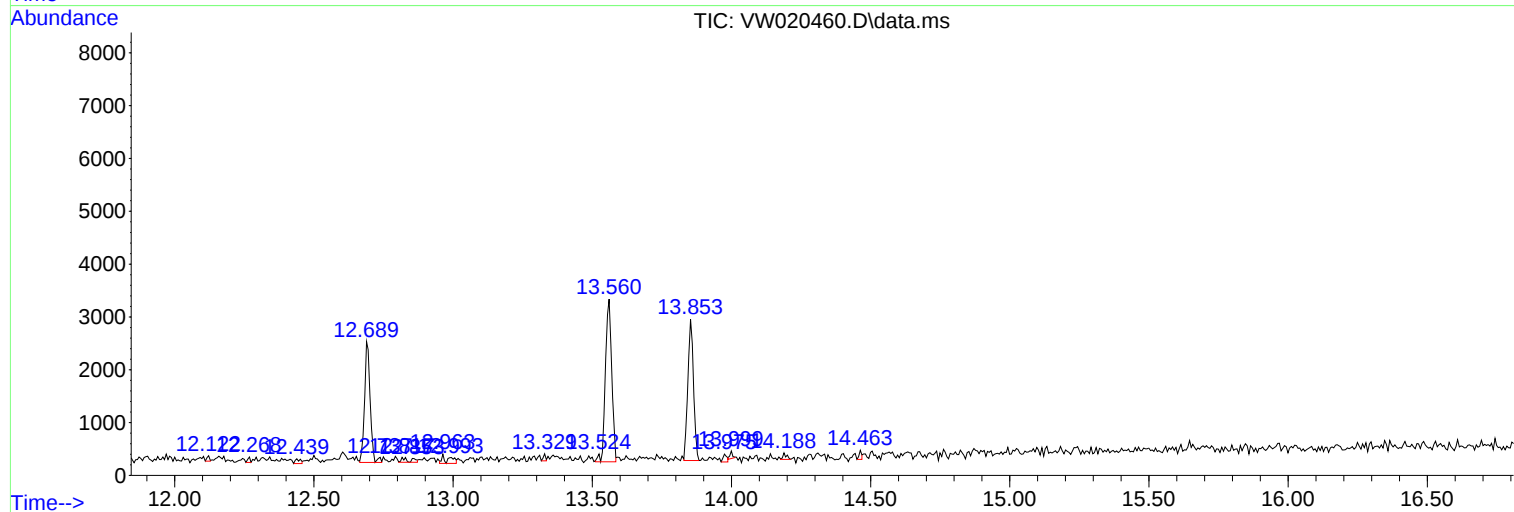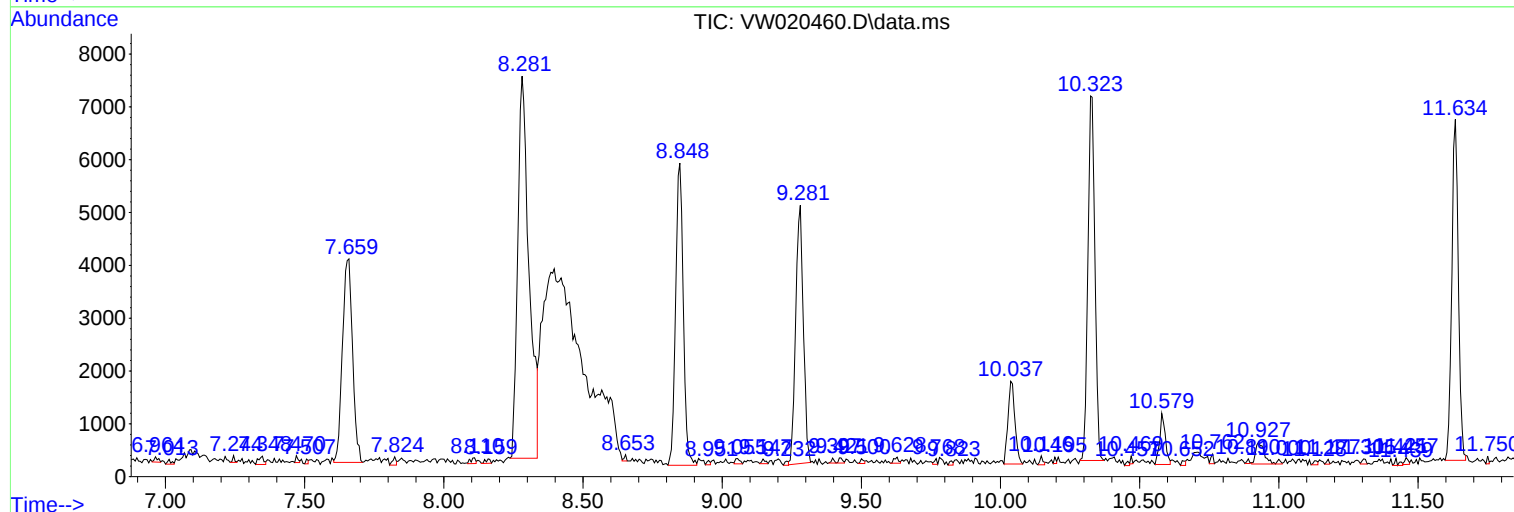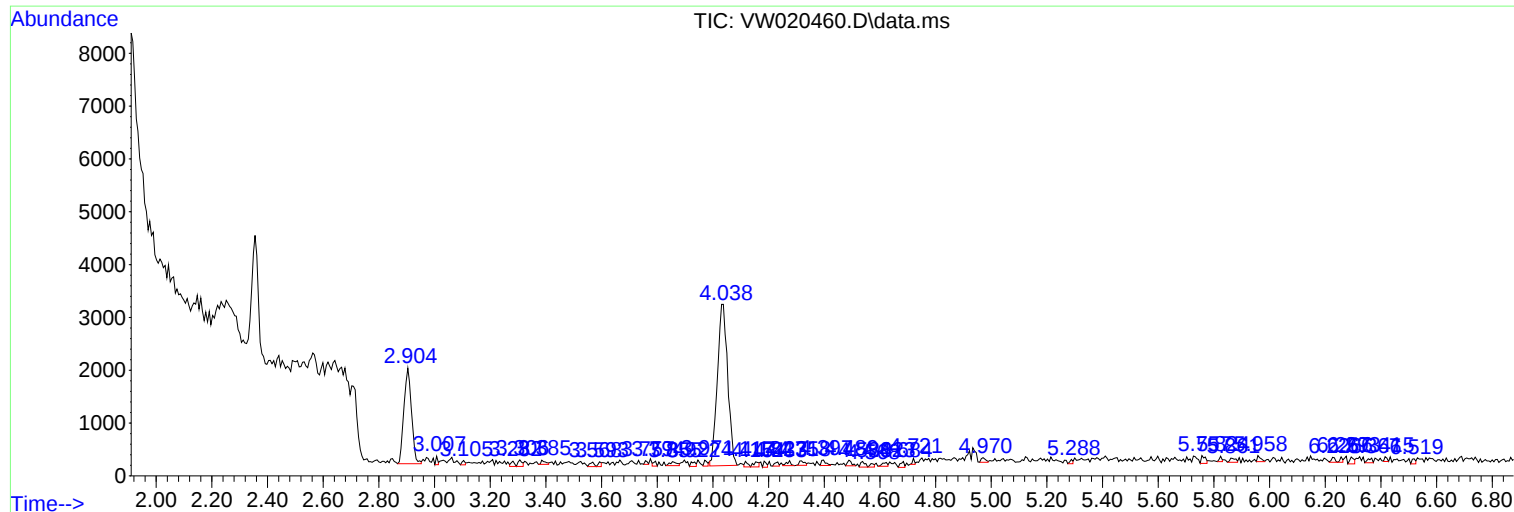

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
Data File : VW020460.D
Acq On : 13 Oct 2021 15:02
Operator : SY/VA
Sample : M4181-02
Misc : 3.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
Data File : VW020460.D
Acq On : 13 Oct 2021 15:02
Operator : SY/VA
Sample : M4181-02
Misc : 3.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
