
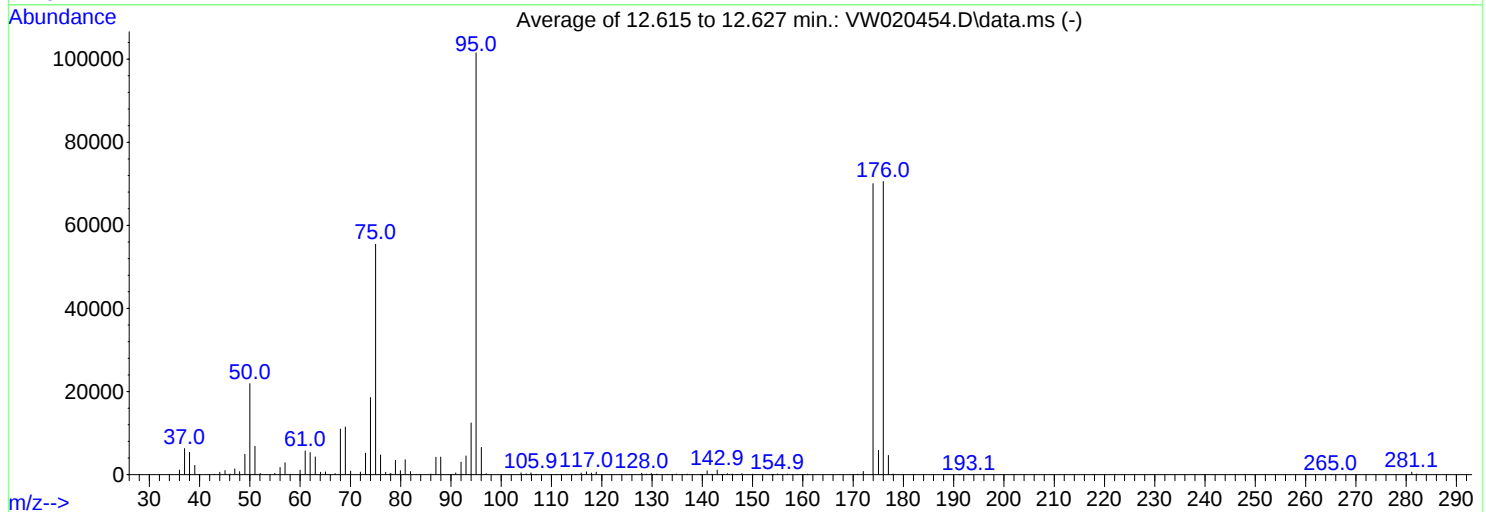


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101321\
 Data File : VW020454.D
 Acq On : 13 Oct 2021 11:13
 Operator : SY/VA
 Sample : BFB451
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB451

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Sat Oct 16 06:56:08 2021

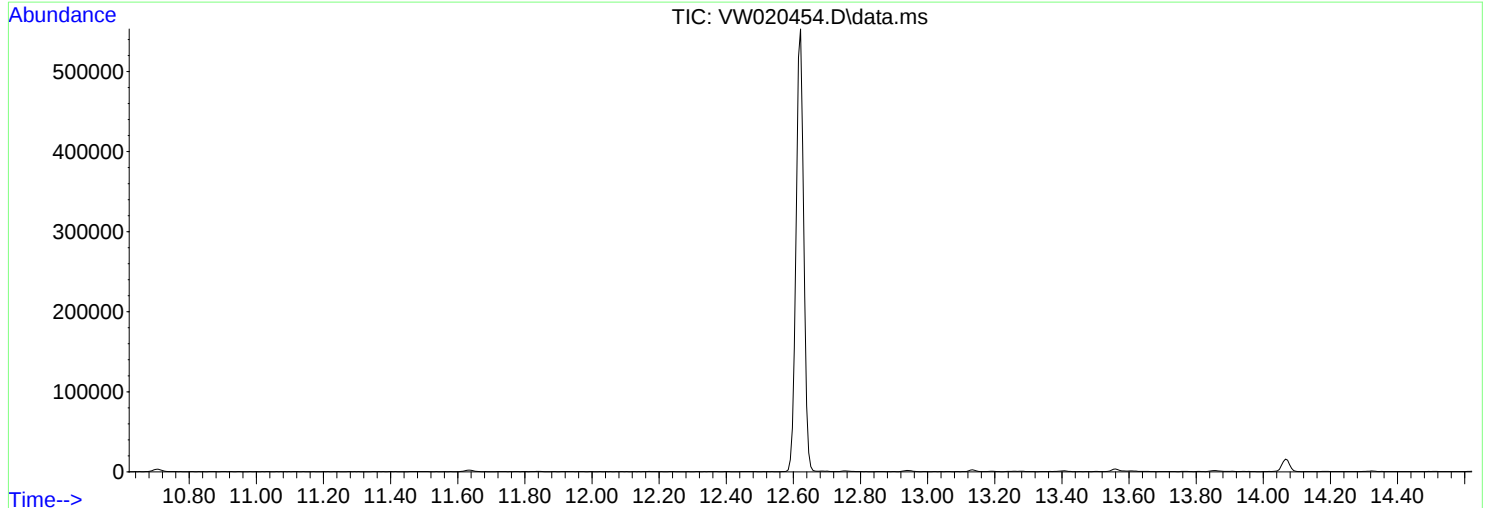

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	21923	PASS
75	95	30	80	54.6	55451	PASS
95	95	100	100	100.0	101523	PASS
96	95	5	9	6.5	6567	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.0	70048	PASS
175	174	5	9	8.3	5847	PASS
176	174	95	105	100.7	70560	PASS
177	176	5	10	6.6	4635	PASS

Scan 1749 (12.566 min): VW020454.D\data.ms
BFB451

m/z	Abundance
39.90	118.0
44.00	213.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451

m/z	Abundance
36.00	1279.0
37.00	6921.0
38.00	6018.0
39.10	2613.0
40.00	229.0
43.00	94.0
44.00	799.0
45.00	1110.0
46.10	158.0
47.00	1598.0
48.00	831.0
49.00	5528.0
50.00	24624.0
51.00	7714.0
52.00	306.0
53.10	98.0
54.90	350.0
56.00	1805.0
57.00	3191.0
58.10	134.0
60.00	1314.0
61.00	6125.0
62.00	5831.0
63.00	4716.0
64.00	691.0
65.10	856.0
65.90	71.0
67.00	289.0
68.00	11891.0
69.00	12512.0
70.00	901.0
72.00	639.0
73.00	5628.0
74.00	20392.0
75.00	59720.0
76.00	5283.0
77.00	700.0
78.10	465.0
79.00	3793.0
80.00	1010.0
80.90	4013.0
81.90	805.0
83.00	101.0
86.10	206.0
87.00	4314.0
88.00	4544.0
90.90	509.0
92.00	3238.0
93.00	4622.0
94.00	13302.0
95.00	106576.0
96.00	6937.0
97.00	245.0
103.90	473.0
104.90	189.0
105.90	457.0
106.80	108.0
109.70	78.0
110.90	94.0
111.90	61.0
113.00	111.0
114.80	98.0
115.90	361.0
116.90	685.0
117.90	382.0
118.90	693.0
125.00	77.0
127.90	376.0
128.90	145.0
129.80	311.0
130.90	121.0
133.00	99.0
134.80	211.0
137.10	118.0
139.90	91.0
141.00	965.0
142.00	150.0
143.00	1239.0
143.90	74.0
144.10	72.0
145.00	276.0
146.00	158.0
147.00	78.0
147.90	204.0
148.90	75.0
150.00	113.0
151.90	85.0
153.80	56.0
154.90	214.0
157.00	170.0
158.90	68.0
160.80	115.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451

170.80	157.0
172.00	790.0
174.00	69928.0
175.00	5687.0
176.00	67976.0
177.00	4257.0
177.90	140.0
191.10	67.0
193.10	92.0
265.00	52.0
281.10	918.0
282.20	149.0
283.10	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451

m/z	Abundance
36.00	1259.0
37.00	6847.0
38.00	5851.0
39.00	2521.0
40.00	148.0
42.90	96.0
44.00	913.0
45.10	1076.0
46.10	194.0
47.00	1618.0
47.90	764.0
49.00	5439.0
50.00	24464.0
51.00	7584.0
52.10	346.0
55.00	366.0
56.00	1994.0
57.00	3265.0
58.00	138.0
60.00	1076.0
61.00	6464.0
62.00	6122.0
63.00	4703.0
64.10	652.0
65.00	671.0
66.00	67.0
67.00	293.0
68.00	12422.0
69.00	13109.0
70.10	1023.0
72.00	715.0
73.00	5760.0
74.00	20040.0
75.00	62656.0
76.00	5322.0
77.00	617.0
77.80	430.0
78.90	3832.0
80.00	1113.0
80.90	3890.0
81.90	751.0
83.10	136.0
86.00	112.0
87.00	4752.0
88.00	4670.0
90.90	418.0
92.00	3350.0
93.00	5146.0
94.00	14094.0
95.00	114544.0
96.10	7343.0
97.00	272.0
103.90	515.0
105.00	177.0
105.90	468.0
107.00	136.0
109.80	72.0
111.00	94.0
111.90	55.0
112.90	75.0
114.80	118.0
115.90	441.0
117.00	831.0
118.00	455.0
118.90	694.0
124.90	58.0
128.00	413.0
128.90	174.0
129.90	391.0
131.00	169.0
133.00	81.0
134.90	192.0
137.00	204.0
139.80	71.0
141.00	1014.0
141.90	124.0
142.90	1118.0
143.90	90.0
145.00	258.0
145.90	172.0
146.80	67.0
147.90	294.0
148.90	78.0
150.00	160.0
151.90	54.0
154.00	59.0
154.90	212.0
156.90	164.0
159.00	93.0
160.90	151.0
170.90	112.0
172.00	834.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451

174.00	76584.0
175.10	6584.0
176.00	80880.0
177.00	5616.0
177.90	159.0
192.90	53.0
281.10	562.0
282.00	208.0
283.00	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451

m/z	Abundance
36.00	776.0
37.00	5031.0
38.00	4172.0
39.10	1563.0
39.90	200.0
44.00	721.0
45.00	847.0
45.90	65.0
47.00	987.0
48.00	619.0
49.00	3718.0
50.00	16680.0
51.00	5152.0
52.00	190.0
55.00	218.0
56.00	1371.0
57.00	2274.0
58.00	127.0
60.00	855.0
61.00	4521.0
62.00	4008.0
63.00	3454.0
64.00	409.0
65.00	433.0
66.90	226.0
68.00	8571.0
69.00	8807.0
70.10	571.0
72.00	513.0
73.00	4108.0
74.00	15257.0
75.00	43976.0
76.00	3659.0
77.00	463.0
78.00	434.0
78.90	2676.0
79.90	815.0
80.90	2871.0
82.00	654.0
83.00	61.0
85.90	115.0
87.00	3502.0
87.90	3509.0
91.00	326.0
92.00	2376.0
93.00	3755.0
94.00	9969.0
95.00	83448.0
96.00	5420.0
97.00	162.0
104.00	352.0
105.00	161.0
105.90	317.0
107.00	106.0
110.90	100.0
113.00	68.0
115.00	99.0
115.90	311.0
116.90	562.0
117.90	304.0
118.90	449.0
127.90	257.0
128.90	143.0
129.90	270.0
130.90	169.0
134.80	119.0
136.80	164.0
139.60	51.0
140.90	789.0
141.80	96.0
142.90	985.0
145.10	127.0
146.00	127.0
147.90	190.0
149.90	91.0
155.00	183.0
156.90	187.0
159.00	67.0
161.00	109.0
171.00	111.0
172.00	675.0
173.90	63632.0
175.00	5271.0
176.00	62824.0
177.00	4031.0
178.00	144.0
281.10	321.0
282.00	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB451