

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101620\
 Data File : VW016914.D
 Acq On : 15 Oct 2020 16:09
 Operator : SY/VA
 Sample : L4421-18
 Misc : 5.55G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG1A4

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 11:00:16 AM

Quant Time: Oct 16 08:15:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 16 08:07:29 2020
 Response via : Initial Calibration

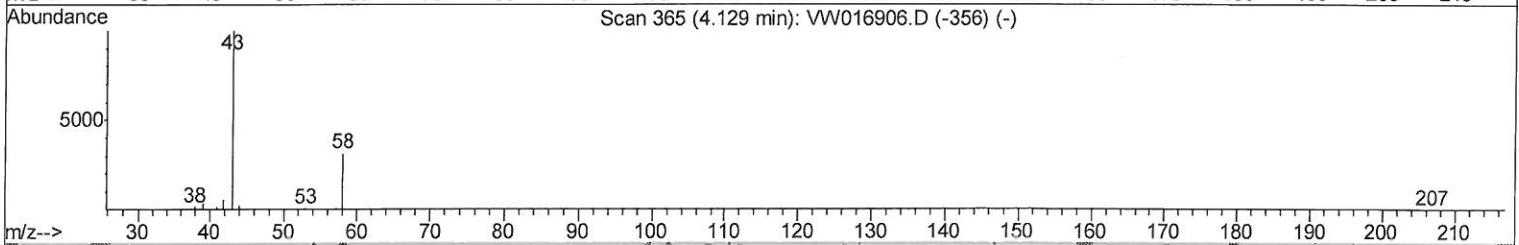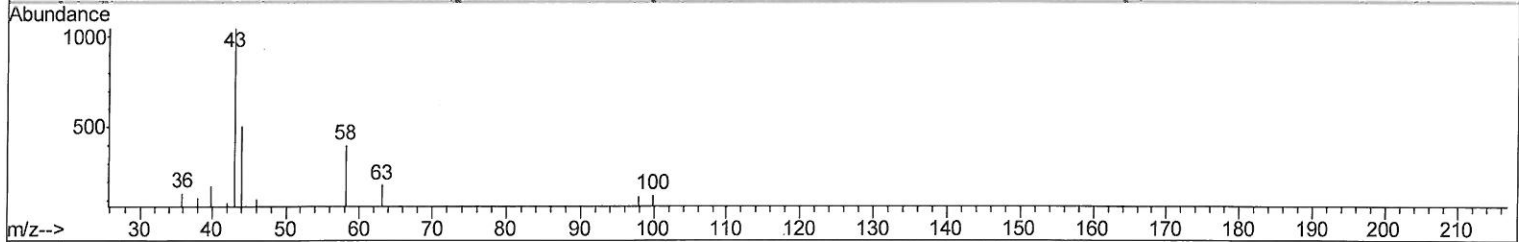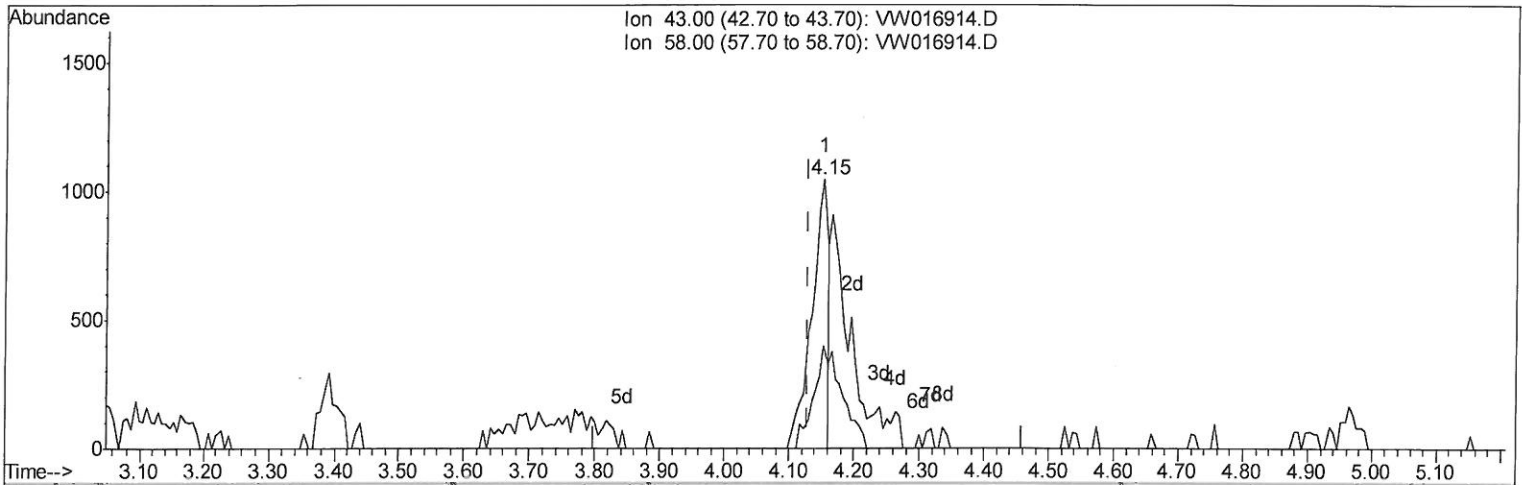

TIC: VW016914.D

(13) Acetone (T)

4.153min (+0.024) 1.86ug/L

response 1846

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	62.51
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101620\
 Data File : VW016914.D
 Acq On : 15 Oct 2020 16:09
 Operator : SY/VA
 Sample : L4421-18
 Misc : 5.55G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BG1A4

Manual Integrations
APPROVED

MMDadoda
 10/19/2020 11:00:16 AM

Quant Time: Oct 16 08:15:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 16 08:07:29 2020
 Response via : Initial Calibration

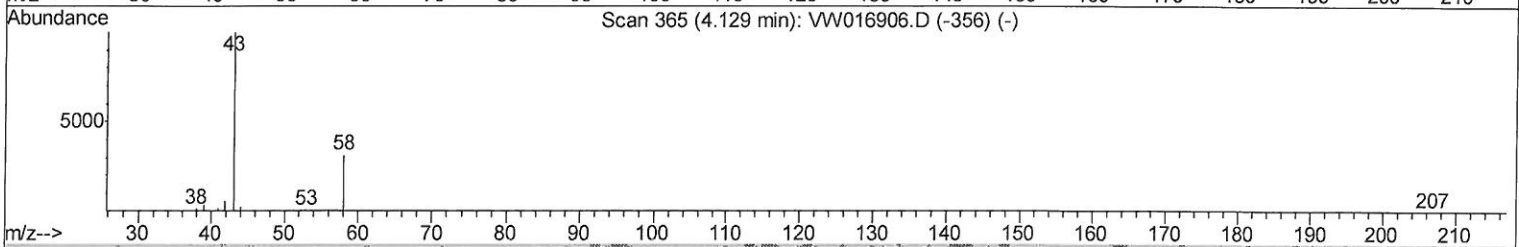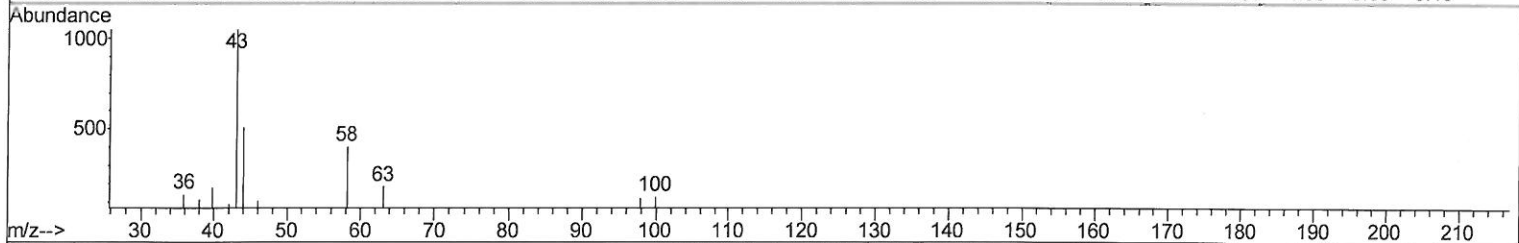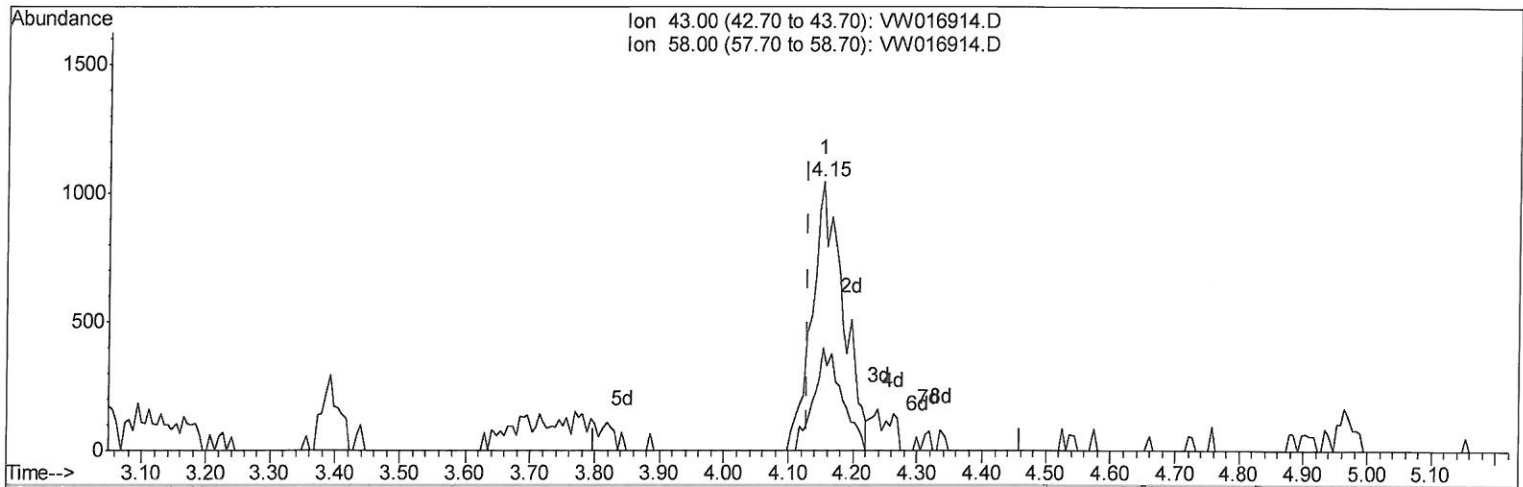

TIC: VW016914.D

(13) Acetone (T)

4.153min (+0.024) 3.54ug/L m

response 3526

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	32.73
0.00	0.00	0.00
0.00	0.00	0.00

5/10/20/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW01620\
 Data File : VW016914.D
 Acq On : 15 Oct 2020 16:09
 Operator : SY/VA
 Sample : L4421-18
 Misc : 5.55G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG1A4

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 11:00:16 AM

Quant Time: Oct 16 08:55:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 16 08:07:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	588265	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	521213	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	232850	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	134019	23.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.36%
7) Chloroethane-d5	2.89	69	115911	23.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.24%
10) 1,1-Dichloroethene-d2	4.02	63	205934	16.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.84%
20) 2-Butanone-d5	7.09	46	60323	45.89	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.78%
24) Chloroform-d	7.65	84	304355	24.52	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.08%
26) 1,2-Dichloroethane-d4	8.31	65	151788	25.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.28%
29) Benzene-d6	8.27	84	621385	26.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.00%
33) 1,2-Dichloropropane-d6	9.27	67	170032	26.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.92%
37) Toluene-d8	10.33	98	569368	25.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.96%
38) trans-1,3-Dichloropropene-	10.58	79	65685	23.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.64%
39) 2-Hexanone-d5	10.93	63	51021	51.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128830	25.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.28%
61) 1,2-Dichlorobenzene-d4	13.86	152	195617	26.49	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.96%

Target Compounds

13) Acetone	4.15	43	3526m)	3.545	ug/L	Ovalue 95
16) Methylene chloride	4.92	84	22204	2.735	ug/L	95
47) Tetrachloroethene	10.87	164	68499	9.332	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101620\
Data File : VW016914.D
Acq On : 15 Oct 2020 16:09
Operator : SY/VA
Sample : L4421-18
Misc : 5.55G/10ML/MSVOA W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG1A4

Manual Integrations
APPROVED

MMDadoda
10/19/2020 11:00:16 AM

Quant Time: Oct 16 08:55:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 16 08:07:29 2020
Response via : Initial Calibration

