

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101720\
 Data File : VW016933.D
 Acq On : 16 Oct 2020 17:15
 Operator : SY/VA
 Sample : L4426-10
 Misc : 4.94G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3Y5

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 11:53:13 AM

Quant Time: Oct 17 00:45:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 17 00:37:07 2020
 Response via : Initial Calibration

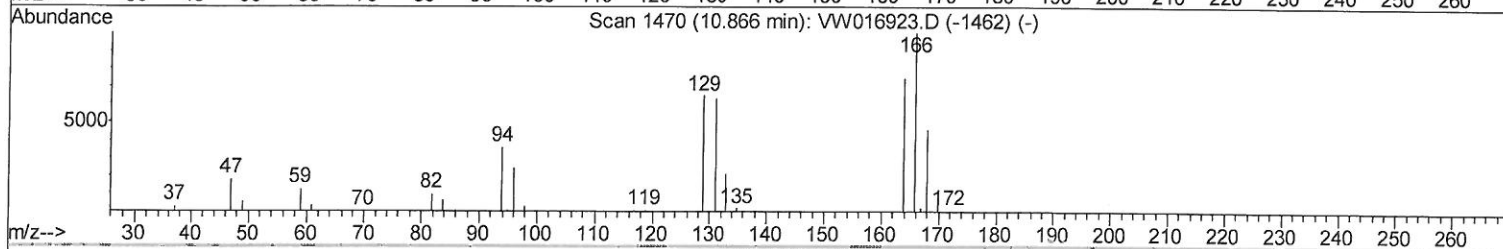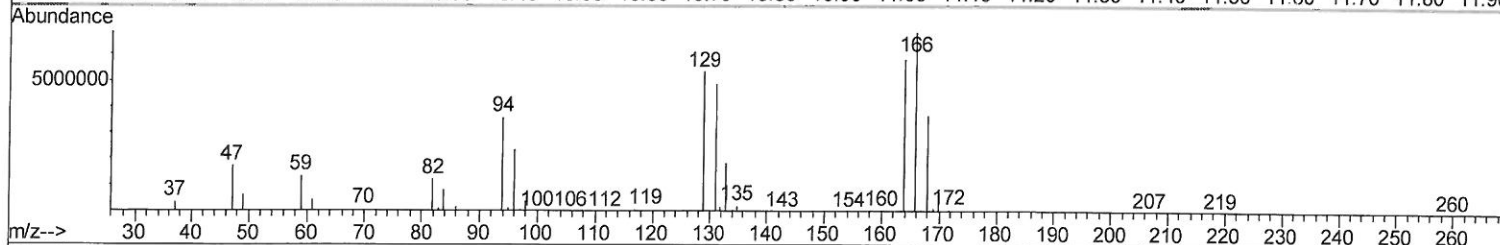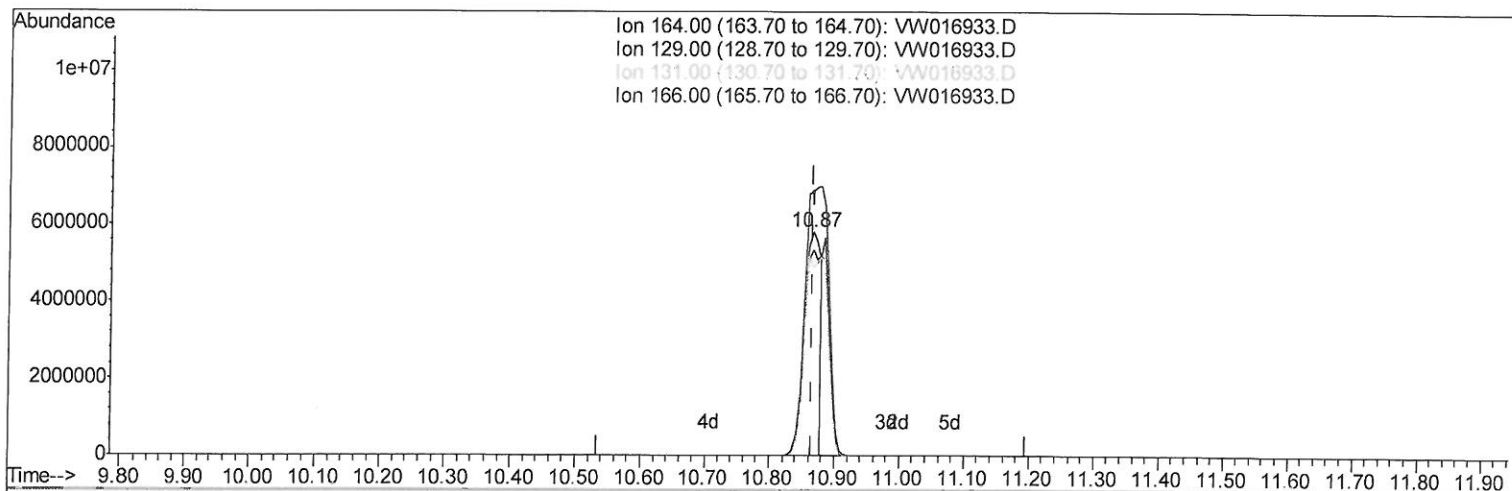

TIC: VW016933.D

(47) Tetrachloroethene (T)

10.865min (-0.000) 1373.89ug/L

response 9980511

Ion	Exp%	Act%
164.00	100	100
129.00	88.20	92.04
131.00	85.30	84.22
166.00	126.20	117.96

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101720\
Data File : VW016933.D
Acq On : 16 Oct 2020 17:15
Operator : SY/VA
Sample : L4426-10
Misc : 4.94G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3Y5

Manual Integrations
APPROVED

MMDadoda
10/19/2020 11:53:13 AM

Quant Time: Oct 17 00:45:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 17 00:37:07 2020
Response via : Initial Calibration

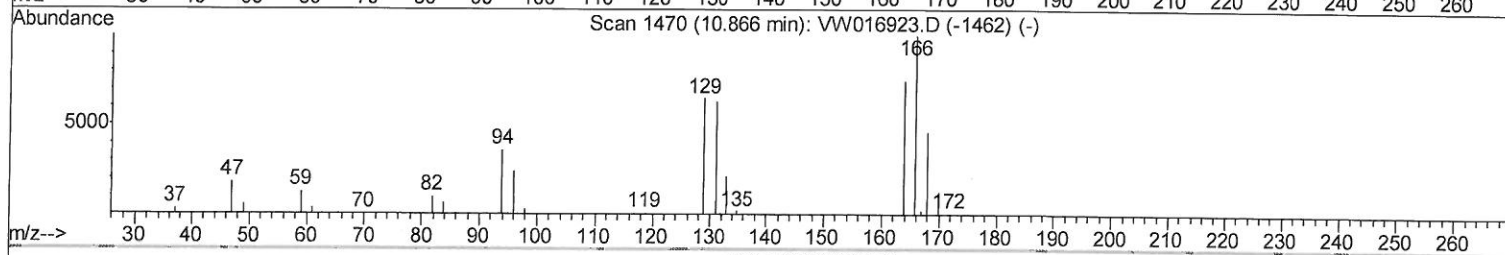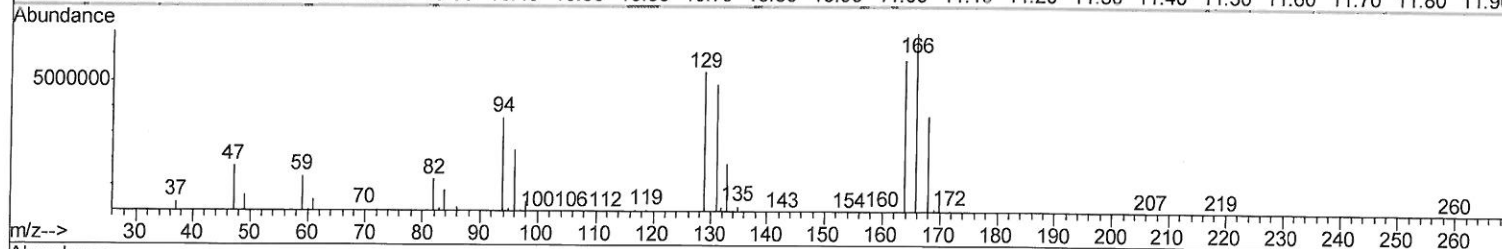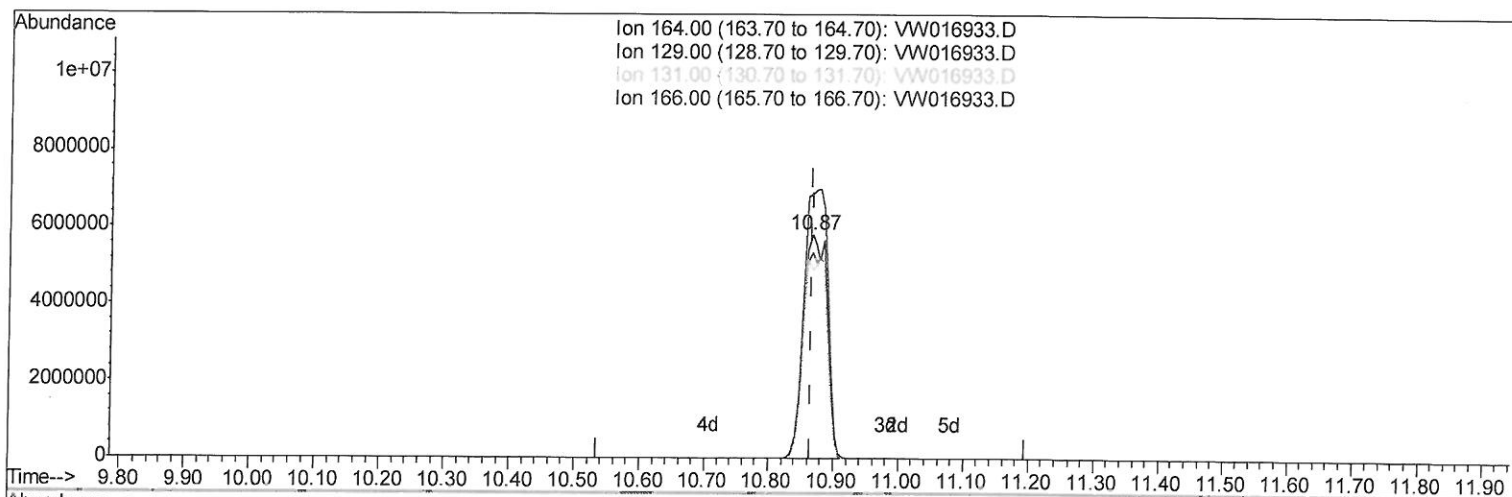

TIC: VW016933.D

(47) Tetrachloroethene (T)

10.865min (-0.000) 1976.55ug/L m

response 14358456

Ion	Exp%	Act%
164.00	100	100
129.00	88.20	92.04
131.00	85.30	84.22
166.00	126.20	117.96

>10/20/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101720\
 Data File : VW016933.D
 Acq On : 16 Oct 2020 17:15
 Operator : SY/VA
 Sample : L4426-10
 Misc : 4.94G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3Y5

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 11:53:13 AM

Quant Time: Oct 17 02:13:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 17 00:37:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	604997	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	515835	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	239912	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	117285	19.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.60%
7) Chloroethane-d5	2.89	69	103858	20.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.96%
10) 1,1-Dichloroethene-d2	4.03	63	182232	14.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.52%
20) 2-Butanone-d5	7.08	46	66877	49.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.94%
24) Chloroform-d	7.65	84	289165	22.65	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	8.31	65	146152	23.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.80%
29) Benzene-d6	8.27	84	578280	24.68	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.72%
33) 1,2-Dichloropropane-d6	9.28	67	164193	26.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.32%
37) Toluene-d8	10.33	98	531706	24.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.20%
38) trans-1,3-Dichloropropene-	10.58	79	63339	22.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.24%
39) 2-Hexanone-d5	10.93	63	50532	51.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128585	25.28	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.12%
61) 1,2-Dichlorobenzene-d4	13.85	152	177515	23.33	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.32%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.13	43	5690	5.562	ug/L	99
14) Carbon disulfide	4.39	76	10202	0.455	ug/L	96
16) Methylene chloride	4.92	84	11786	1.412	ug/L	97
35) Trichloroethene	9.10	95	30345	3.873	ug/L	97
43) 4-Methyl-2-pentanone	10.21	43	7293	2.313	ug/L	99
47) Tetrachloroethene	10.87	164	14358456m	1976.552	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101720\
Data File : VW016933.D
Acq On : 16 Oct 2020 17:15
Operator : SY/VA
Sample : L4426-10
Misc : 4.94G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3Y5

Manual Integrations
APPROVED

MMDadoda
10/19/2020 11:53:13 AM

Quant Time: Oct 17 02:13:15 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 17 00:37:07 2020
Response via : Initial Calibration

