
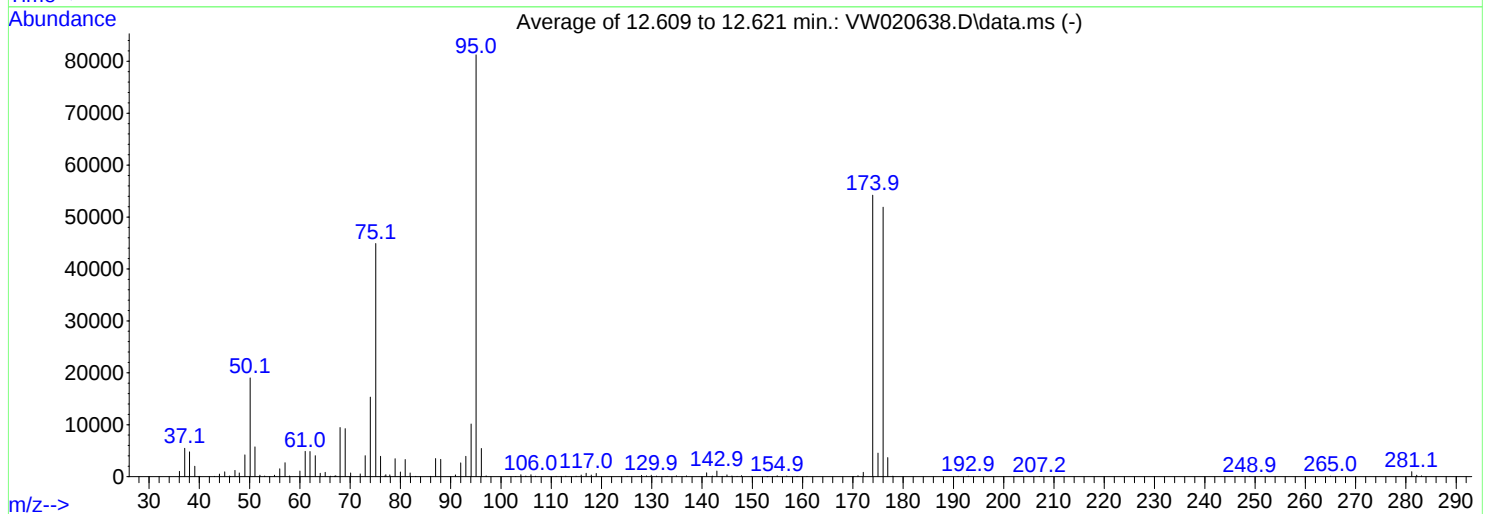


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102021\
Data File : VW020638.D
Acq On : 20 Oct 2021 07:53
Operator : SY/VA
Sample : BFB456
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB456

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Title : SFAM01.0
Last Update : Thu Oct 21 01:08:32 2021

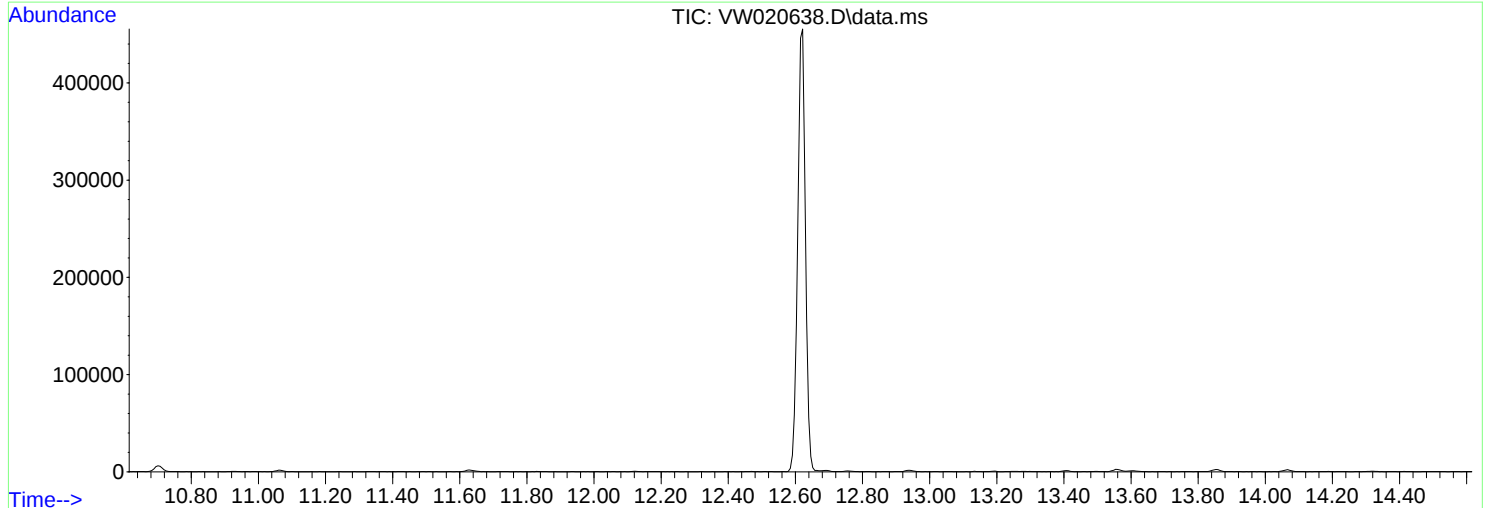

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	19028	PASS
75	95	30	80	55.3	44888	PASS
95	95	100	100	100.0	81243	PASS
96	95	5	9	6.7	5428	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.7	54227	PASS
175	174	5	9	8.4	4545	PASS
176	174	95	105	95.7	51912	PASS
177	176	5	10	7.1	3664	PASS

m/z	Abundance
36.10	1158.0
37.10	6103.0
38.10	5522.0
39.10	2231.0
39.90	220.0
43.00	75.0
44.10	701.0
45.10	1032.0
46.00	238.0
47.10	1309.0
48.00	751.0
49.00	4766.0
50.10	21336.0
51.00	6597.0
52.10	333.0
53.00	141.0
54.10	69.0
55.00	269.0
56.00	1656.0
57.00	3054.0
57.90	120.0
60.00	1304.0
61.10	5442.0
62.00	5570.0
63.10	4452.0
64.00	689.0
65.10	926.0
66.10	86.0
67.10	283.0
68.00	10714.0
69.00	10664.0
70.10	761.0
72.00	600.0
73.00	4676.0
74.00	17032.0
75.10	51160.0
76.10	4374.0
77.10	630.0
77.90	323.0
78.90	3943.0
80.00	1010.0
81.00	3715.0
81.90	851.0
83.00	86.0
87.00	3800.0
88.00	3679.0
91.00	352.0
92.00	2994.0
93.00	4464.0
94.10	11316.0
95.10	92888.0
96.10	6147.0
97.10	193.0
103.00	60.0
103.90	395.0
105.00	140.0
106.00	376.0
106.90	93.0
110.00	51.0
111.00	75.0
111.90	80.0
112.90	102.0
114.90	108.0
115.90	329.0
116.90	746.0
117.90	384.0
118.90	669.0
123.90	51.0
125.10	69.0
128.00	302.0
128.90	154.0
129.90	333.0
130.90	137.0
133.10	79.0
134.90	171.0
136.90	163.0
139.90	78.0
140.90	834.0
142.00	143.0
142.90	1238.0
144.00	67.0
145.00	411.0
146.00	109.0
146.90	72.0
147.90	233.0
149.80	80.0
155.00	173.0
156.80	127.0
159.00	103.0
160.80	90.0
171.00	245.0
172.00	1002.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

174.00	59512.0
175.00	4754.0
176.00	52784.0
177.00	4040.0
178.00	107.0
190.80	94.0
192.90	122.0
207.10	71.0
248.90	78.0
265.00	93.0
281.20	1066.0
282.10	280.0
283.10	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

m/z	Abundance
36.00	1044.0
37.10	5753.0
38.10	4864.0
39.10	2146.0
40.10	203.0
43.00	64.0
44.00	693.0
45.10	989.0
46.20	117.0
47.10	1375.0
47.90	798.0
49.00	4415.0
50.10	20664.0
51.00	6041.0
52.00	266.0
53.00	130.0
53.90	51.0
55.00	294.0
56.00	1745.0
57.10	2894.0
58.00	136.0
60.00	1153.0
61.00	5377.0
62.00	5309.0
63.10	4239.0
64.10	548.0
65.00	772.0
66.10	103.0
66.90	248.0
68.00	10253.0
69.00	10047.0
70.10	796.0
72.00	648.0
73.00	4272.0
74.00	16696.0
75.10	49184.0
76.10	4252.0
77.10	496.0
77.90	389.0
79.00	3501.0
80.00	924.0
81.00	3628.0
81.90	800.0
83.10	89.0
86.00	202.0
87.00	4053.0
88.00	3665.0
91.00	388.0
92.00	3062.0
93.00	4370.0
94.00	11330.0
95.10	90216.0
96.10	6130.0
97.00	173.0
102.90	56.0
104.00	481.0
105.00	140.0
105.90	449.0
106.90	105.0
110.00	86.0
110.90	86.0
112.00	74.0
112.90	79.0
115.00	90.0
115.90	392.0
117.00	695.0
117.90	371.0
118.90	679.0
124.00	51.0
128.00	308.0
128.90	183.0
129.90	349.0
130.90	133.0
132.80	60.0
134.90	205.0
136.90	141.0
140.90	969.0
142.00	118.0
142.90	1195.0
144.00	82.0
144.90	288.0
145.90	127.0
147.00	91.0
147.90	211.0
149.90	83.0
152.90	58.0
155.00	237.0
156.80	134.0
158.80	104.0
160.90	82.0
170.00	55.0
171.00	178.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

172.00	950.0
173.90	64312.0
175.00	5667.0
176.00	67384.0
177.00	4713.0
177.90	137.0
190.80	54.0
265.10	54.0
281.10	662.0
282.20	207.0
283.20	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

Scan 1749 (12.566 min): VW020638.D\data.ms
BFB456

m/z	Abundance
39.90	116.0
44.00	163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

m/z	Abundance
36.00	893.0
37.10	4513.0
38.00	3933.0
39.10	1624.0
39.90	224.0
43.00	55.0
44.00	594.0
45.00	800.0
46.00	135.0
47.10	924.0
48.00	538.0
49.10	3432.0
50.10	15085.0
51.10	4531.0
52.00	202.0
53.00	139.0
54.90	251.0
56.00	1160.0
57.10	2090.0
58.00	95.0
60.00	753.0
61.10	3752.0
62.00	3625.0
63.00	3456.0
64.10	714.0
65.00	790.0
66.10	109.0
67.20	255.0
68.00	7390.0
69.00	6999.0
70.10	563.0
72.00	343.0
73.00	3187.0
74.00	12268.0
75.10	34320.0
76.00	3145.0
76.90	361.0
77.90	302.0
78.90	2948.0
80.00	743.0
80.90	2570.0
82.00	528.0
87.00	2552.0
88.00	2617.0
90.90	281.0
92.00	1936.0
93.00	2941.0
94.00	7781.0
95.00	60624.0
96.10	4007.0
97.00	112.0
104.00	253.0
104.90	86.0
105.90	272.0
106.90	66.0
111.00	71.0
112.90	61.0
114.90	80.0
116.00	249.0
117.00	481.0
118.10	223.0
119.00	509.0
125.10	75.0
127.90	176.0
129.00	111.0
129.90	178.0
131.00	100.0
133.00	143.0
134.90	120.0
136.90	119.0
139.80	58.0
140.90	463.0
142.10	96.0
143.00	793.0
144.00	63.0
145.00	361.0
145.90	112.0
147.80	140.0
149.80	70.0
154.90	110.0
156.90	124.0
159.10	68.0
171.00	137.0
172.10	597.0
174.00	38856.0
175.00	3215.0
176.00	35568.0
176.90	2238.0
178.00	84.0
191.00	89.0
193.00	172.0
207.20	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456

249.00	108.0
264.90	142.0
281.10	1158.0
282.10	328.0
283.10	222.0

Instrument :
MSVOA_W
ClientSampleId :
BFB456