

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
Data File : VW016998.D
Acq On : 26 Oct 2020 14:59
Operator : SY/VA
Sample : L4502-11
Misc : 4.53G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG438

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:35:20 PM

Quant Time: Oct 27 08:25:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 27 08:16:51 2020
Response via : Initial Calibration

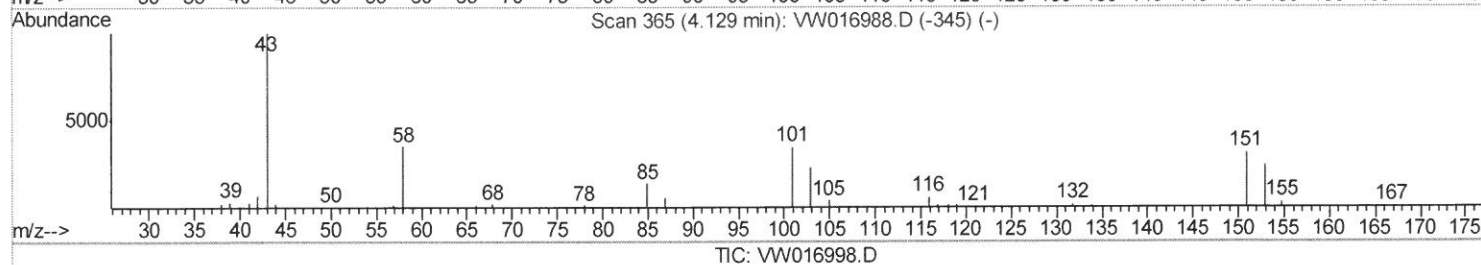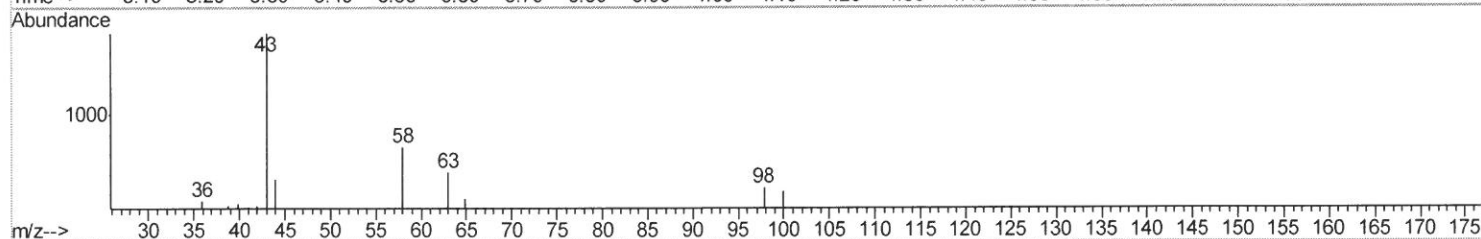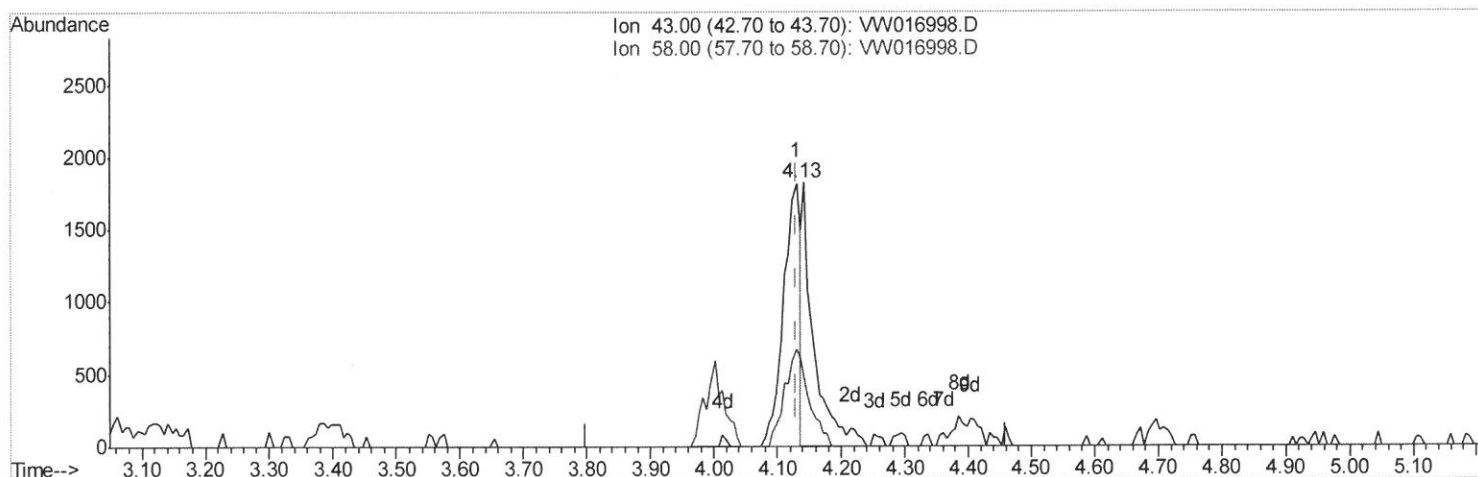

(13) Acetone (T)

4.129min (-0.000) 4.19ug/L

response 3316

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	53.50
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
 Data File : VW016998.D
 Acq On : 26 Oct 2020 14:59
 Operator : SY/VA
 Sample : L4502-11
 Misc : 4.53G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG438

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:35:20 PM

Quant Time: Oct 27 08:25:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 27 08:16:51 2020
 Response via : Initial Calibration

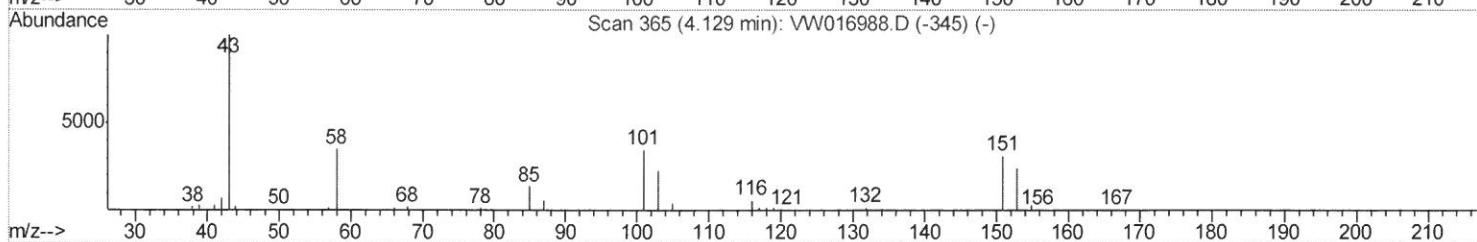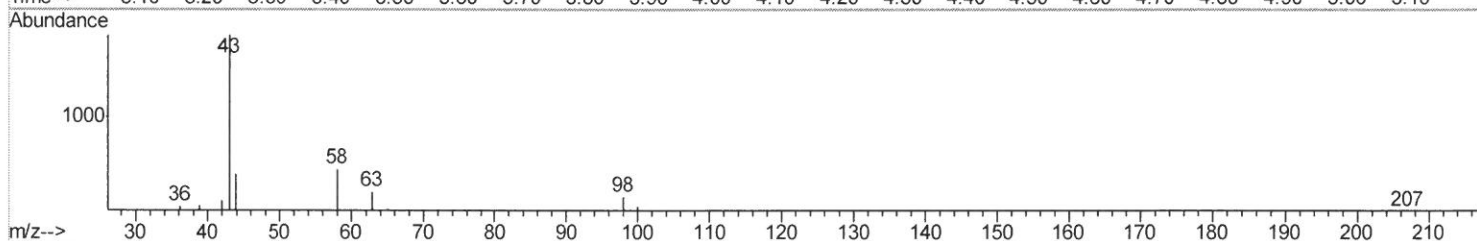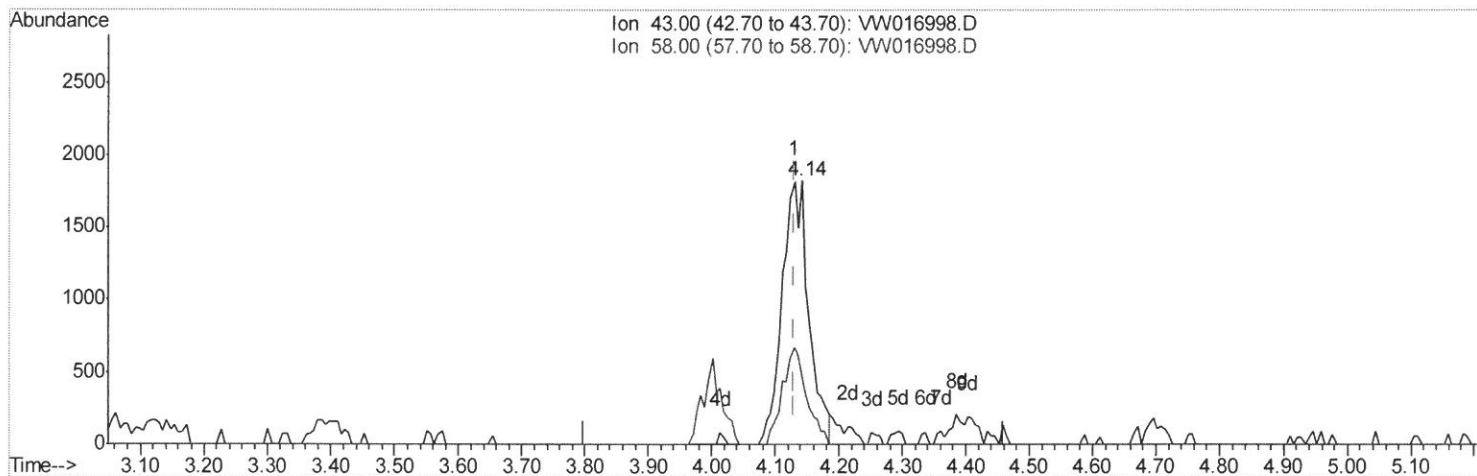

TIC: VW016998.D

(13) Acetone (T)

4.141min (+0.012) 6.72ug/L m

response 5319

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	33.35
0.00	0.00	0.00
0.00	0.00	0.00

11/09/20 hy

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
 Data File : VW016998.D
 Acq On : 26 Oct 2020 14:59
 Operator : SY/VA
 Sample : L4502-11
 Misc : 4.53G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG438

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:35:20 PM

Quant Time: Oct 27 09:03:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 27 08:16:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	541036	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	470953	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	189735	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	125633	20.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.48%
7) Chloroethane-d5	2.89	69	97365	20.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.48%
10) 1,1-Dichloroethene-d2	4.03	63	177499	14.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.44%
20) 2-Butanone-d5	7.08	46	60211	51.19	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.38%
24) Chloroform-d	7.65	84	254775	20.42	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.68%
26) 1,2-Dichloroethane-d4	8.31	65	129185	22.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.00%
29) Benzene-d6	8.27	84	526651	21.77	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.08%
33) 1,2-Dichloropropane-d6	9.27	67	147634	22.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.44%
37) Toluene-d8	10.33	98	484797	21.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.16%
38) trans-1,3-Dichloropropene-	10.58	79	59045	21.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.20%
39) 2-Hexanone-d5	10.93	63	50041	54.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	118174	23.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.04%
61) 1,2-Dichlorobenzene-d4	13.85	152	147382	22.10	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.40%

Target Compounds

				Ovalue	
5) Vinyl chloride	2.36	62	2588	0.332 ug/L	# 1
13) Acetone	4.14	43	5319m	6.720 ug/L	99
14) Carbon disulfide	4.39	76	21253	0.990 ug/L	99
16) Methylene chloride	4.93	84	7277	1.017 ug/L	94
43) 4-Methyl-2-pentanone	10.21	43	3182	1.155 ug/L	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
Data File : VW016998.D
Acq On : 26 Oct 2020 14:59
Operator : SY/VA
Sample : L4502-11
Misc : 4.53G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG438

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:35:20 PM

Quant Time: Oct 27 09:03:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 27 08:16:51 2020
Response via : Initial Calibration

