

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
Data File : VW017001.D
Acq On : 26 Oct 2020 16:09
Operator : SY/VA
Sample : VIBLK26
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK26

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:35:26 PM

Quant Time: Oct 27 08:25:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 27 08:16:51 2020
Response via : Initial Calibration

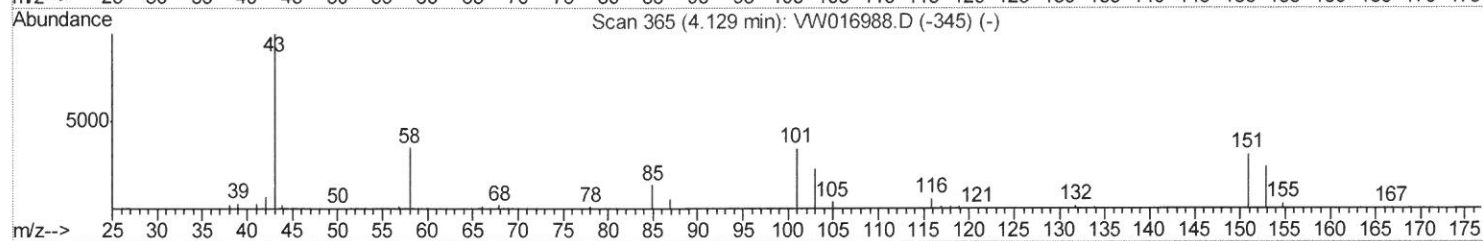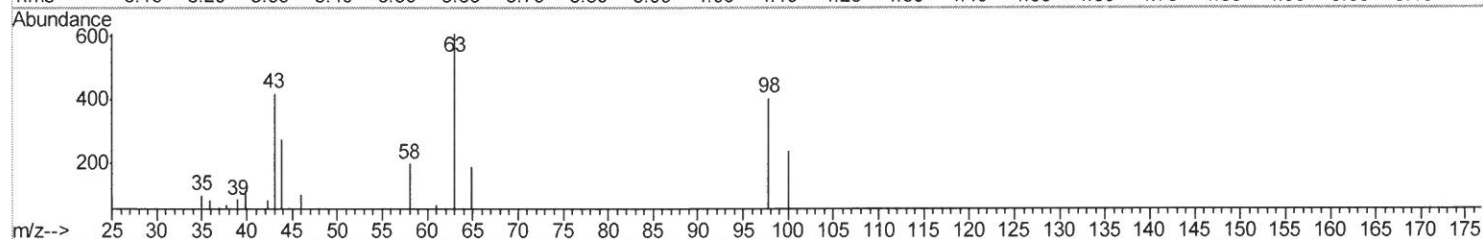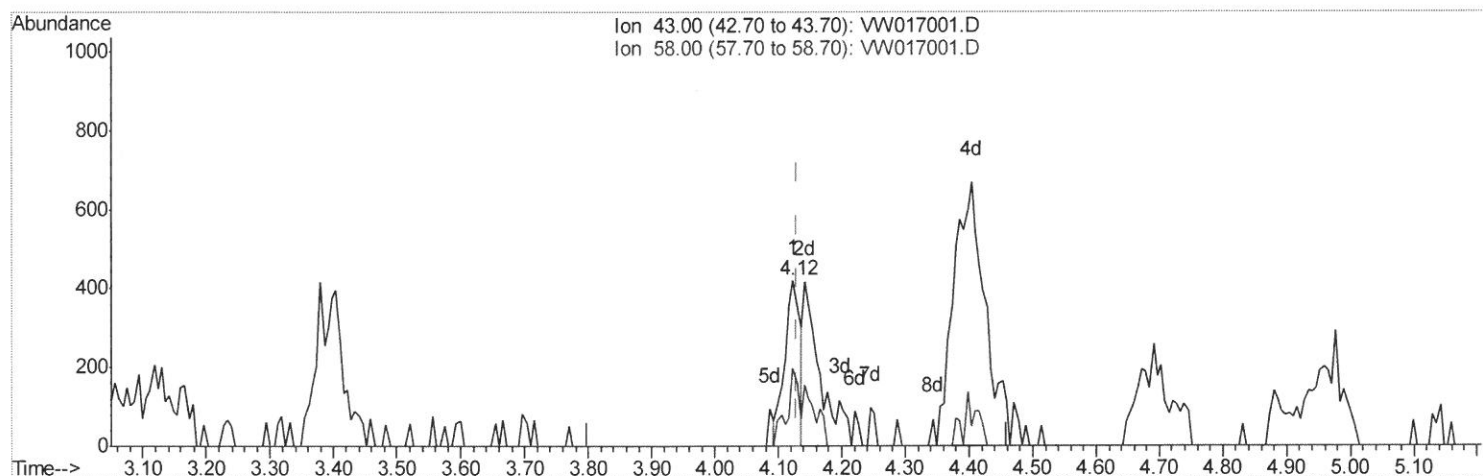

TIC: VW017001.D

(13) Acetone (T)

4.123min (-0.006) 0.94ug/L

response 697

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	25.97
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
 Data File : VW017001.D
 Acq On : 26 Oct 2020 16:09
 Operator : SY/VA
 Sample : VIBLK26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK26

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:35:26 PM

Quant Time: Oct 27 08:25:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 27 08:16:51 2020
 Response via : Initial Calibration

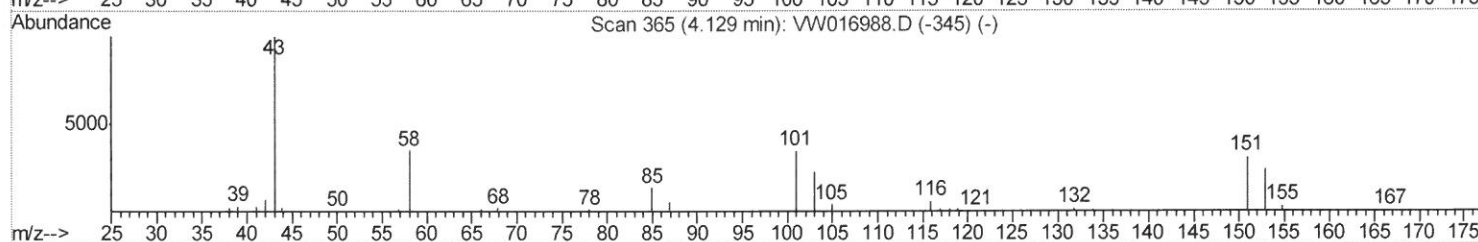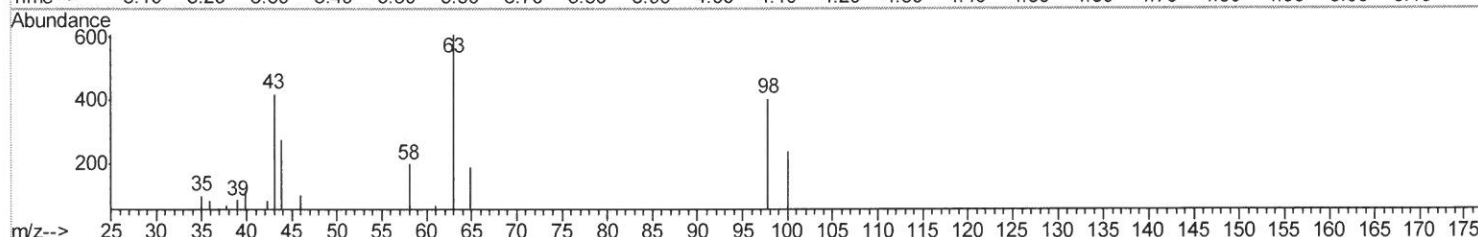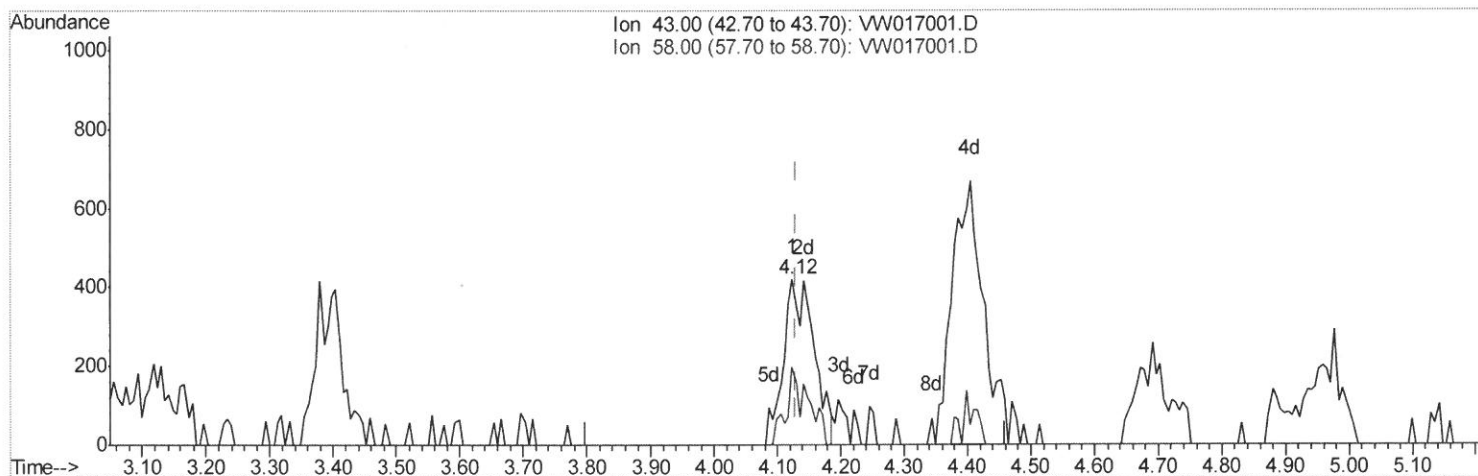

TIC: VW017001.D

(13) Acetone (T)

4.123min (-0.006) 1.90ug/L m

response 1405

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	12.88
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
 Data File : VW017001.D
 Acq On : 26 Oct 2020 16:09
 Operator : SY/VA
 Sample : VIBLK26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK26

Manual Integrations
 APPROVED

MMDadoda
 10/27/2020 3:35:26 PM

Quant Time: Oct 27 09:13:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 27 08:16:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	505062	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	471019	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	237210	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	122964	21.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.40%
7) Chloroethane-d5	2.89	69	98268	21.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.04%
10) 1,1-Dichloroethene-d2	4.02	63	181670	16.02	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.08%
20) 2-Butanone-d5	7.08	46	80720	73.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.02%#
24) Chloroform-d	7.65	84	277037	23.78	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.12%
26) 1,2-Dichloroethane-d4	8.31	65	148208	27.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.12%
29) Benzene-d6	8.27	84	564390	23.33	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.32%
33) 1,2-Dichloropropane-d6	9.27	67	160822	24.63	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.52%
37) Toluene-d8	10.32	98	541693	23.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.12%
38) trans-1,3-Dichloropropene-	10.58	79	69854	25.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.80%
39) 2-Hexanone-d5	10.93	63	67996	74.15	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	148.30%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	155522	31.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.04%#
61) 1,2-Dichlorobenzene-d4	13.85	152	211037	25.31	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.24%

Target Compounds

13) Acetone	4.12	43	1405m	1.902	ug/L	Ovalue
16) Methylene chloride	4.93	84	6490	0.972	ug/L	92
43) 4-Methyl-2-pentanone	10.21	43	2677	0.972	ug/L	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102620\
Data File : VW017001.D
Acq On : 26 Oct 2020 16:09
Operator : SY/VA
Sample : VIBLK26
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK26

Manual Integrations
APPROVED

MMDadoda
10/27/2020 3:35:26 PM

Quant Time: Oct 27 09:13:30 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 27 08:16:51 2020
Response via : Initial Calibration

