

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
 Data File : VW017012.D
 Acq On : 28 Oct 2020 15:12
 Operator : SY/VA
 Sample : L4502-20
 Misc : 5.95G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG443

Manual Integrations
 APPROVED

MMDadoda
 10/30/2020 1:33:30 PM

Quant Time: Oct 29 08:09:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 29 08:01:00 2020
 Response via : Initial Calibration

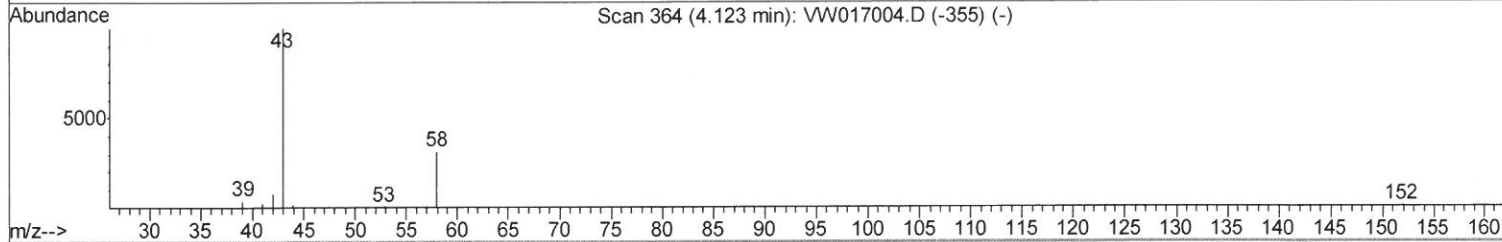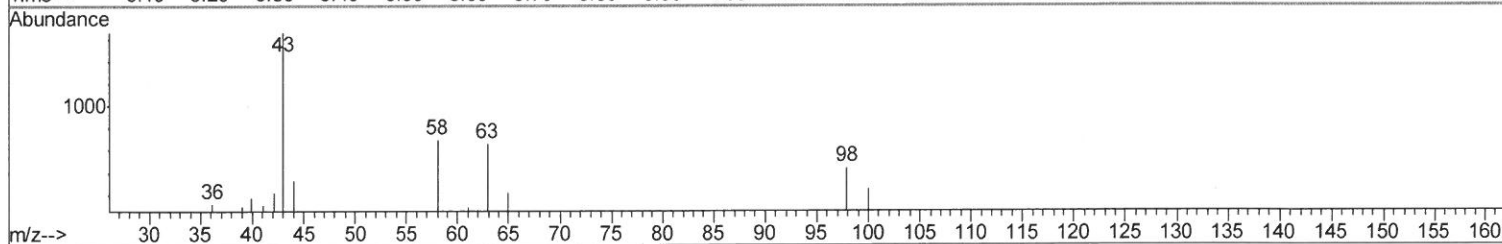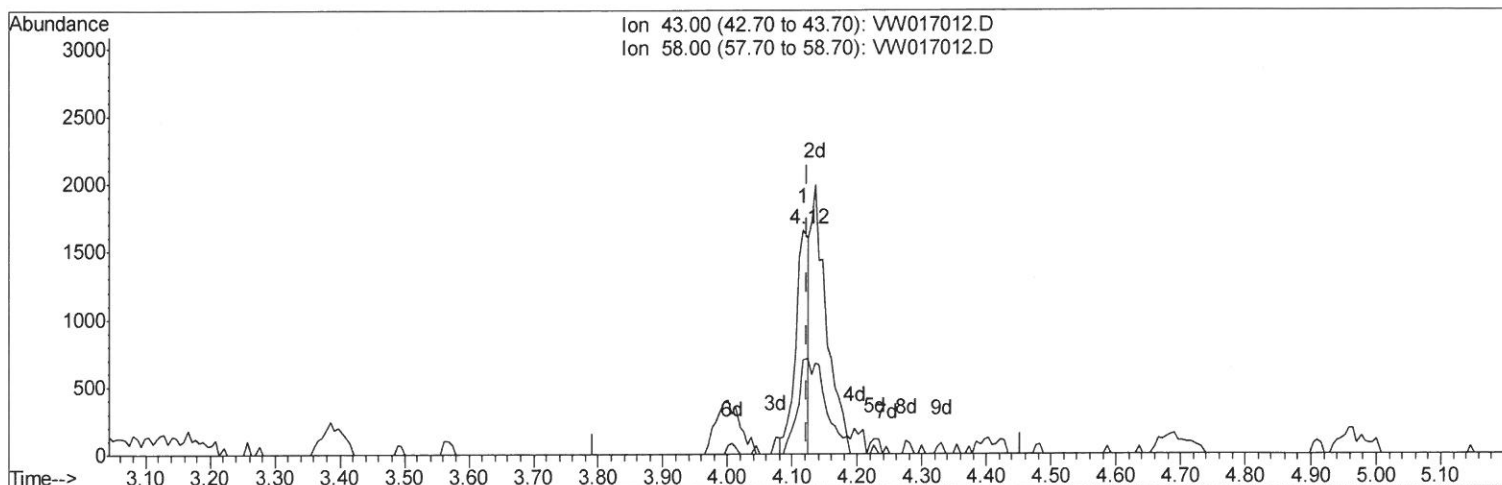

TIC: VW017012.D

(13) Acetone (T)

4.117min (-0.006) 3.22ug/L

response 2271

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	46.72
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
 Data File : VW017012.D
 Acq On : 28 Oct 2020 15:12
 Operator : SY/VA
 Sample : L4502-20
 Misc : 5.95G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG443

Manual Integrations
 APPROVED

MMDadoda
 10/30/2020 1:33:30 PM

Quant Time: Oct 29 08:09:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 29 08:01:00 2020
 Response via : Initial Calibration

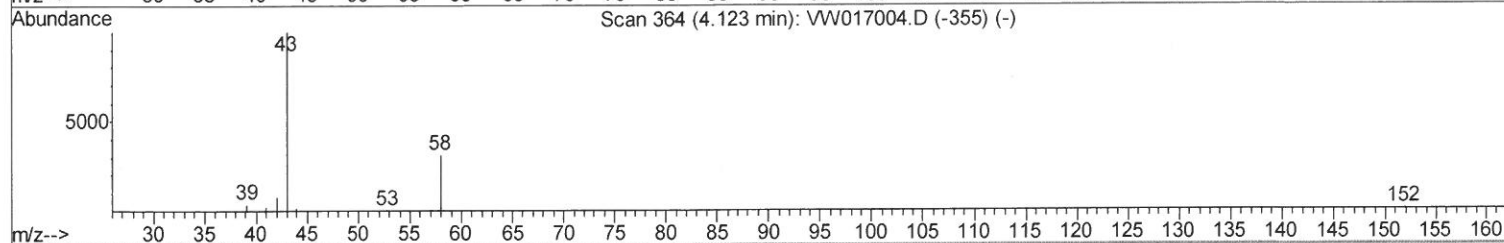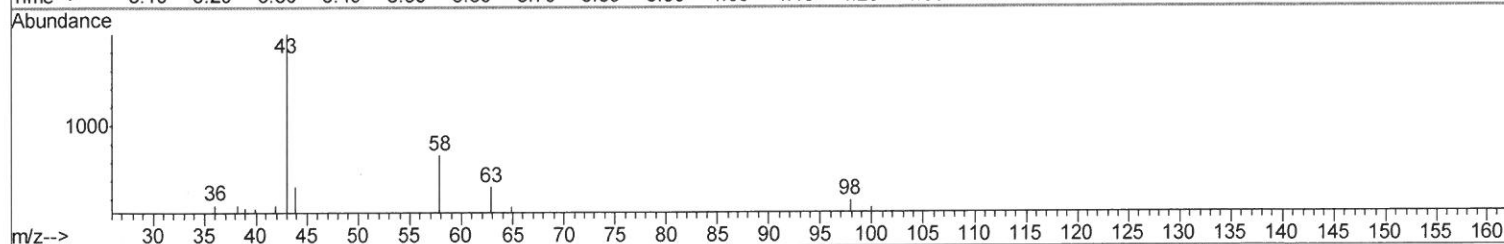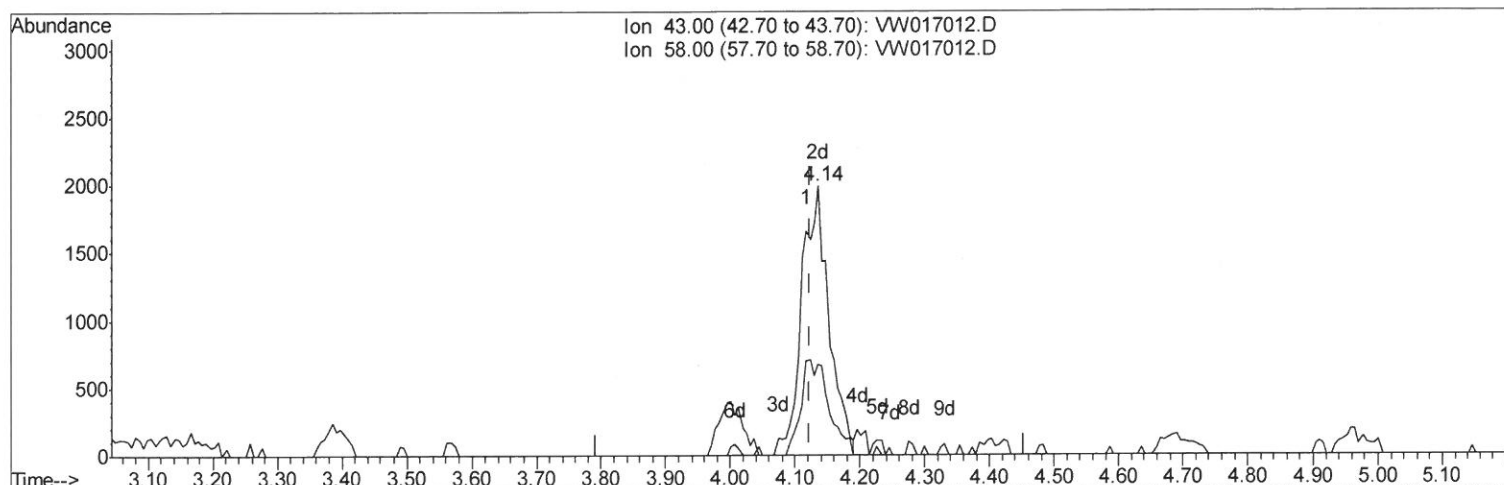

TIC: VW017012.D

(13) Acetone (T)

4.135min (+0.012) 8.30ug/L m

21/06/2020

response 5856

Ion	Exp%	Act%
43.00	100	100
58.00	34.90	18.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
 Data File : VW017012.D
 Acq On : 28 Oct 2020 15:12
 Operator : SY/VA
 Sample : L4502-20
 Misc : 5.95G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG443

Manual Integrations
 APPROVED

MMDadoda
 10/30/2020 1:33:30 PM

Quant Time: Oct 29 08:48:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 29 08:01:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	482450	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	417005	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	188208	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	139955	25.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.56%			
7) Chloroethane-d5	2.89	69	108495	25.15	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.60%			
10) 1,1-Dichloroethene-d2	4.02	63	204173	18.85	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 75.40%			
20) 2-Butanone-d5	7.08	46	48768	46.50	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 93.00%			
24) Chloroform-d	7.65	84	277207	24.91	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 99.64%			
26) 1,2-Dichloroethane-d4	8.31	65	130631	24.94	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 99.76%			
29) Benzene-d6	8.27	84	580831	27.12	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 108.48%			
33) 1,2-Dichloropropane-d6	9.27	67	157541	27.25	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 109.00%			
37) Toluene-d8	10.32	98	544952	27.02	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 108.08%			
38) trans-1,3-Dichloropropene-	10.58	79	61501	25.06	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 100.24%			
39) 2-Hexanone-d5	10.93	63	40751	50.20	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 100.40%			
48) 1,1,2,2-Tetrachloroethane-	12.69	84	105511	23.96	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 95.84%			
61) 1,2-Dichlorobenzene-d4	13.85	152	171840	25.98	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 103.92%			

Target Compounds

13) Acetone	4.14	43	5856m	8.297	ug/L	Ovalue 11/6/20 by
14) Carbon disulfide	4.39	76	8508	0.444	ug/L	98
16) Methylene chloride	4.91	84	11043	1.731	ug/L	94
22) cis-1,2-Dichloroethene	7.17	96	3417	0.512	ug/L	91
34) Benzene	8.32	78	15334	0.666	ug/L	100
35) Trichloroethene	9.09	95	295691	46.346	ug/L	99
43) 4-Methyl-2-pentanone	10.21	43	2407	0.987	ug/L #	80
47) Tetrachloroethene	10.87	164	10326824	1759.592	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
Data File : VW017012.D
Acq On : 28 Oct 2020 15:12
Operator : SY/VA
Sample : L4502-20
Misc : 5.95G/10ML/MSVOA W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG443

Manual Integrations
APPROVED

MMDadoda
10/30/2020 1:33:30 PM

Quant Time: Oct 29 08:48:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 29 08:01:00 2020
Response via : Initial Calibration

