

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
Data File : VW017014.D
Acq On : 28 Oct 2020 16:23
Operator : SY/VA
Sample : L4502-21
Misc : 5.33G/10ML/MSVOA W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG444

Manual Integrations
APPROVED

MMDadoda
10/30/2020 1:33:34 PM

Quant Time: Oct 29 08:09:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 29 08:01:00 2020
Response via : Initial Calibration

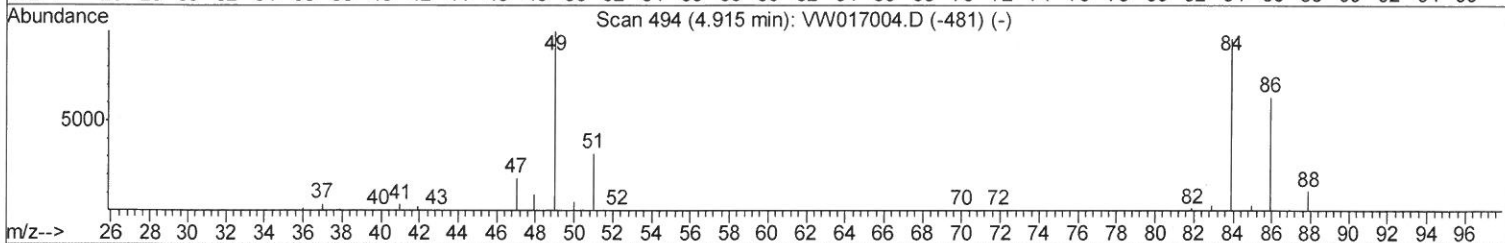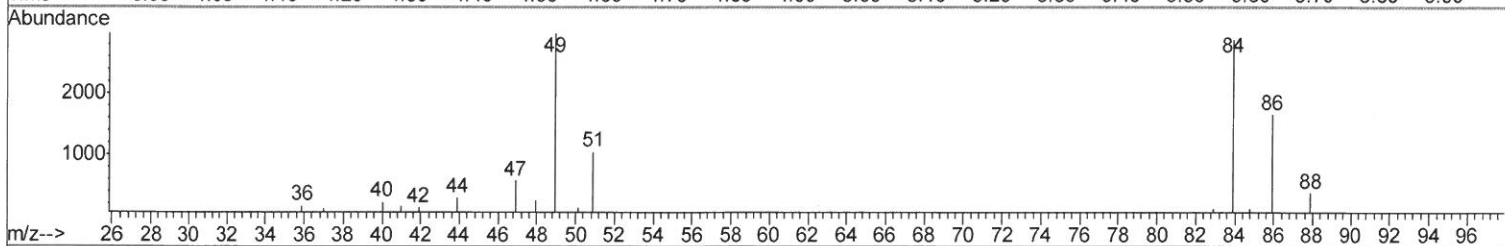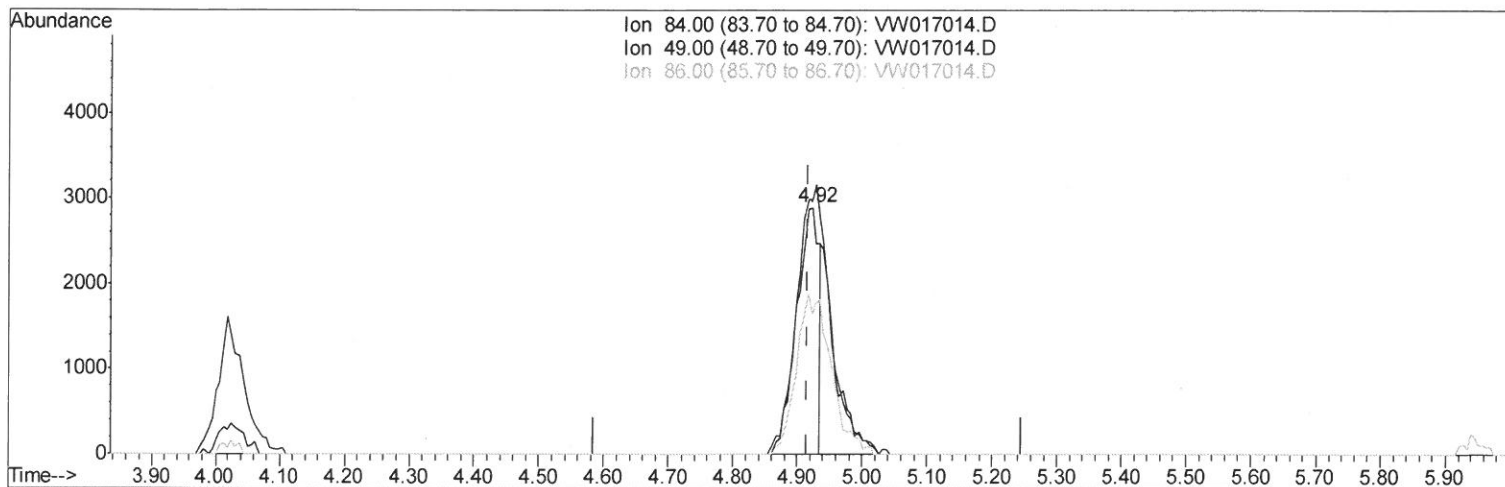

TIC: VW017014.D

(16) Methylene chloride (T)

4.922min (+0.006) 1.17ug/L

response 7101

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	103.39
86.00	67.70	57.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
 Data File : VW017014.D
 Acq On : 28 Oct 2020 16:23
 Operator : SY/VA
 Sample : L4502-21
 Misc : 5.33G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG444

Manual Integrations
 APPROVED

MMDadoda
 10/30/2020 1:33:34 PM

Quant Time: Oct 29 08:09:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 29 08:01:00 2020
 Response via : Initial Calibration

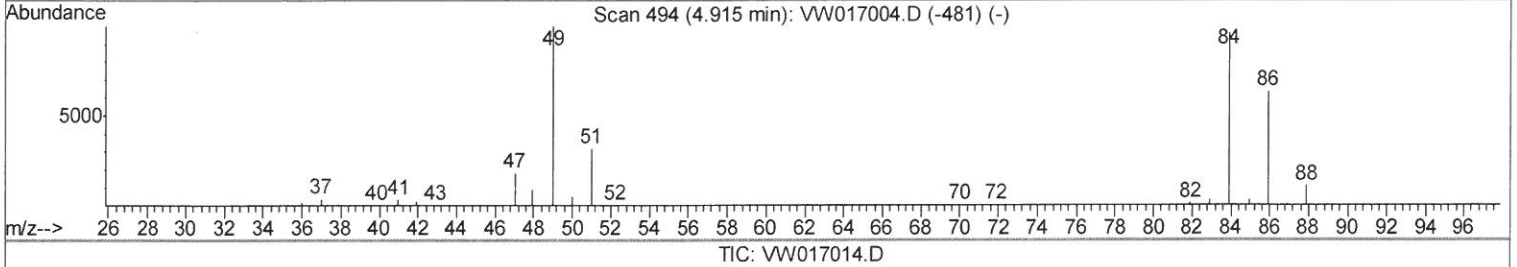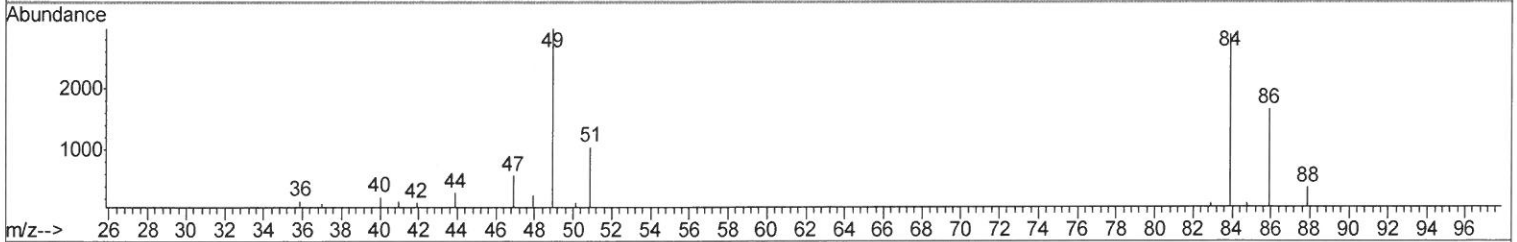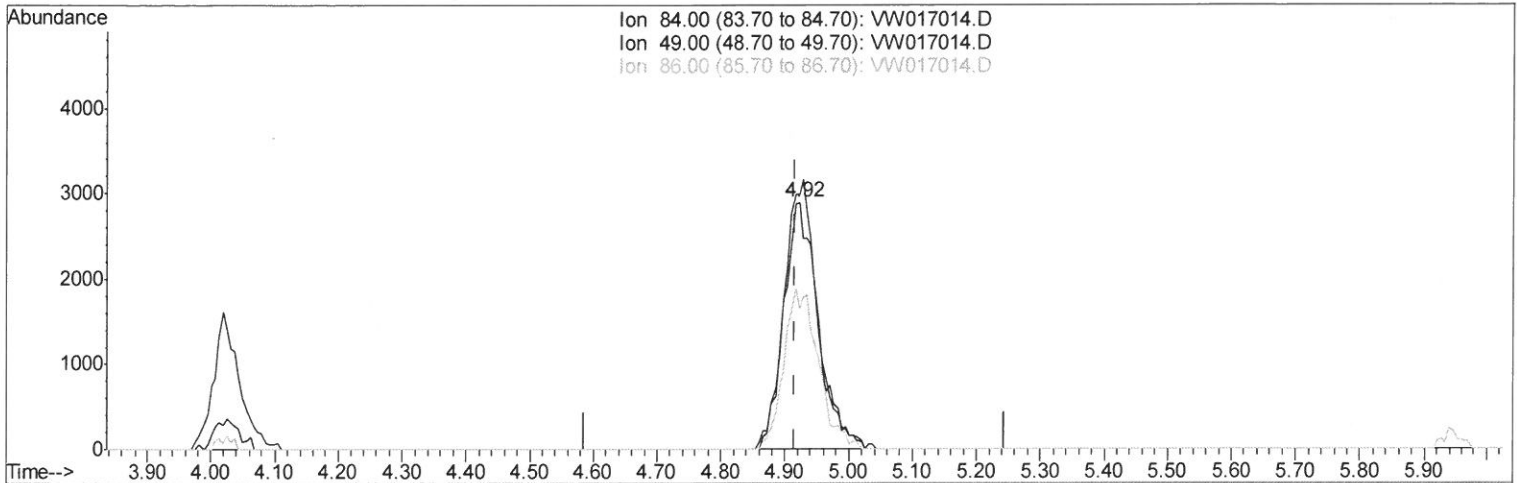

(16) Methylene chloride (T)

4.922min (+0.006) 1.78ug/L m > 11/06/20 Sy
 response 10814

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	103.39
86.00	67.70	57.25
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
 Data File : VW017014.D
 Acq On : 28 Oct 2020 16:23
 Operator : SY/VA
 Sample : L4502-21
 Misc : 5.33G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG444

Manual Integrations
 APPROVED

MMDadoda
 10/30/2020 1:33:34 PM

Quant Time: Oct 29 08:54:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 29 08:01:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	459520	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	415590	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	192642	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	125638	23.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.76%
7) Chloroethane-d5	2.89	69	98350	23.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.72%
10) 1,1-Dichloroethene-d2	4.03	63	179863	17.44	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.76%
20) 2-Butanone-d5	7.08	46	51175	51.22	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.44%
24) Chloroform-d	7.65	84	254773	24.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.16%
26) 1,2-Dichloroethane-d4	8.31	65	125062	25.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.28%
29) Benzene-d6	8.27	84	534305	25.03	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.12%
33) 1,2-Dichloropropane-d6	9.27	67	145860	25.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.24%
37) Toluene-d8	10.33	98	499308	24.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.36%
38) trans-1,3-Dichloropropene-	10.58	79	59143	24.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.72%
39) 2-Hexanone-d5	10.93	63	43066	53.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.46%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	110530	25.18	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	175187	25.87	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.48%

Target Compounds

					Ovalue
13) Acetone	4.13	43	4331	6.443 ug/L	98
14) Carbon disulfide	4.39	76	6071	0.333 ug/L	99
16) Methylene chloride	4.92	84	10814m	1.780 ug/L	86
17) Methyl tert-butyl Ether	5.43	73	3561	0.543 ug/L	84
22) cis-1,2-Dichloroethene	7.17	96	2252	0.354 ug/L	99
35) Trichloroethene	9.09	95	201379	31.671 ug/L	94
43) 4-Methyl-2-pentanone	10.21	43	2216	0.912 ug/L	96
47) Tetrachloroethene	10.87	164	4453007	761.333 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102820\
Data File : VW017014.D
Acq On : 28 Oct 2020 16:23
Operator : SY/VA
Sample : L4502-21
Misc : 5.33G/10ML/MSVOA W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG444

Manual Integrations
APPROVED

MMDadoda
10/30/2020 1:33:34 PM

Quant Time: Oct 29 08:54:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 29 08:01:00 2020
Response via : Initial Calibration

