


Methylene Chloride


Response Ratio

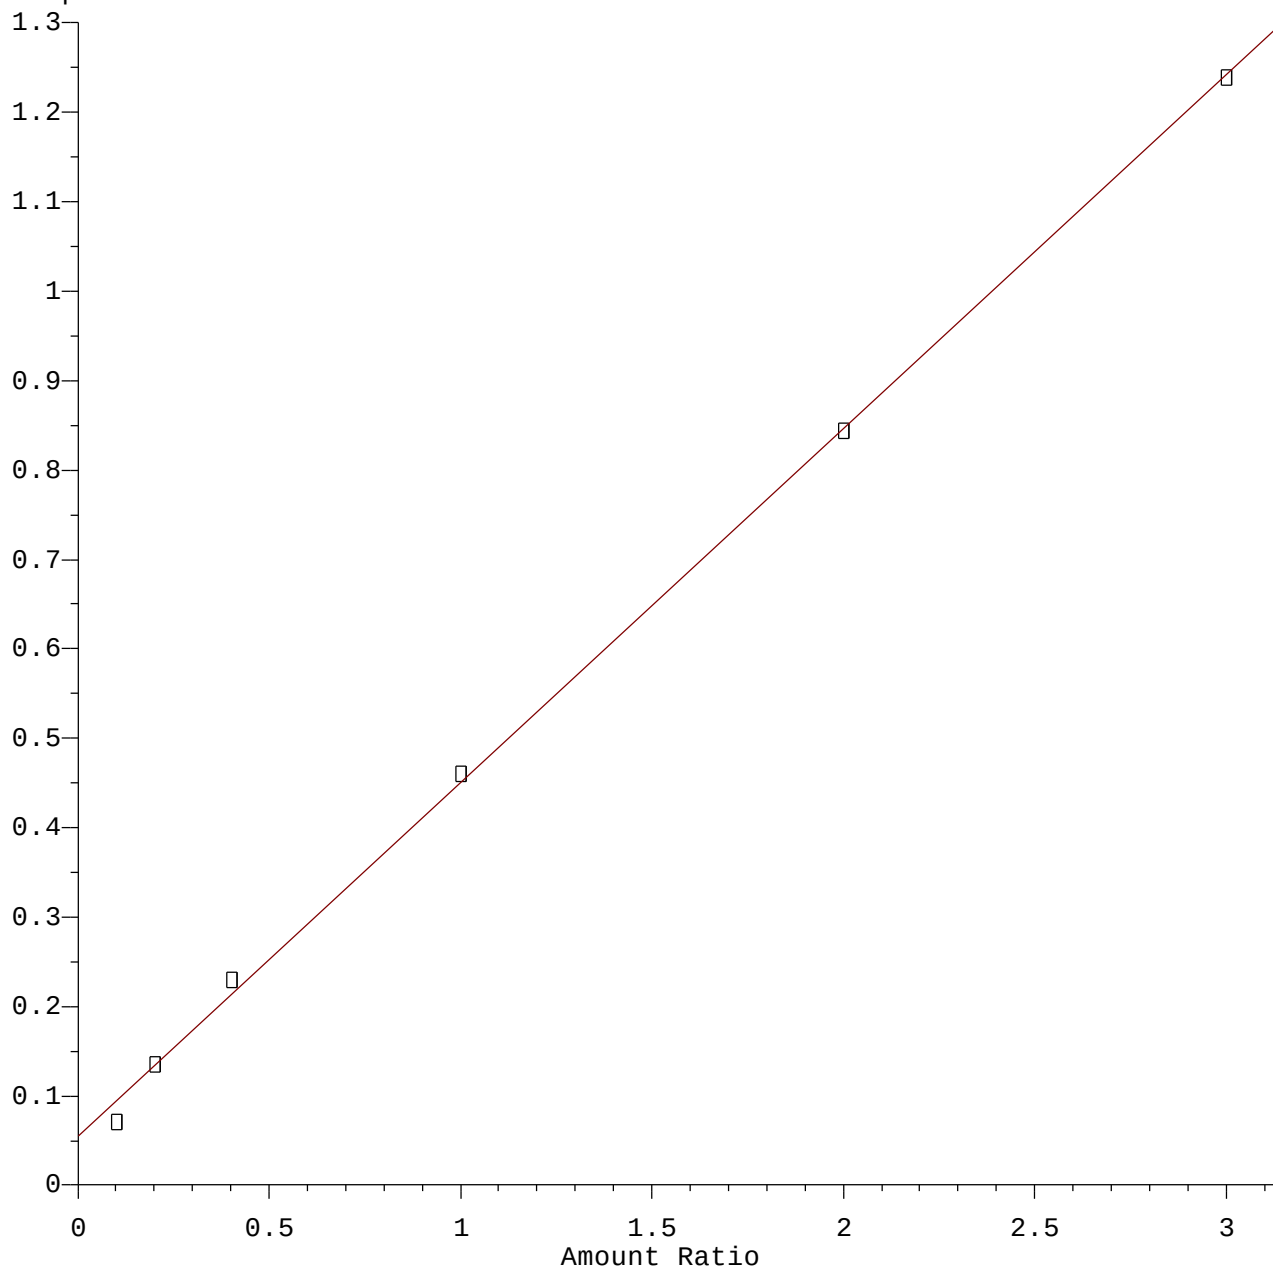

Resp Ratio = $3.96 \times 10^{-1} \times \text{Amt} + 5.37 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Calibration Table Last Updated: Thu Nov 01 03:48:08 2018

trans-1,4-Dichloro-2-butene

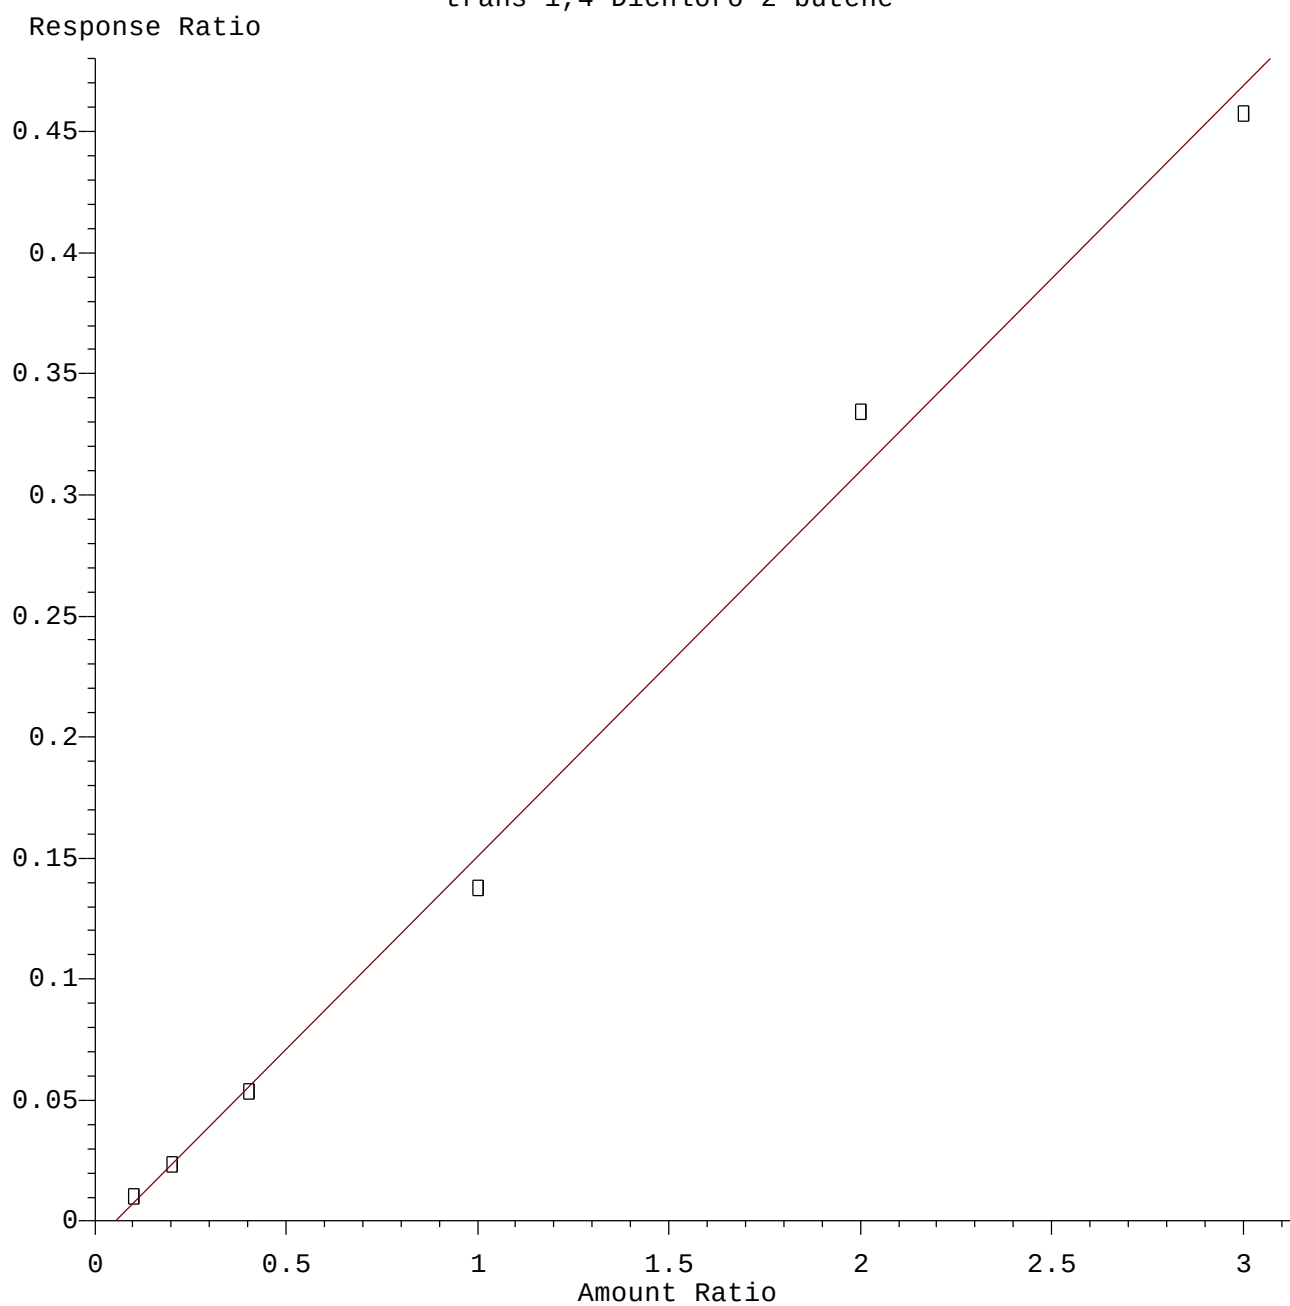

Resp Ratio = $1.59 \times 10^{-1} \times \text{Amt} - 8.47 \times 10^{-3}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Calibration Table Last Updated: Thu Nov 01 03:48:08 2018