

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110218\
 Data File : VW006569.D
 Acq On : 01 Nov 2018 19:33
 Operator : SY/AP
 Sample : J5700-01
 Misc : 4.74G/5ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SI-1

Quant Time: Nov 02 04:07:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 01 03:48:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	197109	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	330398	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	300816	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	138387	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	103554	61.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	122.24%	
35) Dibromofluoromethane	7.88	113	106856	51.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.06%	
50) Toluene-d8	10.33	98	386486	48.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.92%	
62) 4-Bromofluorobenzene	12.62	95	124049	43.35	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.70%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110218\
Data File : VW006569.D
Acq On : 01 Nov 2018 19:33
Operator : SY/AP
Sample : J5700-01
Misc : 4.74G/5ML/MSVOA W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SI-1

Quant Time: Nov 02 04:07:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 01 03:48:08 2018
Response via : Initial Calibration

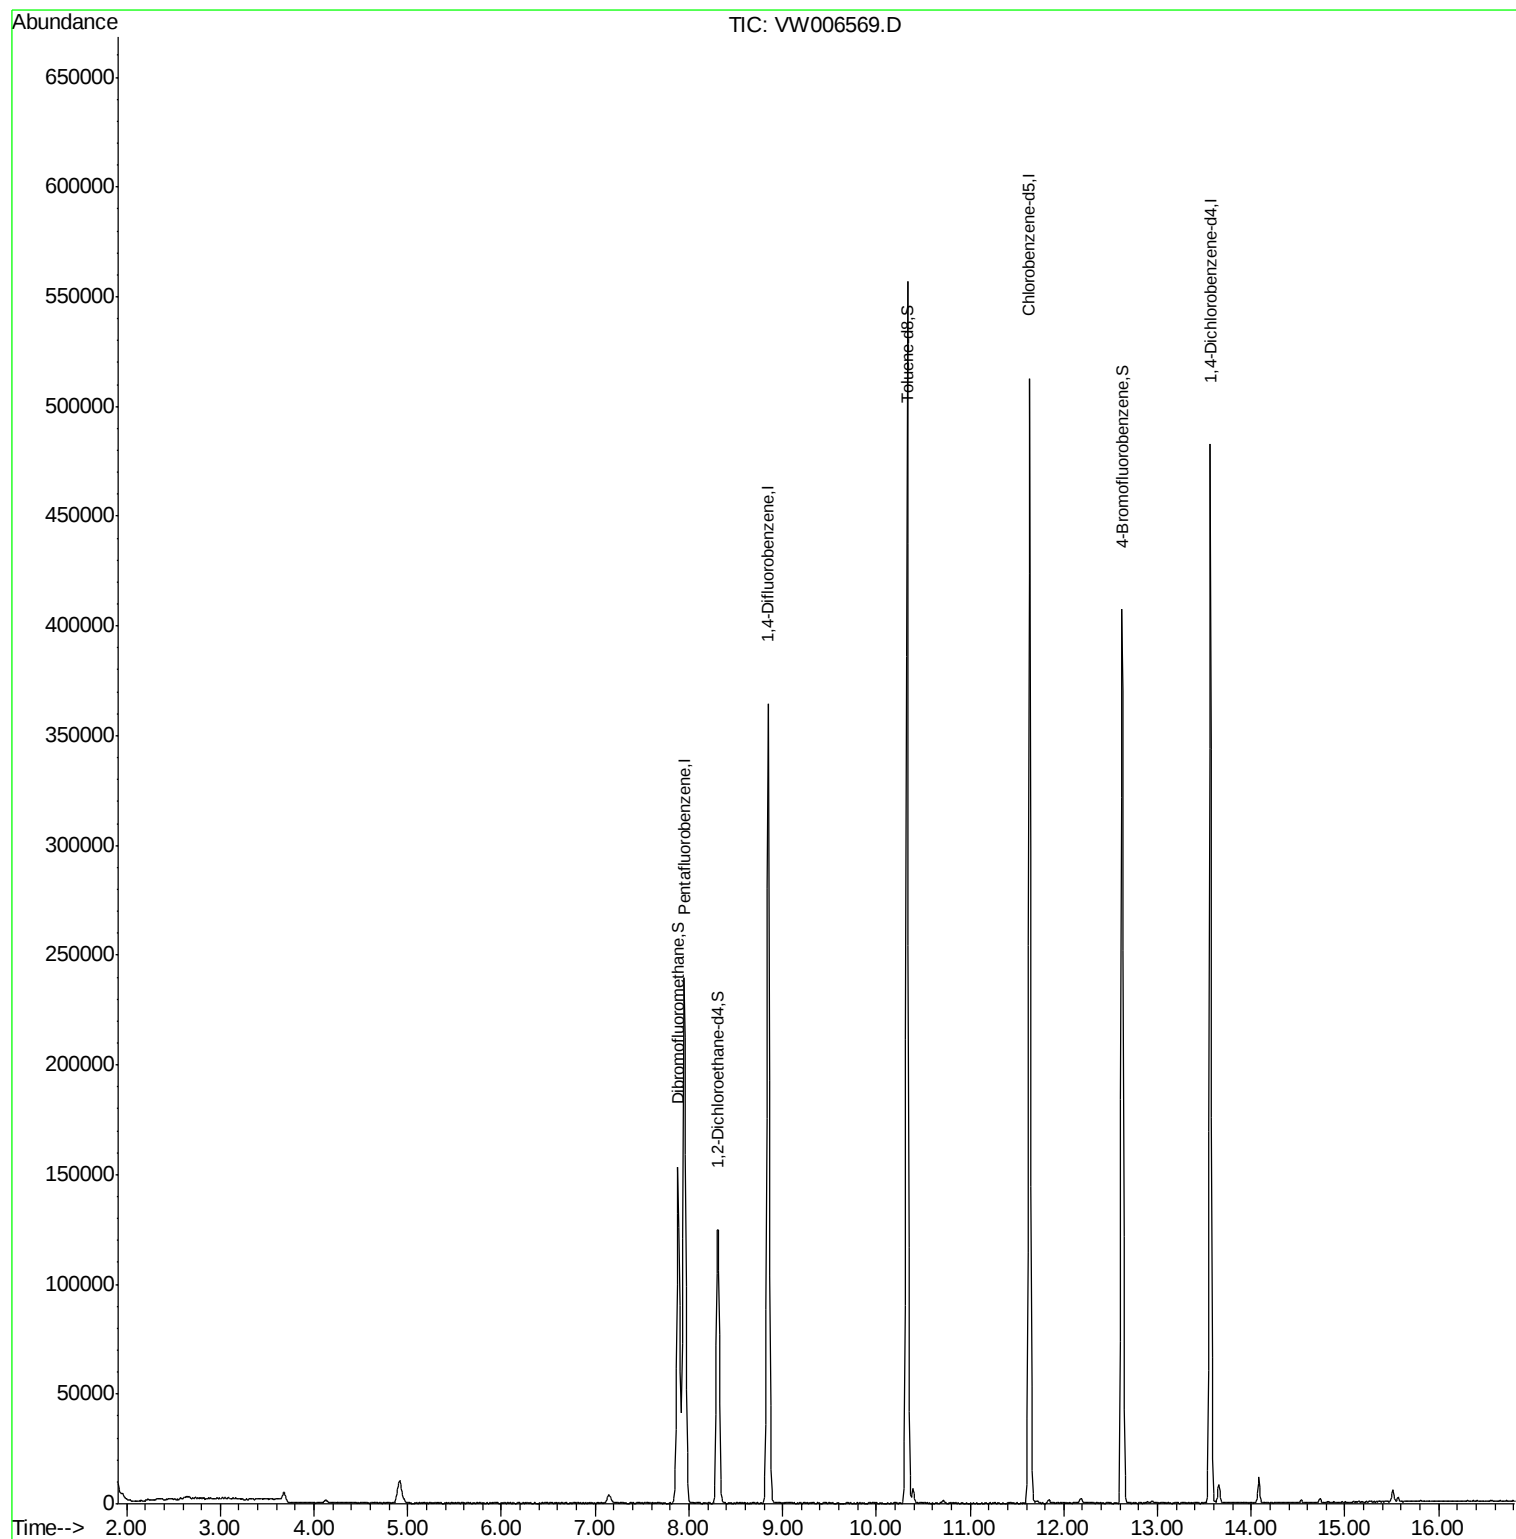

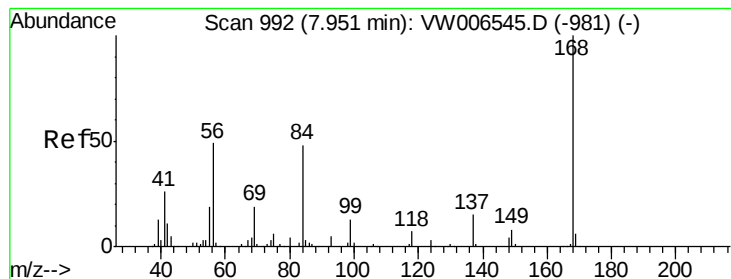

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006569.D

Acq: 01 Nov 2018 19:33

Instrument :

MSVOA_W

ClientSampleId :


SI-1

Tot Ion:168 Resp: 197109

Ion Ratio Lower Upper

168 100

99 47.3 37.4 56.0

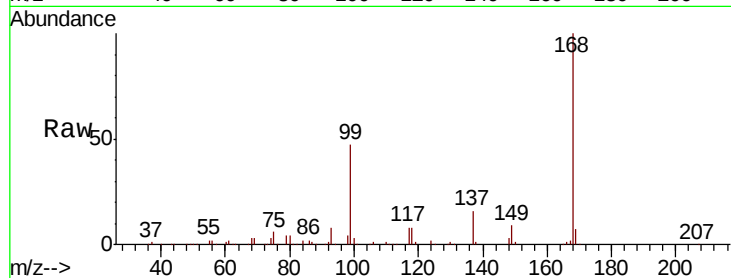

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time-->

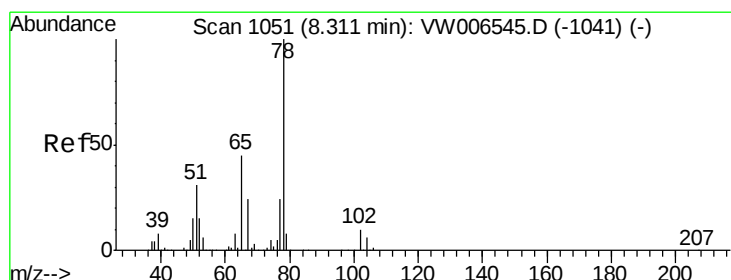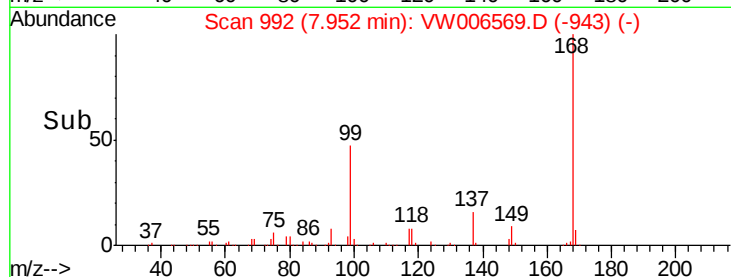

#33

1,2-Dichloroethane-d4

Concen: 61.118 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.01 min

Lab File: VW006569.D


Acq: 01 Nov 2018 19:33

Tgt Ion: 65 Resp: 103554

Ion Ratio Lower Upper

65 100

67 50.7 0.0 104.4

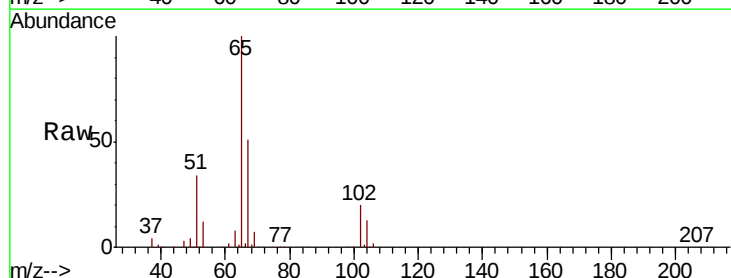

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

50000

40000


30000


20000

10000

0

Time-->




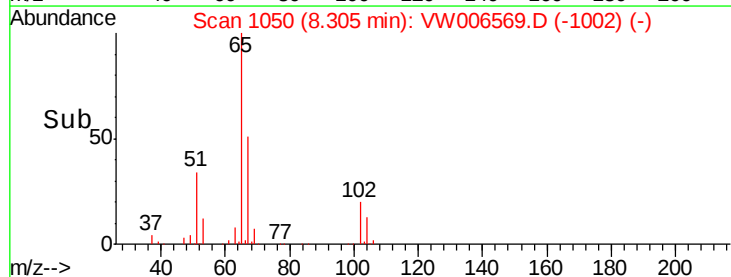


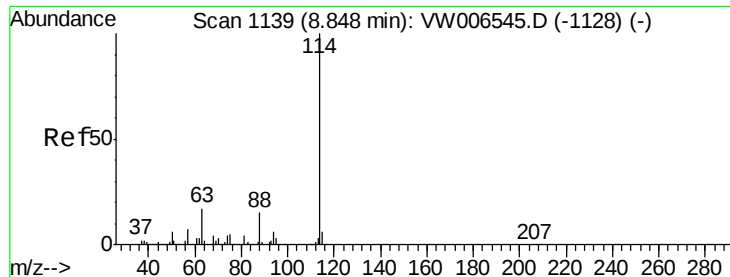

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006569.D
 Acq: 01 Nov 2018 19:33




Instrument :
 MSVOA_W
 ClientSampleId :
 SI-1


Tot Ion:114 Resp: 330398
 Ion Ratio Lower Upper
 114 100
 63 17.9 0.0 34.4
 88 14.5 0.0 29.0

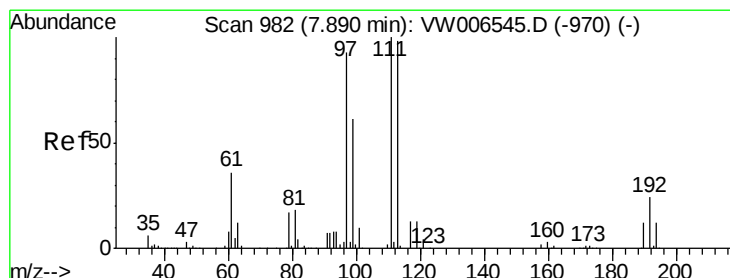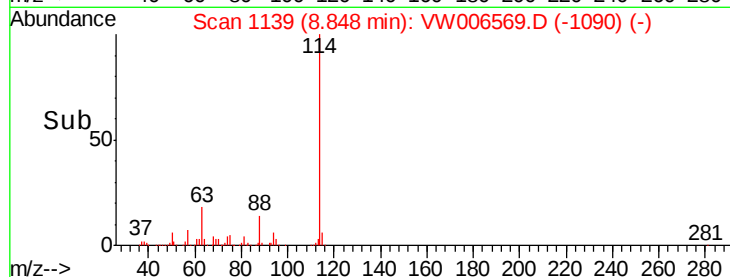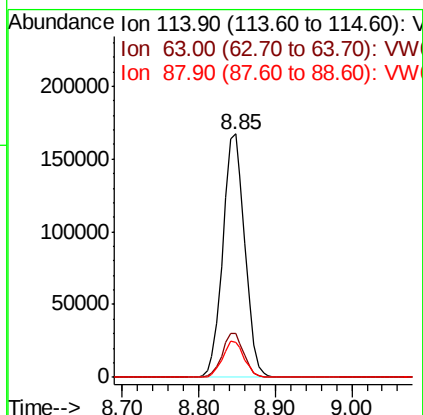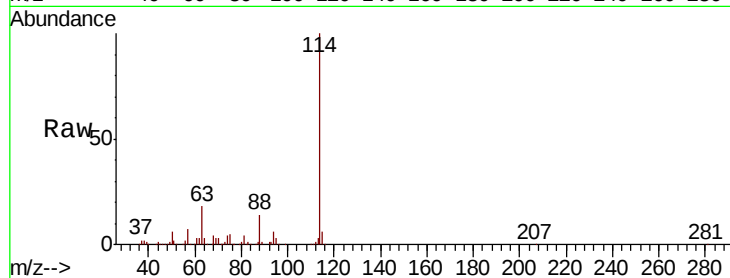

#35
 Dibromofluoromethane
 Concen: 51.534 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.01 min
 Lab File: VW006569.D
 Acq: 01 Nov 2018 19:33

Tgt Ion:113 Resp: 106856
 Ion Ratio Lower Upper
 113 100
 111 102.1 82.2 123.2
 192 24.1 19.0 28.6

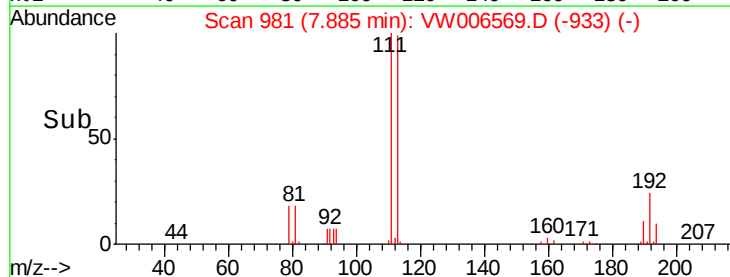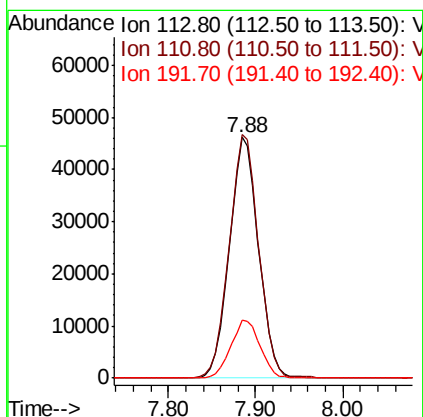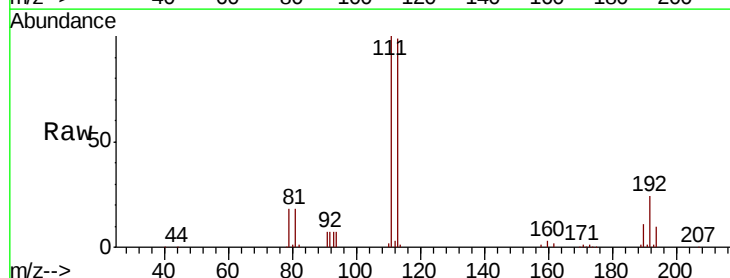

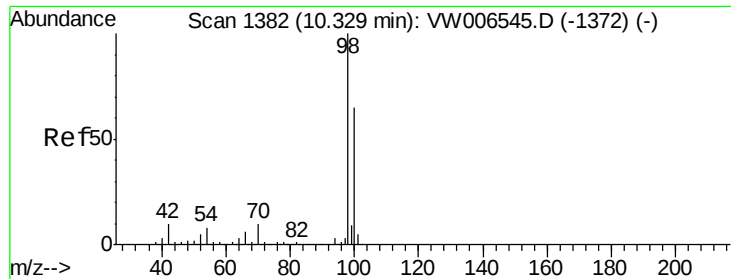

#50

Toluene-d8

Concen: 48.963 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW006569.D

Acq: 01 Nov 2018 19:33

Instrument :

MSVOA_W

ClientSampleId :





SI-1

Tot Ion: 98 Resp: 386486

Ion Ratio Lower Upper

98 100

100 64.0 51.6 77.4

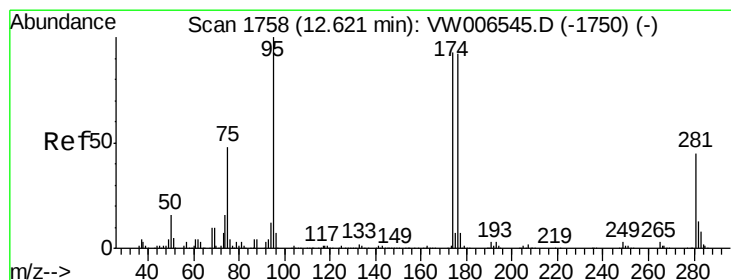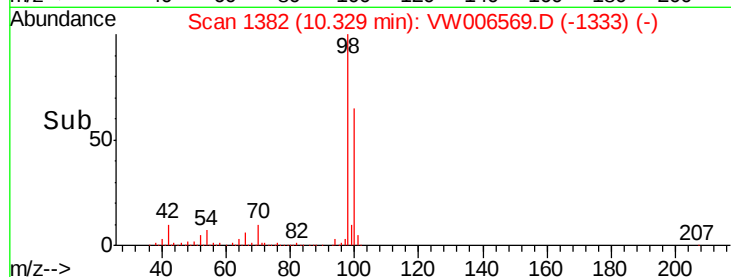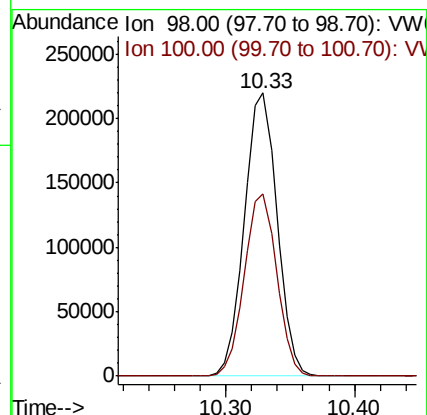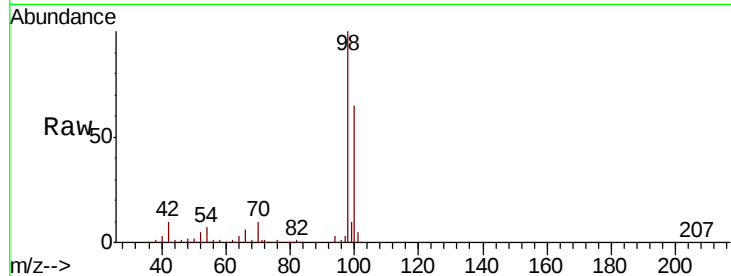

#62

4-Bromofluorobenzene

Concen: 43.348 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006569.D

Acq: 01 Nov 2018 19:33




Tgt Ion: 95 Resp: 124049


Ion Ratio Lower Upper

95 100

174 98.6 0.0 192.4

176 96.4 0.0 187.4

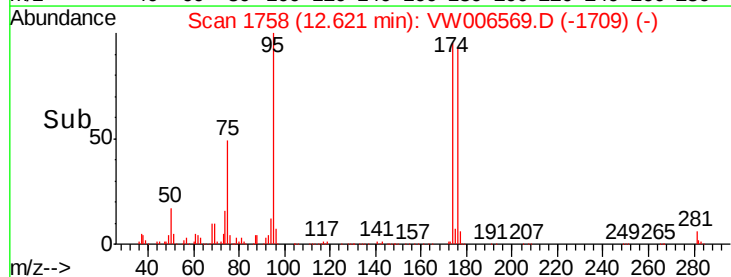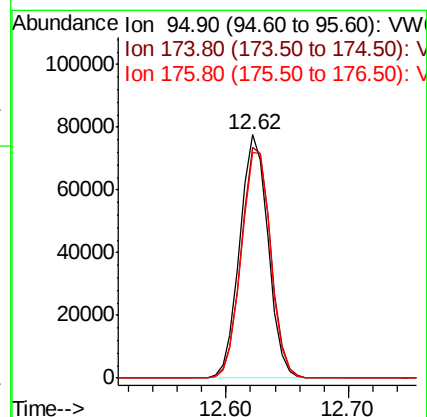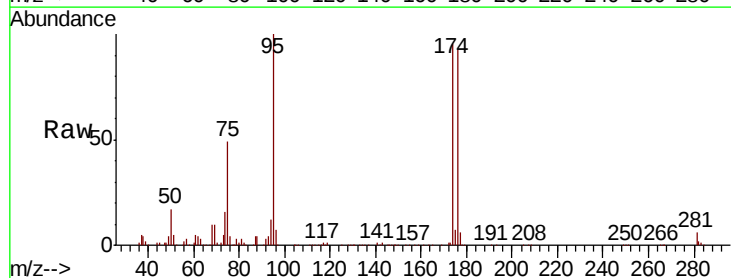


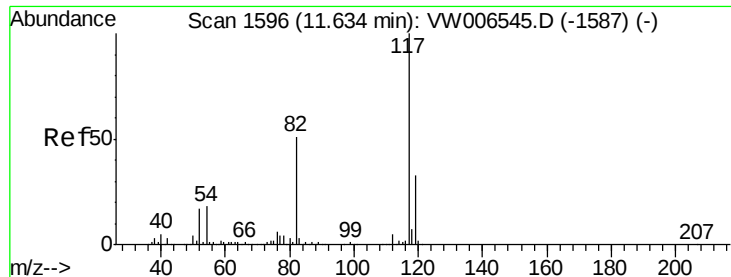

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW006569.D
Acq: 01 Nov 2018 19:33

Instrument :
MSVOA_W
ClientSampled :
SI-1

Tot Ion	Ratio	Lower	Upper
117	100		
82	50.4	40.8	61.2
119	32.9	26.1	39.1



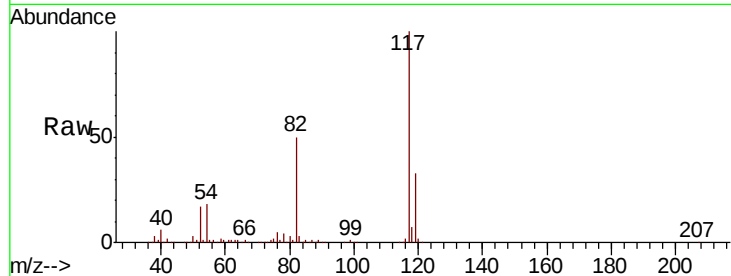


Abundance

Ion 116.90 (116.60 to 117.60): V


Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

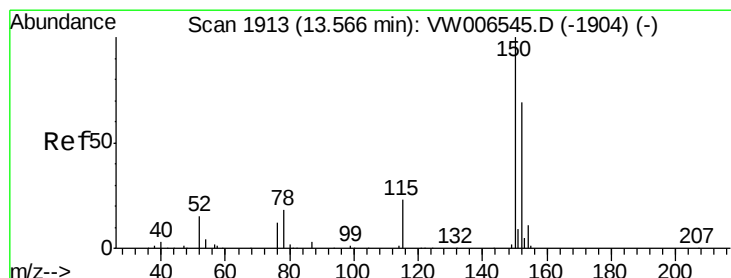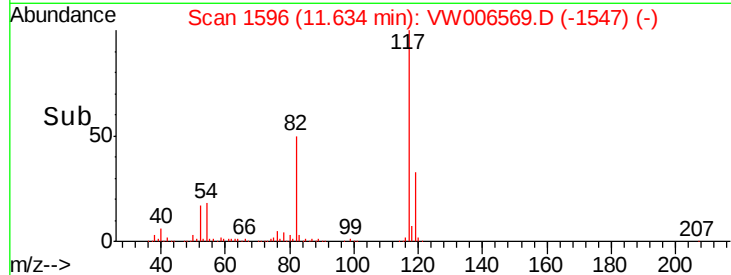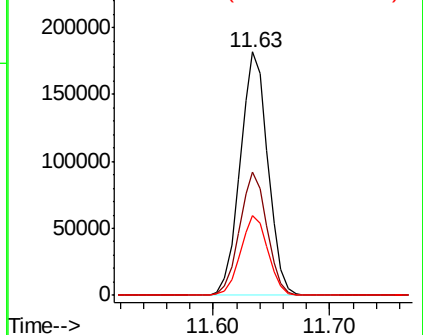

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. 0.00 min
Lab File: VW006569.D
Acq: 01 Nov 2018 19:33

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.4	26.6	79.8
150	157.0	0.0	344.6

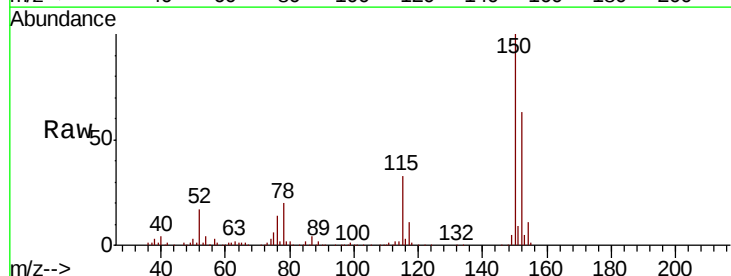

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

