


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110218\
Data File : VW006550.D
Acq On : 01 Nov 2018 09:29
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Title : SW846 8260
Last Update : Thu Nov 01 03:48:08 2018

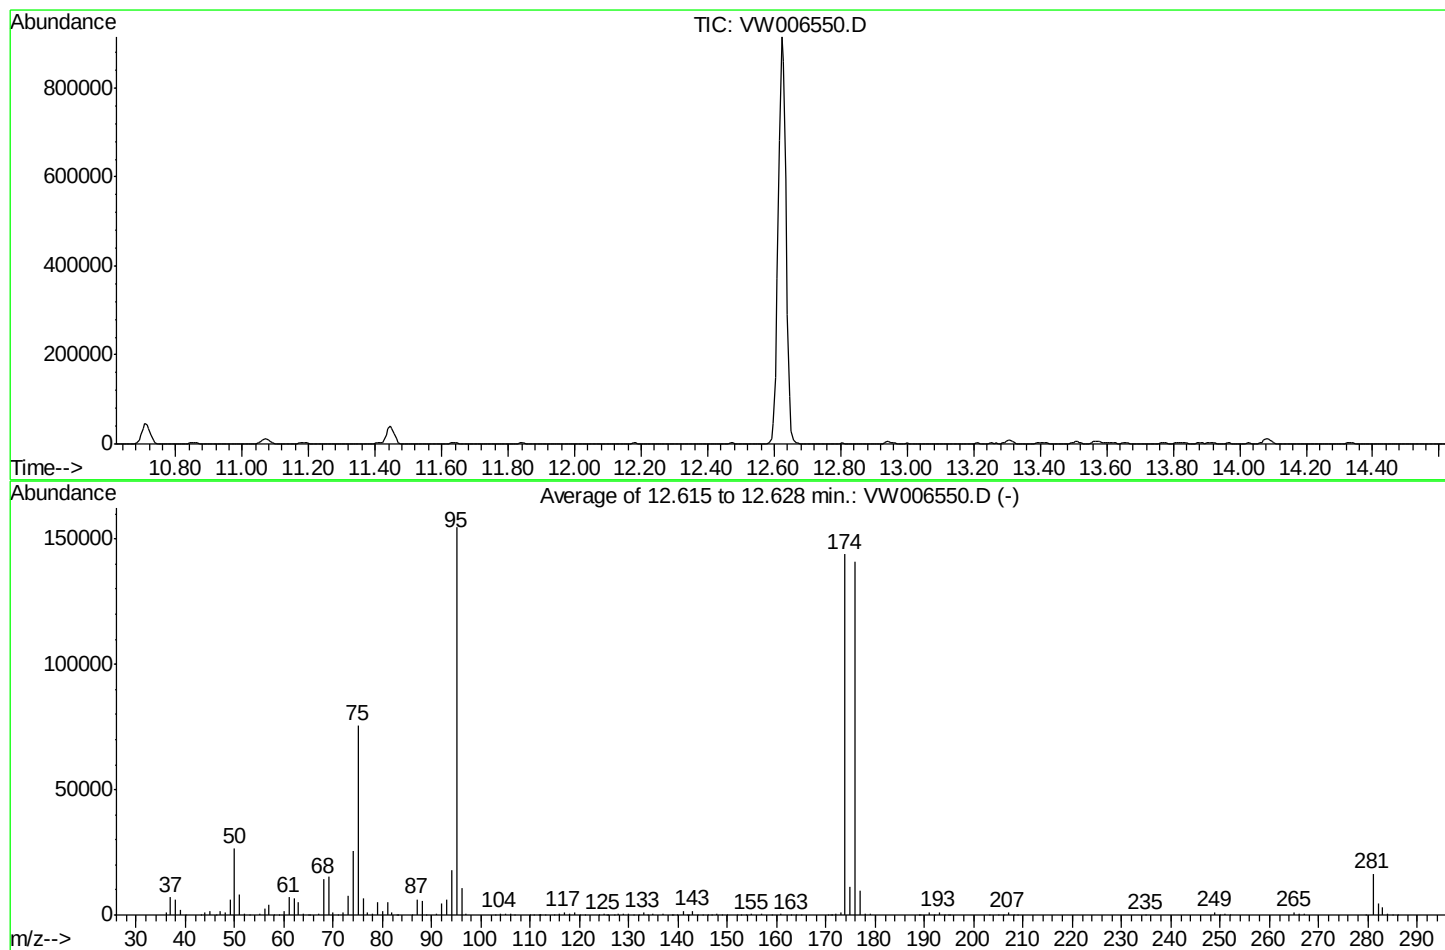

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	26341	PASS
75	95	30	60	48.7	75376	PASS
95	95	100	100	100.0	154637	PASS
96	95	5	9	6.9	10662	PASS
173	174	0.00	2	0.8	1121	PASS
174	95	50	100	93.1	143928	PASS
175	174	5	9	7.7	11081	PASS
176	174	95	101	97.9	140946	PASS
177	176	5	9	6.9	9662	PASS