

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110920\
 Data File : VW017114.D
 Acq On : 09 Nov 2020 11:23
 Operator : SY/VA
 Sample : VW1109SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK26

Quant Time: Nov 10 08:03:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 10 07:51:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	462276	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	432857	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	208072	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	141761	24.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.40%
7) Chloroethane-d5	2.89	69	112094	24.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.92%
10) 1,1-Dichloroethene-d2	4.02	63	180970	17.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.52%
20) 2-Butanone-d5	7.08	46	66165	50.81	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.62%
24) Chloroform-d	7.65	84	268639	24.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.56%
26) 1,2-Dichloroethane-d4	8.30	65	141700	26.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.64%
29) Benzene-d6	8.27	84	529838	24.04	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.16%
33) 1,2-Dichloropropane-d6	9.27	67	152299	24.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.92%
37) Toluene-d8	10.32	98	490256	23.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.36%
38) trans-1,3-Dichloropropene-	10.58	79	65197	23.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.88%
39) 2-Hexanone-d5	10.93	63	51708	48.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.20%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	136590	25.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	187114	25.52	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.08%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	7948	1.275 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110920\
Data File : VW017114.D
Acq On : 09 Nov 2020 11:23
Operator : SY/VA
Sample : VW1109SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK26

Quant Time: Nov 10 08:03:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 10 07:51:56 2020
Response via : Initial Calibration

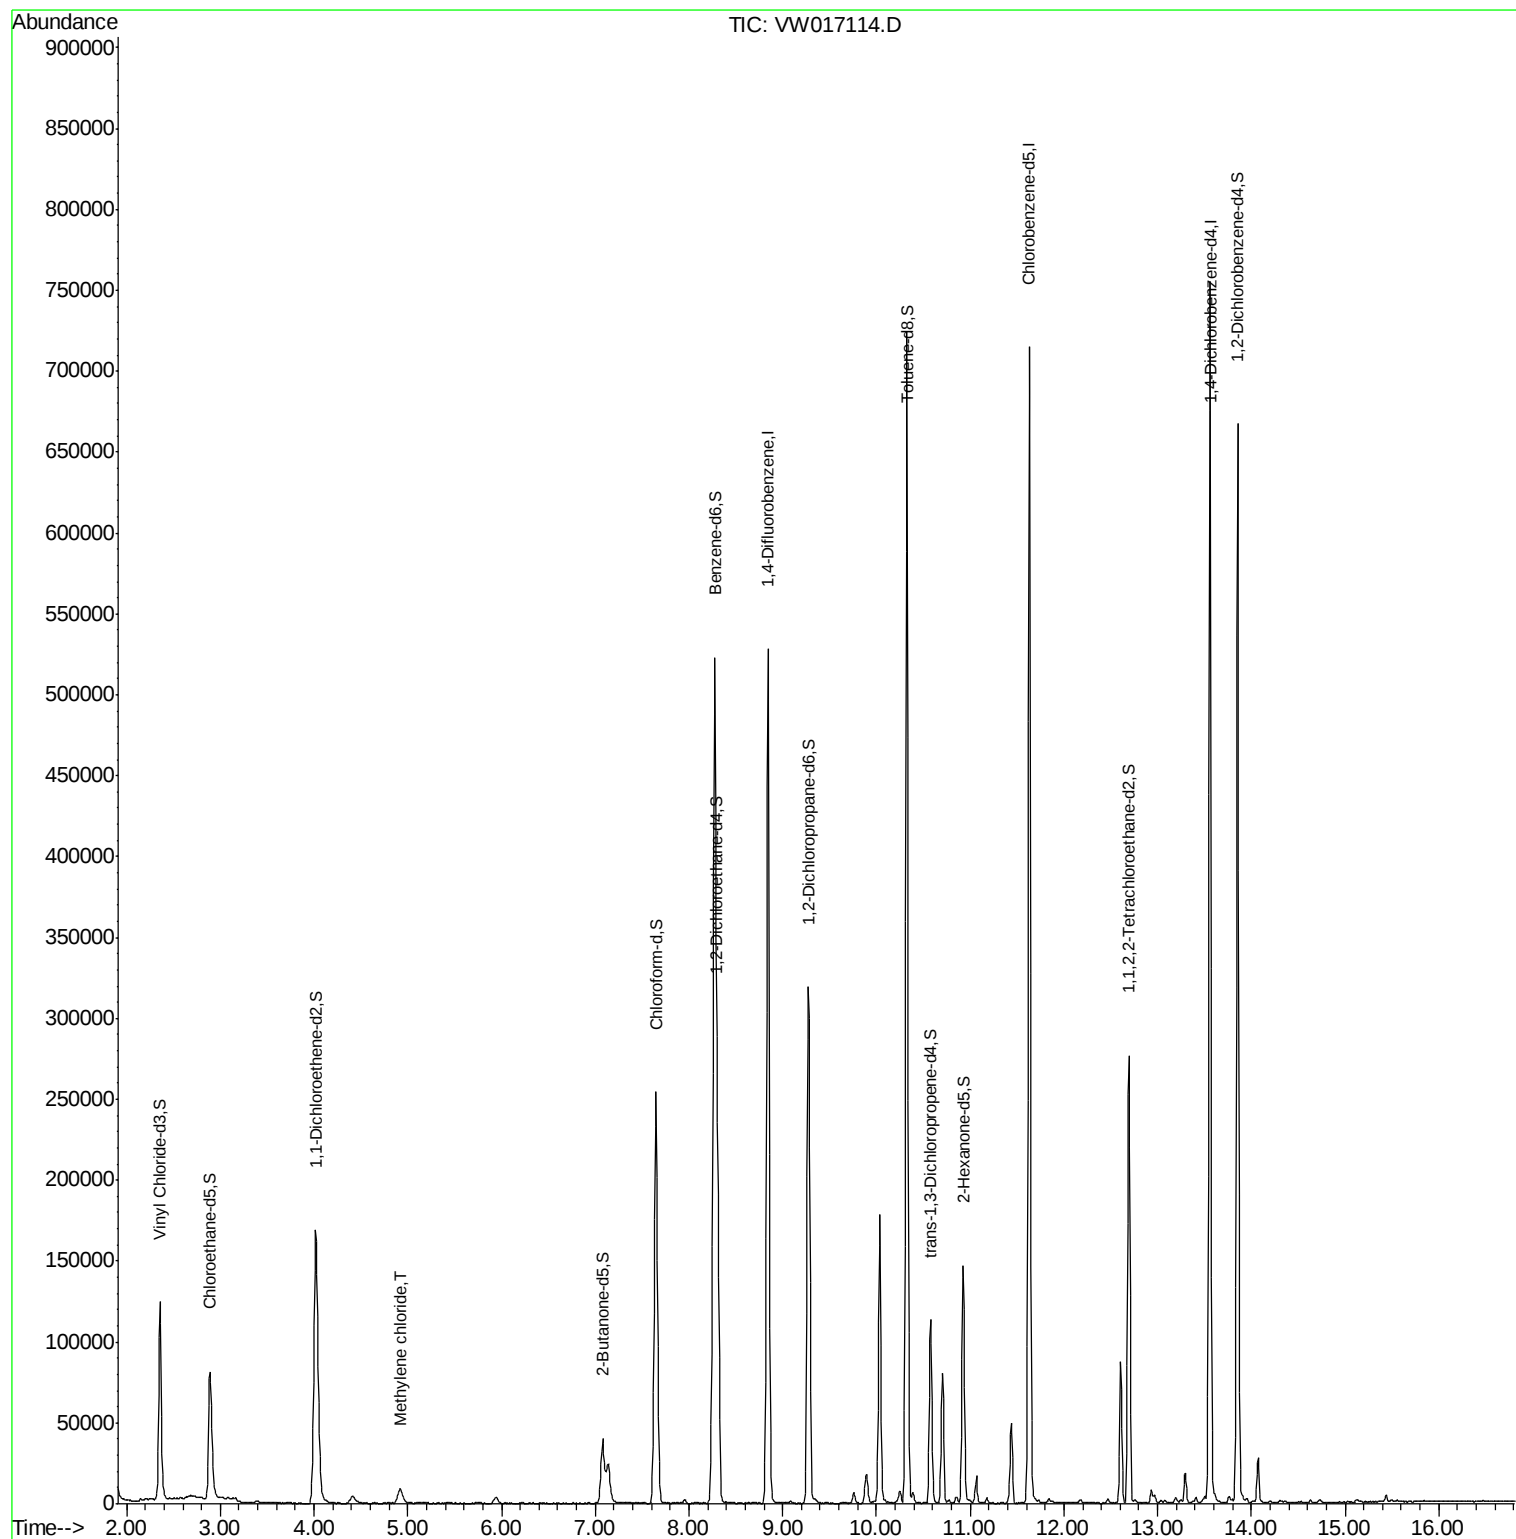

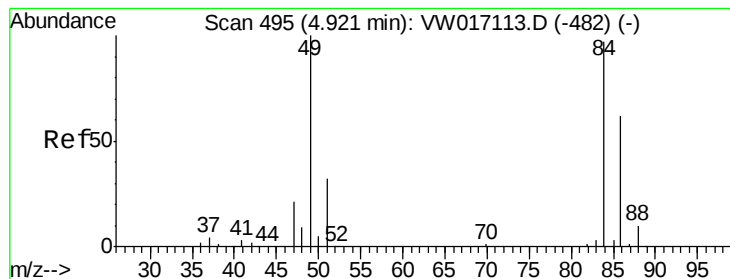

#16
 Methvlene chloride
 Concen: 1.275 ug/L
 RT: 4.92 min Scan# 495
 Delta R.T. -0.00 min
 Lab File: VW017114.D
 Acq: 09 Nov 2020 11:23

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK26

Tot Ion: 84 Resp: 7948
 Ion Ratio Lower Upper
 84 100
 49 111.9 72.3 134.3
 86 62.5 45.1 83.7

