


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110920\
 Data File : VW017112.D
 Acq On : 09 Nov 2020 09:34
 Operator : SY/VA
 Sample : BFB01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB01

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Title : VOC Analysis
 Last Update : Wed Nov 11 06:41:07 2020

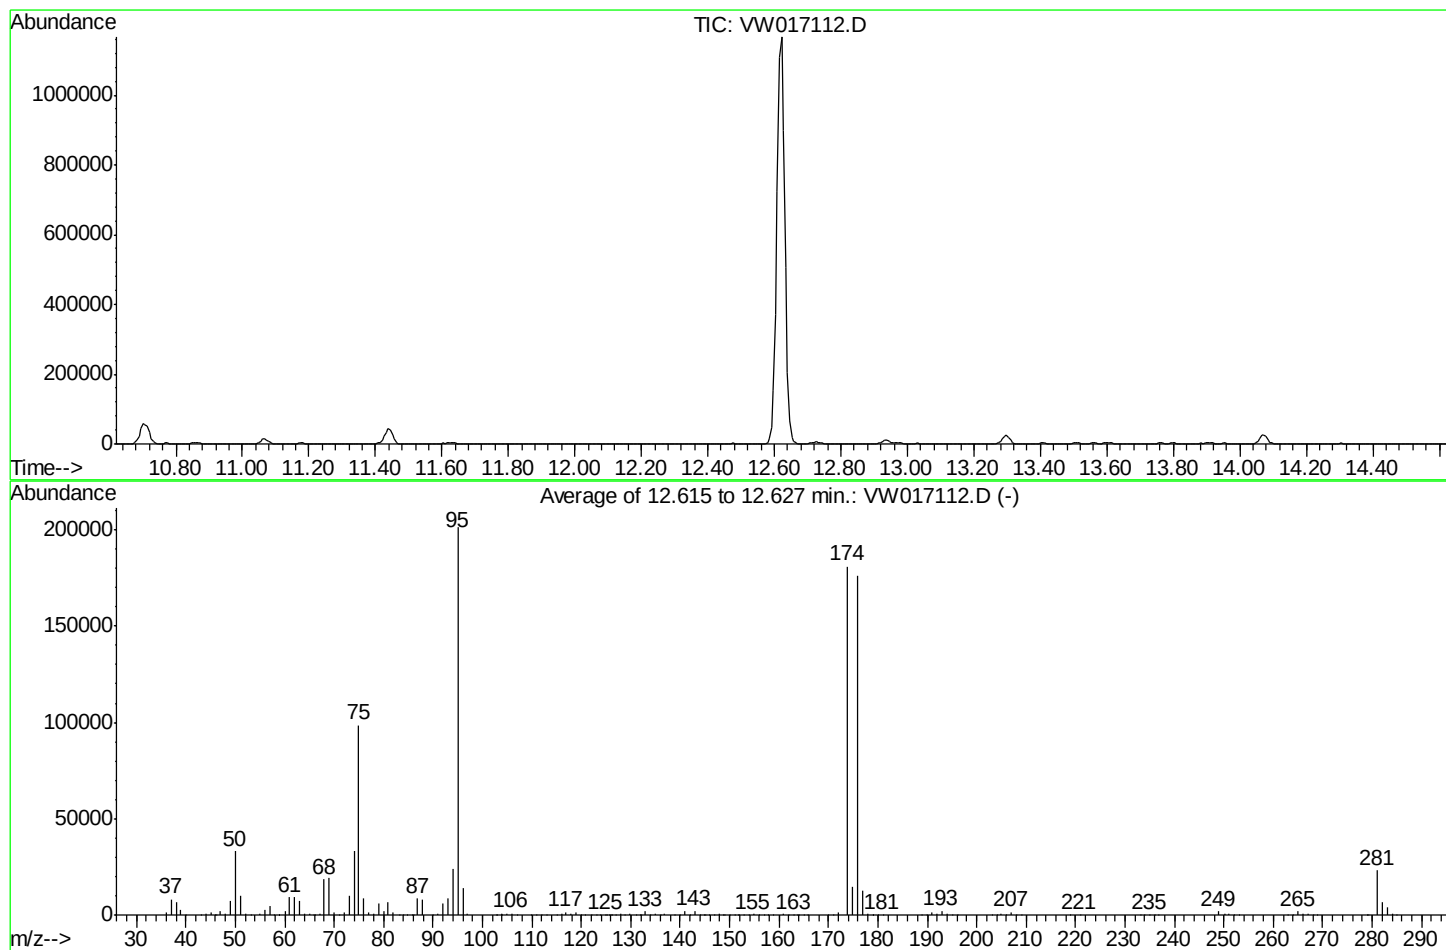

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	33186	PASS
75	95	30	80	49.0	98653	PASS
95	95	100	100	100.0	201258	PASS
96	95	5	9	6.9	13841	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.0	181034	PASS
175	174	5	9	7.9	14353	PASS
176	174	95	101	97.3	176149	PASS
177	176	5	9	7.0	12389	PASS

m/z	Abundance
36.00	1432.0
37.00	8915.0
38.00	7868.0
39.00	3027.0
40.00	294.0
42.90	174.0
44.00	1456.0
45.00	1937.0
46.00	165.0
47.00	1779.0
48.00	1030.0
49.00	7899.0
50.00	36640.0
51.00	10631.0
52.00	572.0
53.10	118.0
55.10	492.0
56.00	3182.0
57.00	5427.0
57.90	263.0
59.00	389.0
60.00	1992.0
61.00	9832.0
62.00	9865.0
63.00	7657.0
64.00	665.0
65.00	686.0
66.10	149.0
67.10	503.0
68.00	19768.0
69.00	20672.0
70.00	1678.0
70.90	129.0
72.00	1122.0
73.00	11914.0
74.00	35368.0
75.00	106128.0
76.00	9082.0
77.00	1309.0
78.00	754.0
78.90	6807.0
79.90	2097.0
80.90	6850.0
81.90	1469.0
83.00	223.0
84.80	68.0
85.80	233.0
86.90	8973.0
88.00	9034.0
89.80	88.0
90.90	840.0
91.90	6272.0
93.00	9711.0
94.00	25680.0
95.00	206208.0
96.00	14997.0
97.00	473.0
102.80	505.0
103.00	516.0
103.80	941.0
105.10	485.0
105.90	898.0
106.90	270.0
109.90	264.0
110.80	314.0
111.90	189.0
112.80	178.0
114.90	379.0
116.00	781.0
117.00	1640.0
117.90	1183.0
119.00	1535.0
119.80	110.0
120.70	89.0
121.90	129.0
124.10	176.0
124.80	869.0
125.70	387.0
125.90	374.0
126.90	131.0
127.90	916.0
128.90	278.0
129.90	643.0
130.90	476.0
131.80	140.0
133.00	3023.0
133.90	682.0
134.90	740.0
136.10	117.0
136.90	401.0
138.90	93.0
140.00	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

140.90	1890.0
142.10	271.0
142.90	2268.0
143.90	164.0
144.90	398.0
146.00	335.0
146.90	481.0
147.90	572.0
149.10	395.0
149.90	283.0
150.90	73.0
151.70	127.0
153.00	161.0
154.00	85.0
154.90	420.0
156.00	165.0
156.90	303.0
157.90	120.0
158.80	341.0
161.00	492.0
161.80	84.0
163.00	632.0
163.80	94.0
164.90	451.0
165.90	66.0
170.00	51.0
171.00	274.0
171.90	1554.0
173.90	172608.0
175.00	13305.0
175.90	166528.0
176.90	12820.0
178.00	437.0
178.90	515.0
180.00	207.0
181.00	68.0
188.90	291.0
189.90	189.0
191.10	2470.0
191.90	619.0
192.90	3485.0
194.10	815.0
195.00	323.0
196.00	64.0
202.90	358.0
204.00	81.0
204.90	726.0
206.00	186.0
207.00	2310.0
208.00	398.0
209.00	282.0
218.90	106.0
220.90	140.0
233.80	58.0
234.90	302.0
236.00	86.0
236.80	86.0
249.00	2583.0
250.10	677.0
250.90	993.0
252.00	299.0
253.00	168.0
262.80	61.0
263.90	83.0
265.00	2998.0
265.90	770.0
267.10	630.0
268.00	158.0
268.90	114.0
279.20	249.0
281.10	35688.0
282.00	9141.0
283.00	5553.0
284.10	1054.0
285.00	300.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

m/z	Abundance
35.90	1756.0
37.00	8894.0
38.00	7491.0
39.00	2661.0
40.00	217.0
43.00	220.0
44.10	1223.0
45.10	1468.0
46.20	240.0
47.00	2408.0
47.90	1006.0
49.00	8022.0
50.00	36232.0
51.00	11145.0
52.00	375.0
53.10	103.0
55.00	582.0
56.00	3212.0
57.00	5176.0
57.90	244.0
58.90	204.0
60.00	1953.0
61.00	10135.0
62.00	10546.0
63.00	7956.0
64.00	957.0
65.10	510.0
65.80	88.0
67.00	576.0
68.00	20648.0
69.00	21976.0
70.00	1781.0
70.90	77.0
71.90	1248.0
73.00	11243.0
74.00	36912.0
75.00	110528.0
76.00	9687.0
76.90	1388.0
77.90	820.0
78.90	6985.0
79.90	1943.0
80.90	6684.0
81.90	1637.0
83.00	224.0
83.90	61.0
85.80	224.0
86.90	9406.0
87.90	8636.0
90.90	976.0
92.00	6537.0
93.00	9332.0
94.00	26160.0
95.00	227136.0
96.00	15468.0
96.90	578.0
102.90	337.0
104.00	1123.0
105.00	346.0
105.90	1155.0
106.80	243.0
110.00	315.0
110.90	324.0
112.00	263.0
112.90	239.0
114.80	366.0
115.90	805.0
116.90	1465.0
117.80	861.0
118.90	1419.0
119.90	63.0
120.70	63.0
121.90	156.0
123.00	60.0
123.90	152.0
125.00	682.0
126.20	92.0
126.90	74.0
127.90	811.0
128.80	464.0
129.80	882.0
131.00	372.0
131.70	68.0
132.10	86.0
133.00	1923.0
135.00	423.0
136.10	126.0
136.80	384.0
138.90	89.0
140.90	2283.0
141.90	400.0
143.00	2742.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

143.90	158.0
144.90	317.0
145.90	294.0
146.90	383.0
148.00	640.0
148.80	242.0
149.80	382.0
151.90	118.0
152.90	240.0
153.90	153.0
154.80	671.0
155.90	128.0
156.90	463.0
157.80	103.0
158.90	291.0
160.80	534.0
163.10	315.0
164.00	119.0
164.90	207.0
171.10	250.0
171.90	1316.0
173.90	200576.0
174.90	16305.0
176.00	194112.0
176.90	13967.0
177.90	540.0
179.10	404.0
180.10	91.0
188.90	233.0
190.90	1727.0
192.00	400.0
193.00	2075.0
194.10	521.0
195.10	200.0
203.00	231.0
204.00	69.0
205.00	361.0
205.90	114.0
207.00	1382.0
208.00	346.0
208.90	179.0
218.80	91.0
220.90	115.0
235.00	247.0
236.00	86.0
236.90	66.0
249.00	2110.0
250.10	359.0
251.00	575.0
251.80	116.0
252.90	56.0
265.10	1983.0
266.00	323.0
267.10	418.0
267.90	52.0
269.00	72.0
278.90	98.0
281.10	22112.0
282.10	6727.0
283.00	3504.0
284.00	744.0
285.00	313.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

m/z	Abundance
36.00	1225.0
37.00	6583.0
38.00	4988.0
39.00	2337.0
39.90	227.0
40.90	65.0
43.10	93.0
44.00	937.0
45.00	1135.0
46.10	137.0
47.00	1675.0
47.90	922.0
49.00	5661.0
50.00	26688.0
51.00	8131.0
52.00	318.0
55.00	359.0
56.00	2180.0
57.00	3923.0
58.00	112.0
58.70	133.0
60.00	1358.0
61.00	7290.0
62.00	6938.0
63.00	5603.0
64.00	632.0
64.90	458.0
65.80	55.0
66.90	341.0
68.00	14858.0
69.00	16063.0
70.00	1302.0
71.00	98.0
71.90	983.0
73.00	7443.0
74.00	27888.0
75.00	79304.0
76.00	6776.0
76.90	1054.0
77.90	654.0
78.90	4992.0
80.00	1463.0
80.90	5593.0
82.00	1239.0
83.10	176.0
86.00	165.0
86.90	7527.0
87.90	6355.0
90.90	679.0
92.00	4901.0
93.00	7368.0
94.00	20848.0
95.00	170432.0
96.00	11058.0
97.00	288.0
102.80	223.0
103.90	829.0
104.90	351.0
105.90	743.0
107.00	216.0
109.80	200.0
110.90	254.0
111.80	152.0
112.80	180.0
115.00	179.0
116.00	555.0
117.00	1350.0
118.00	780.0
118.90	1089.0
119.90	52.0
122.00	64.0
123.00	61.0
123.80	146.0
125.10	304.0
126.10	141.0
126.90	59.0
127.80	730.0
128.90	284.0
130.00	575.0
130.90	226.0
131.80	55.0
133.00	785.0
134.00	118.0
134.90	341.0
136.90	407.0
139.00	101.0
140.00	227.0
141.00	1866.0
141.90	153.0
142.90	1996.0
144.00	158.0
145.10	208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

145.90	310.0
146.90	199.0
147.90	456.0
149.00	156.0
150.00	155.0
151.90	133.0
153.00	158.0
153.80	129.0
154.90	625.0
155.80	157.0
156.90	310.0
157.90	131.0
159.00	152.0
161.00	309.0
163.00	128.0
164.90	107.0
168.80	121.0
169.90	59.0
170.90	116.0
171.90	921.0
173.90	169920.0
175.00	13451.0
175.90	167808.0
176.90	10380.0
177.90	504.0
178.90	324.0
180.00	86.0
188.90	86.0
191.00	747.0
192.00	177.0
193.00	970.0
194.00	222.0
194.90	139.0
202.80	81.0
205.10	218.0
205.90	70.0
207.00	1041.0
208.00	150.0
209.00	92.0
221.00	54.0
233.00	53.0
235.00	133.0
248.90	726.0
250.10	224.0
251.10	292.0
251.90	118.0
252.80	83.0
265.00	979.0
266.10	262.0
266.90	219.0
268.00	56.0
281.10	11949.0
282.10	3733.0
283.10	2028.0
284.00	413.0
285.10	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01

Scan 1749 (12.566 min): VW017112.D
BFB01

m/z	Abundance
40.00	142.0
41.10	51.0
44.00	281.0
168.90	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB01