

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
Data File : VW017142.D
Acq On : 10 Nov 2020 16:00
Operator : SY/VA
Sample : VIBLK18
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK18

Manual Integrations
APPROVED

MMDadoda
11/12/2020 1:42:59 PM

Quant Time: Nov 11 05:40:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 11 05:30:56 2020
Response via : Initial Calibration

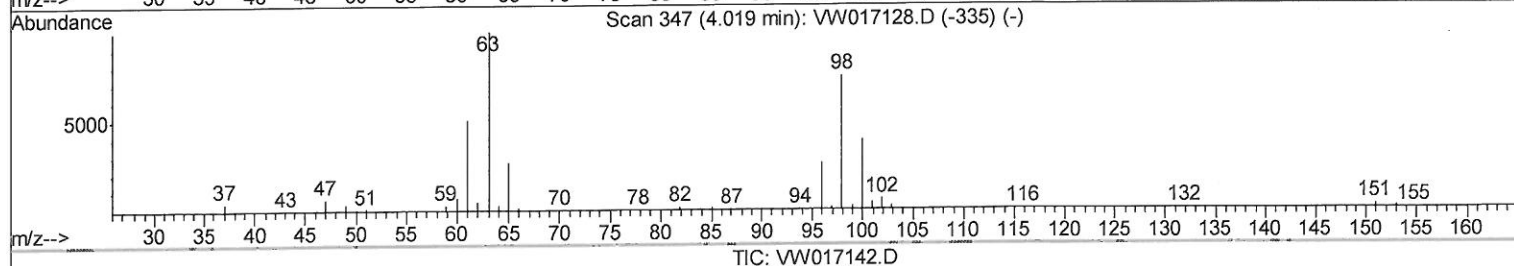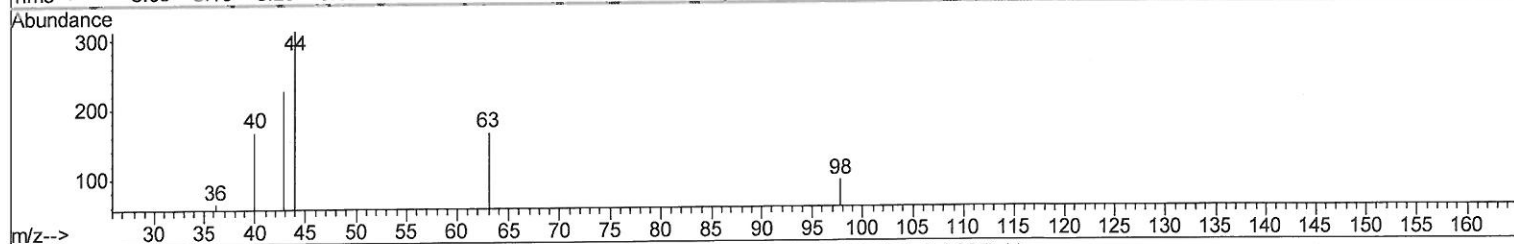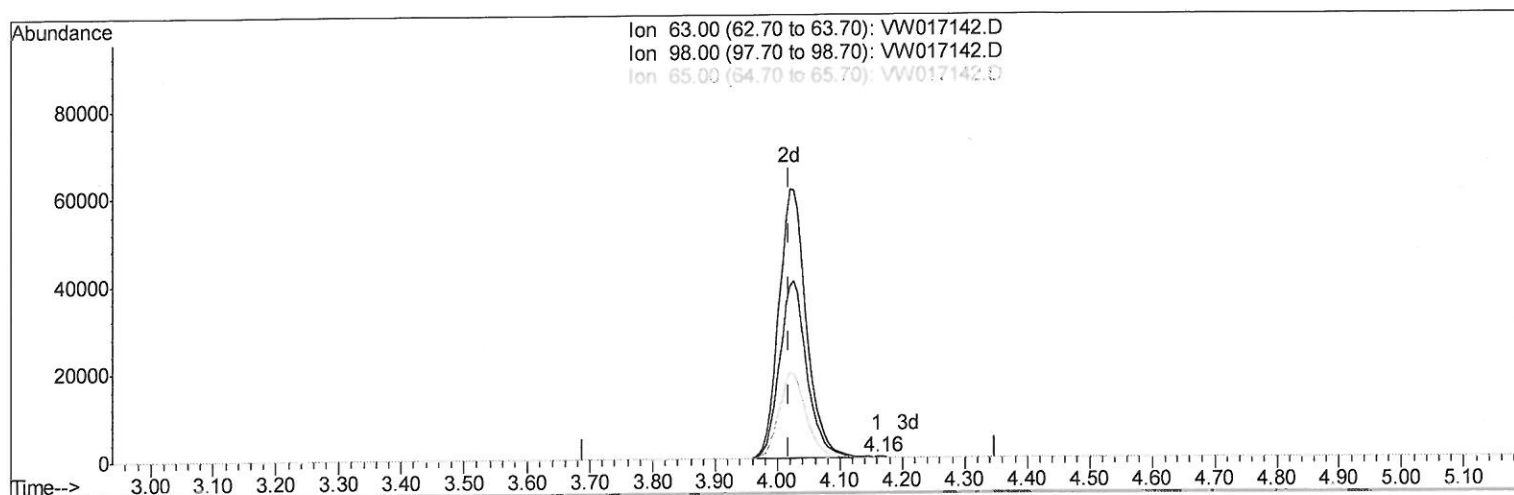

(10) 1,1-Dichloroethene-d2 (S)

4.159min (+0.140) 0.02ug/L

response 211

Ion	Exp%	Act%
63.00	100	100
98.00	83.10	66.82
65.00	24.20	24.64
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017142.D
 Acq On : 10 Nov 2020 16:00
 Operator : SY/VA
 Sample : VIBLK18
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK18

Manual Integrations
APPROVED

MMDadoda
 11/12/2020 1:42:59 PM

Quant Time: Nov 11 05:40:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

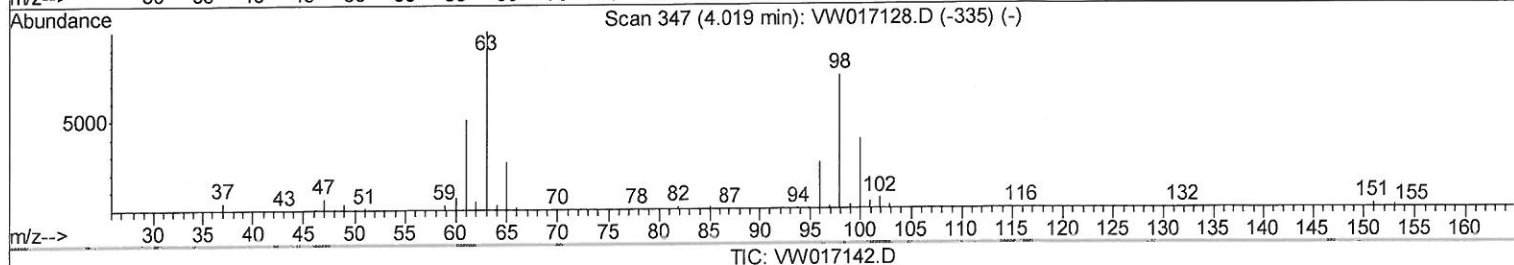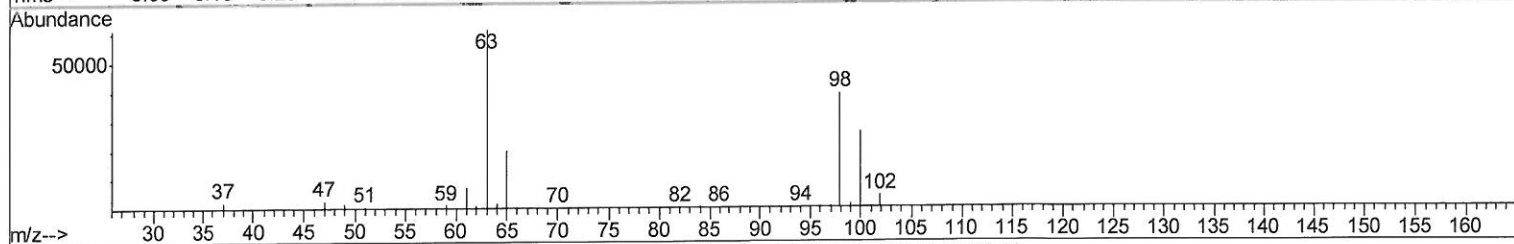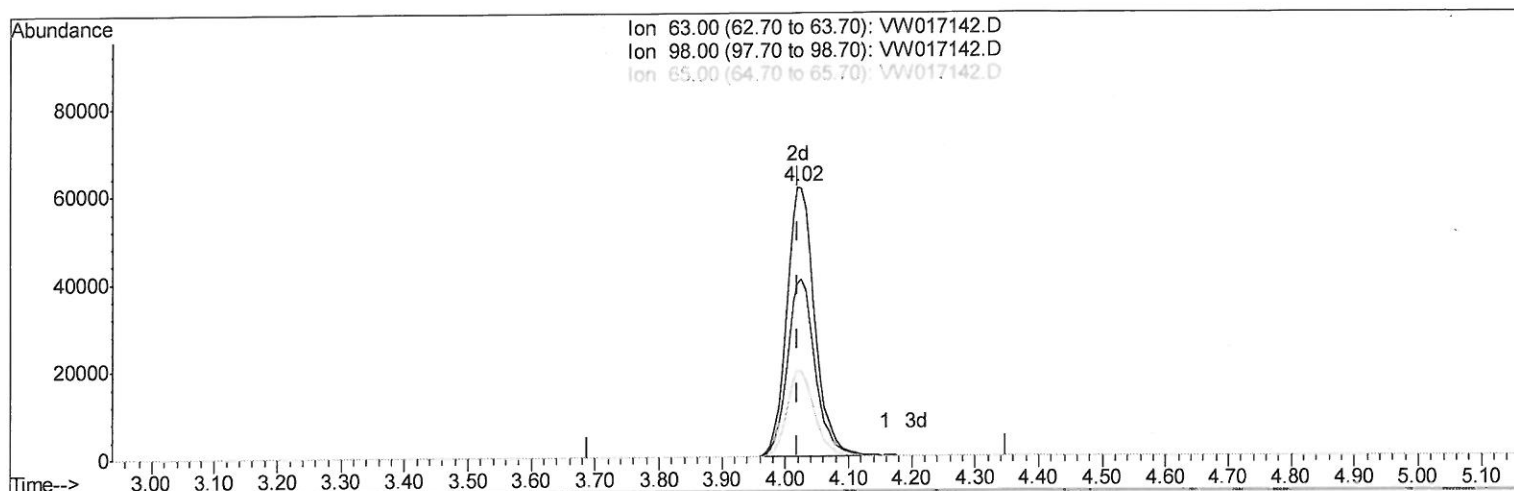

(10) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 19.56ug/L m

response 187885

Ion	Exp%	Act%
63.00	100	100
98.00	83.10	0.08#
65.00	24.20	0.03#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017142.D
 Acq On : 10 Nov 2020 16:00
 Operator : SY/VA
 Sample : VIBLK18
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK18

Manual Integrations
 APPROVED

MMDadoda
 11/12/2020 1:42:59 PM

Quant Time: Nov 11 06:22:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	426410	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	393337	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	181122	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	145841	27.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 108.60%	
7) Chloroethane-d5	2.90	69	119340	28.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 115.32%	
10) 1,1-Dichloroethene-d2	4.02	63	187885m	19.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 78.24%	
20) 2-Butanone-d5	7.09	46	52129	43.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 86.80%	
24) Chloroform-d	7.65	84	283020	28.43	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 113.72%	
26) 1,2-Dichloroethane-d4	8.31	65	138453	27.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 111.92%	
29) Benzene-d6	8.28	84	551292	27.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 110.08%	
33) 1,2-Dichloropropane-d6	9.28	67	156657	28.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 113.12%	
37) Toluene-d8	10.33	98	517986	27.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 109.72%	
38) trans-1,3-Dichloropropene-	10.58	79	61176	24.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 97.96%	
39) 2-Hexanone-d5	10.93	63	41519	42.94	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 85.88%	
48) 1,1,2,2-Tetrachloroethane-	12.69	84	119981	24.86	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 99.44%	
61) 1,2-Dichlorobenzene-d4	13.85	152	182632	28.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 114.48%	

11/18/2020

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
16) Methylene chloride	4.92	84	8337	1.450	ug/L	95
43) 4-Methyl-2-pentanone	10.21	43	2599	0.873	ug/L #	78
44) Toluene	10.39	91	5344	0.235	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
Data File : VW017142.D
Acq On : 10 Nov 2020 16:00
Operator : SY/VA
Sample : VIBLK18
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK18

Manual Integrations
APPROVED

MMDadoda
11/12/2020 1:42:59 PM

Quant Time: Nov 11 06:22:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 11 05:30:56 2020
Response via : Initial Calibration

