

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017145.D
 Acq On : 10 Nov 2020 17:11
 Operator : SY/VA
 Sample : L4659-19
 Misc : 5.54G/10ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4B9

Manual Integrations
 APPROVED

MMDadoda
 11/12/2020 1:43:01 PM

Quant Time: Nov 11 05:40:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

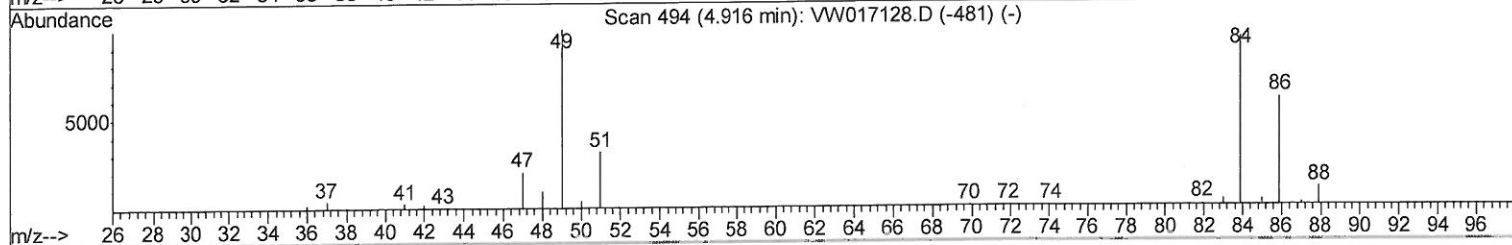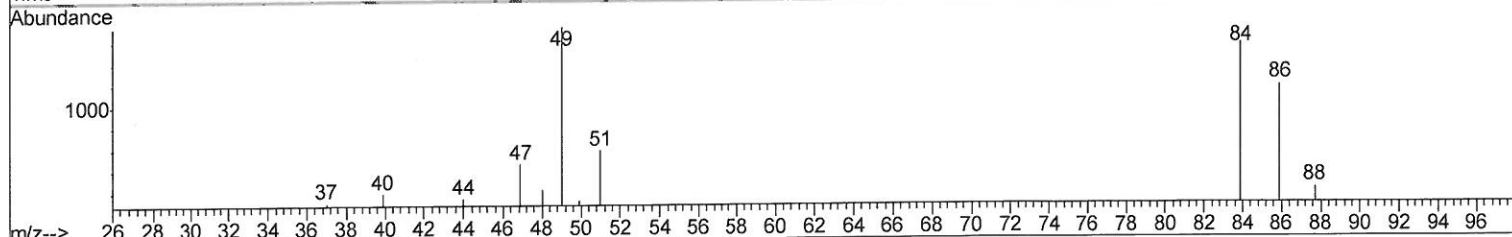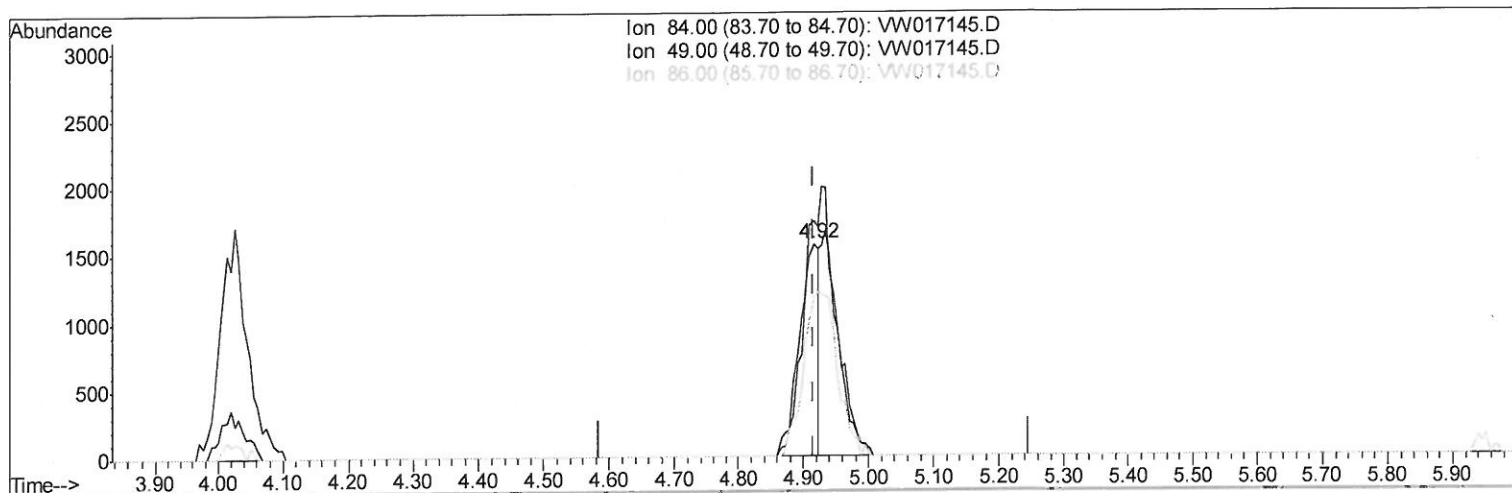

(16) Methylene chloride (T)

4.916min (0.000) 0.44ug/L

response 2883

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	110.97
86.00	64.40	74.74
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017145.D
 Acq On : 10 Nov 2020 17:11
 Operator : SY/VA
 Sample : L4659-19
 Misc : 5.54G/10ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4B9

Manual Integrations
 APPROVED

MMDadoda
 11/12/2020 1:43:01 PM

Quant Time: Nov 11 05:40:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

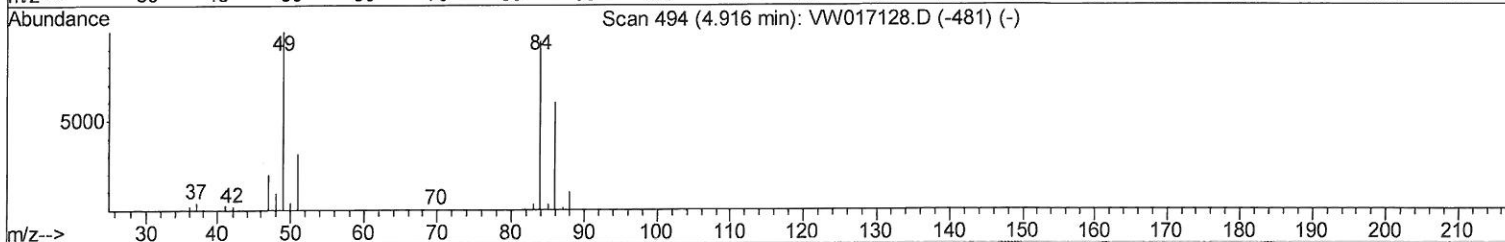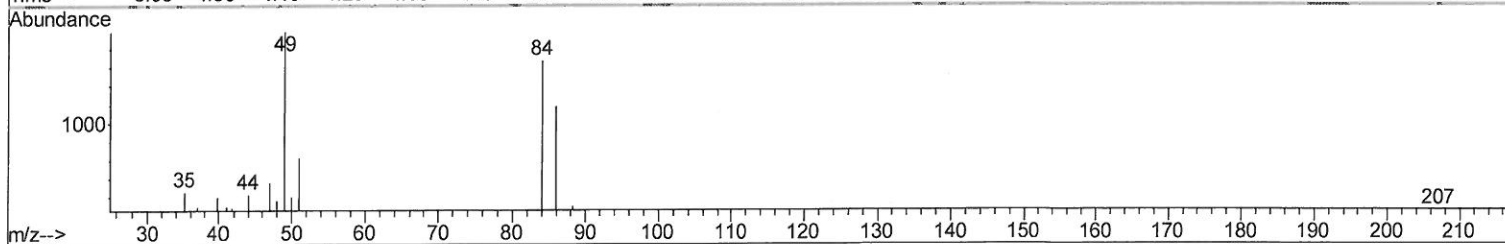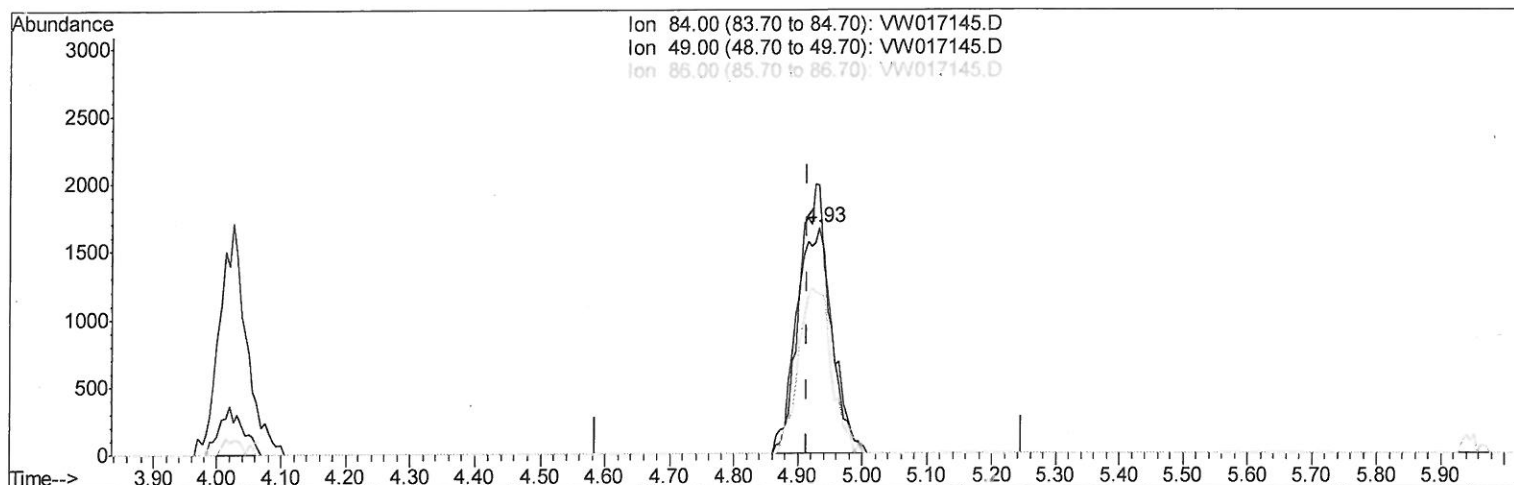

TIC: VW017145.D

(16) Methylene chloride (T)

4.934min (+0.018) 0.94ug/L m

> 11/18/2020

response 6092

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	118.92
86.00	64.40	70.90
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017145.D
 Acq On : 10 Nov 2020 17:11
 Operator : SY/VA
 Sample : L4659-19
 Misc : 5.54G/10ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4B9

Manual Integrations
 APPROVED

MMDadoda
 11/12/2020 1:43:01 PM

Quant Time: Nov 11 06:38:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	481425	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	435387	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	184166	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	139041	22.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.72%
7) Chloroethane-d5	2.90	69	114636	24.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.12%
10) 1,1-Dichloroethene-d2	4.02	63	183280	16.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.60%
20) 2-Butanone-d5	7.09	46	49238	36.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.62%
24) Chloroform-d	7.65	84	265694	23.64	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.56%
26) 1,2-Dichloroethane-d4	8.31	65	131901	23.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.44%
29) Benzene-d6	8.28	84	532425	24.01	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.04%
33) 1,2-Dichloropropane-d6	9.28	67	147922	24.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.48%
37) Toluene-d8	10.33	98	499564	23.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.60%
38) trans-1,3-Dichloropropene-	10.58	79	55851	20.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.80%
39) 2-Hexanone-d5	10.93	63	39511	36.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.84%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	109512	20.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	162837	25.10	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	6546	7.210	ug/L	92
14) Carbon disulfide	4.39	76	6863	0.422	ug/L	97
16) Methylene chloride	4.93	84	6092m	0.939	ug/L	97
43) 4-Methyl-2-pentanone	10.21	43	5091	1.544	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
Data File : VW017145.D
Acq On : 10 Nov 2020 17:11
Operator : SY/VA
Sample : L4659-19
Misc : 5.54G/10ML/MSVOA W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG4B9

Manual Integrations
APPROVED

MMDadoda
11/12/2020 1:43:01 PM

Quant Time: Nov 11 06:38:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 11 05:30:56 2020
Response via : Initial Calibration

