

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111020\
 Data File : VW017144.D
 Acq On : 10 Nov 2020 16:47
 Operator : SY/VA
 Sample : VIBLK19
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK19

Quant Time: Nov 11 06:31:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 05:30:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	421144	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	396915	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	178277	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	137262	25.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.52%
7) Chloroethane-d5	2.90	69	111289	27.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.92%
10) 1,1-Dichloroethene-d2	4.03	63	174229	18.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.44%
20) 2-Butanone-d5	7.09	46	45799	38.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.22%
24) Chloroform-d	7.65	84	260532	26.50	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	8.31	65	127029	25.99	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.96%
29) Benzene-d6	8.28	84	510440	25.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.00%
33) 1,2-Dichloropropane-d6	9.28	67	143014	25.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.32%
37) Toluene-d8	10.33	98	474074	24.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.48%
38) trans-1,3-Dichloropropene-	10.58	79	56188	22.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.16%
39) 2-Hexanone-d5	10.93	63	36582	37.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.98%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	106758	21.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.68%
61) 1,2-Dichlorobenzene-d4	13.85	152	170376	27.13	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.52%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	7554	1.330 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111020\
Data File : VW017144.D
Acq On : 10 Nov 2020 16:47
Operator : SY/VA
Sample : VIBLK19
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK19

Quant Time: Nov 11 06:31:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 11 05:30:56 2020
Response via : Initial Calibration

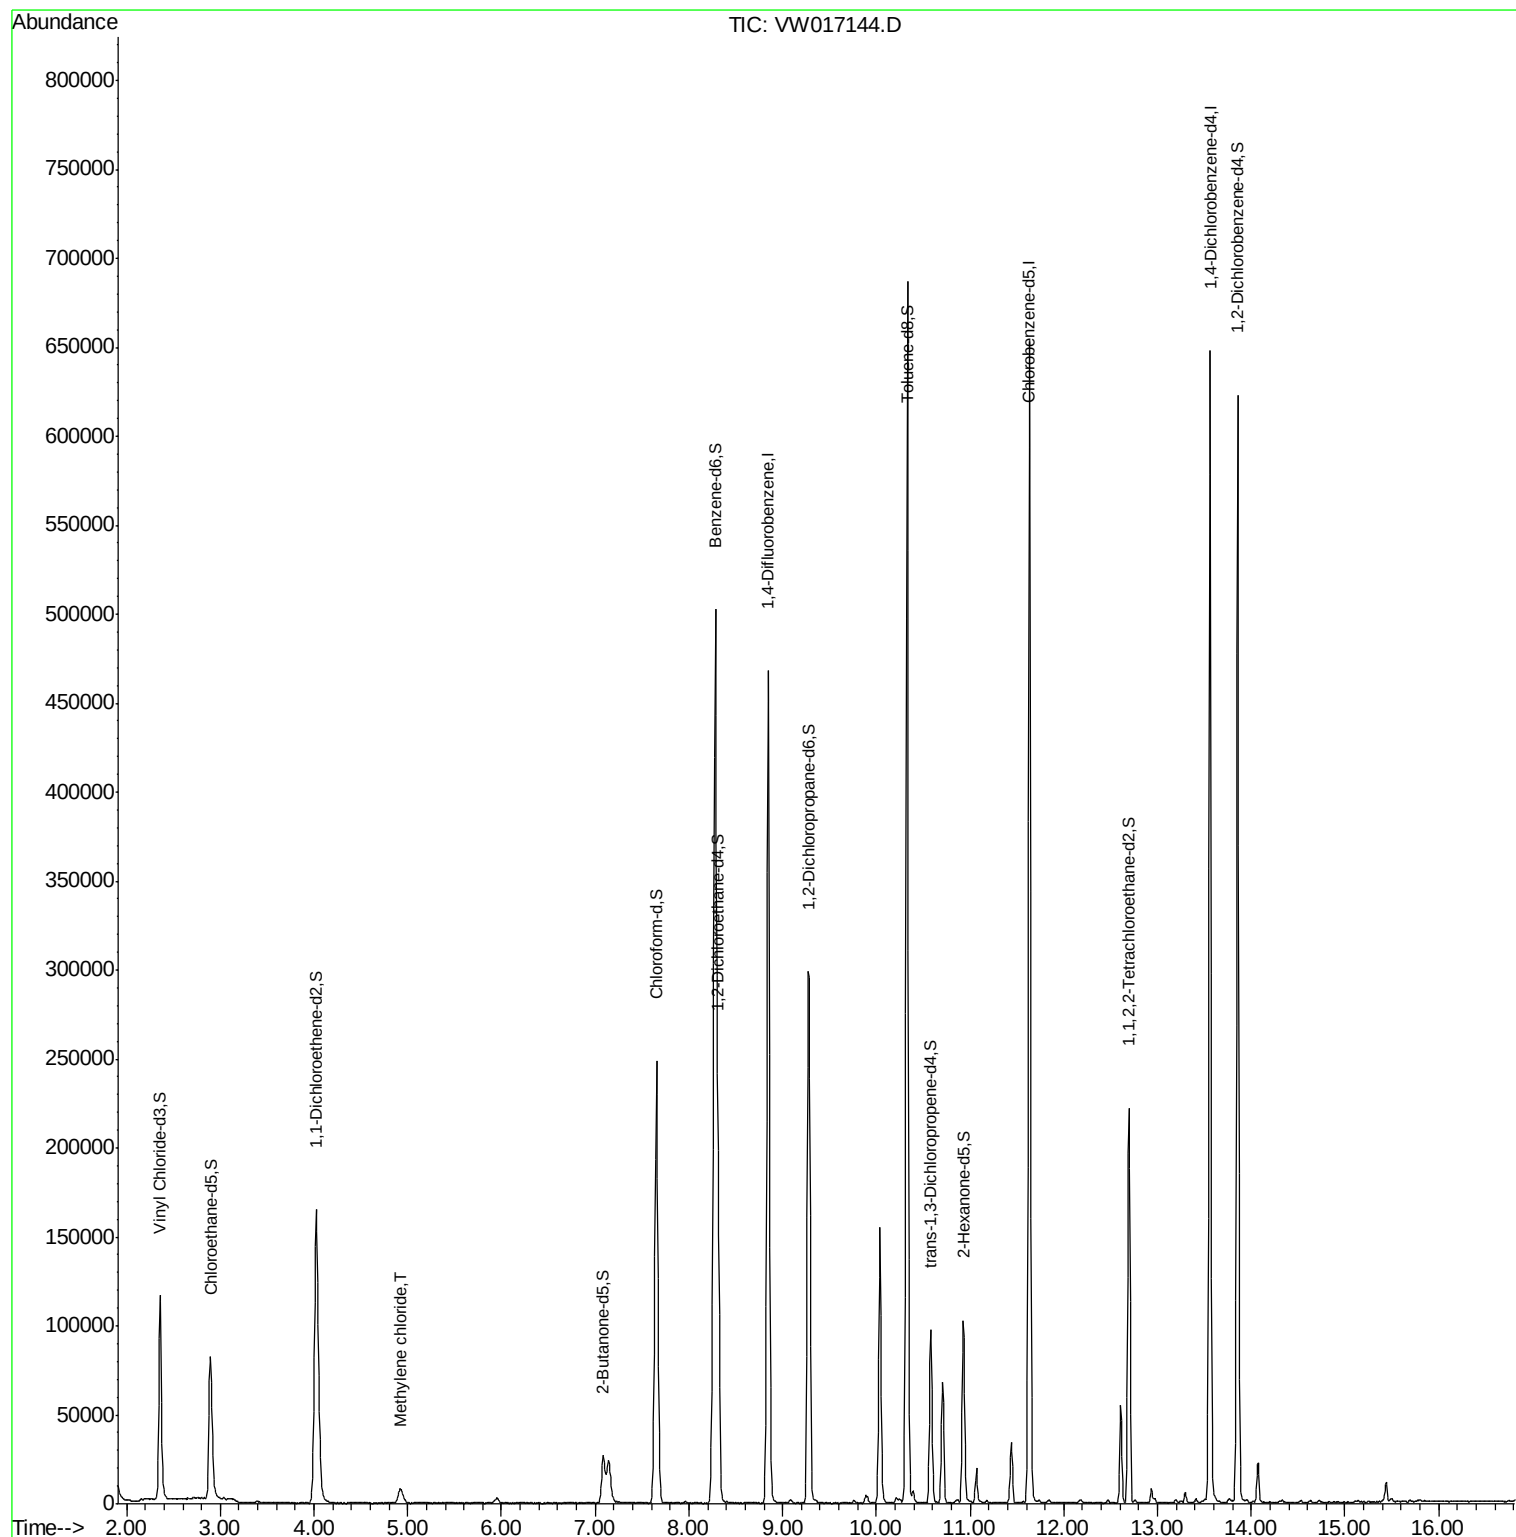

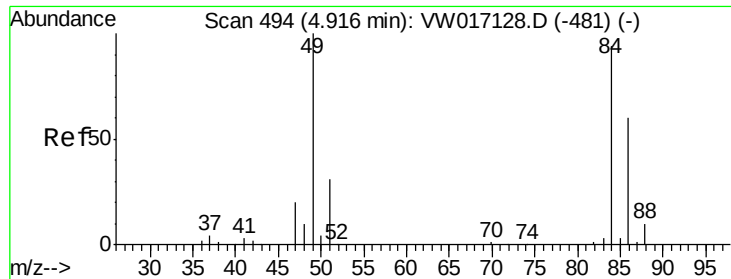

#16
 Methylene chloride
 Concen: 1.330 ug/L
 RT: 4.92 min Scan# 494
 Delta R.T. 0.00 min
 Lab File: VW017144.D
 Acq: 10 Nov 2020 16:47

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK19

Tot Ion:	84	Resp:	7554
Ion	Ratio	Lower	Upper
84	100		
49	89.6	72.3	134.3
86	66.5	45.1	83.7

