

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
 Data File : VW017166.D
 Acq On : 11 Nov 2020 16:11
 Operator : SY/VA
 Sample : VIBLK25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK25

Manual Integrations
APPROVED

MMDadoda
 11/13/2020 11:41:09 AM

Quant Time: Nov 12 03:16:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 03:07:51 2020
 Response via : Initial Calibration

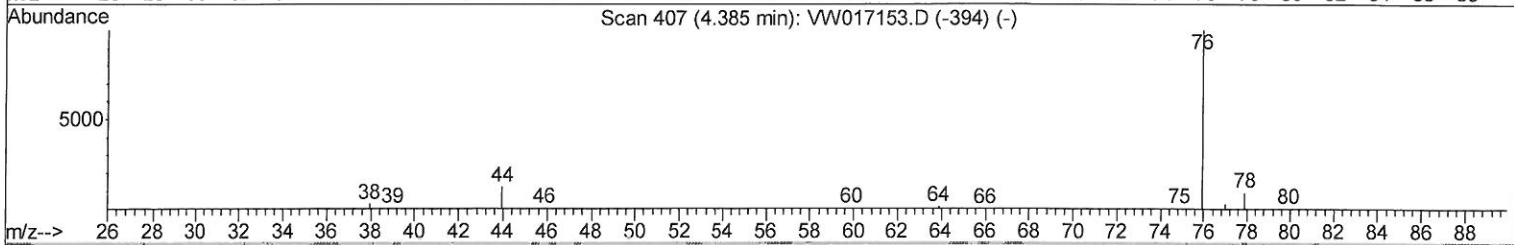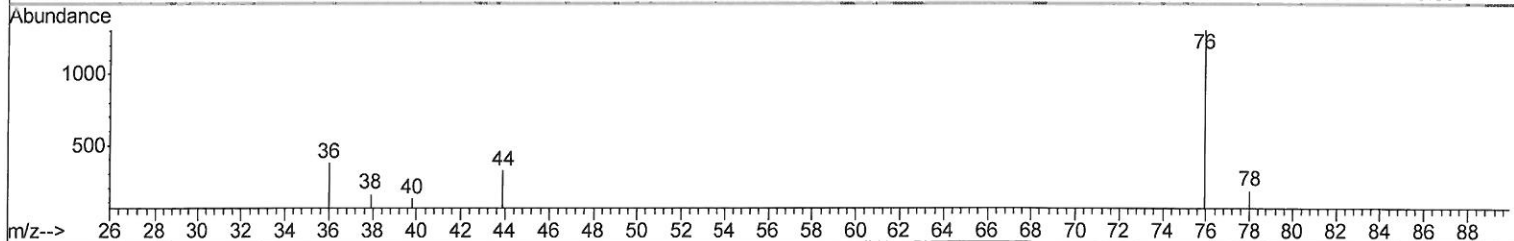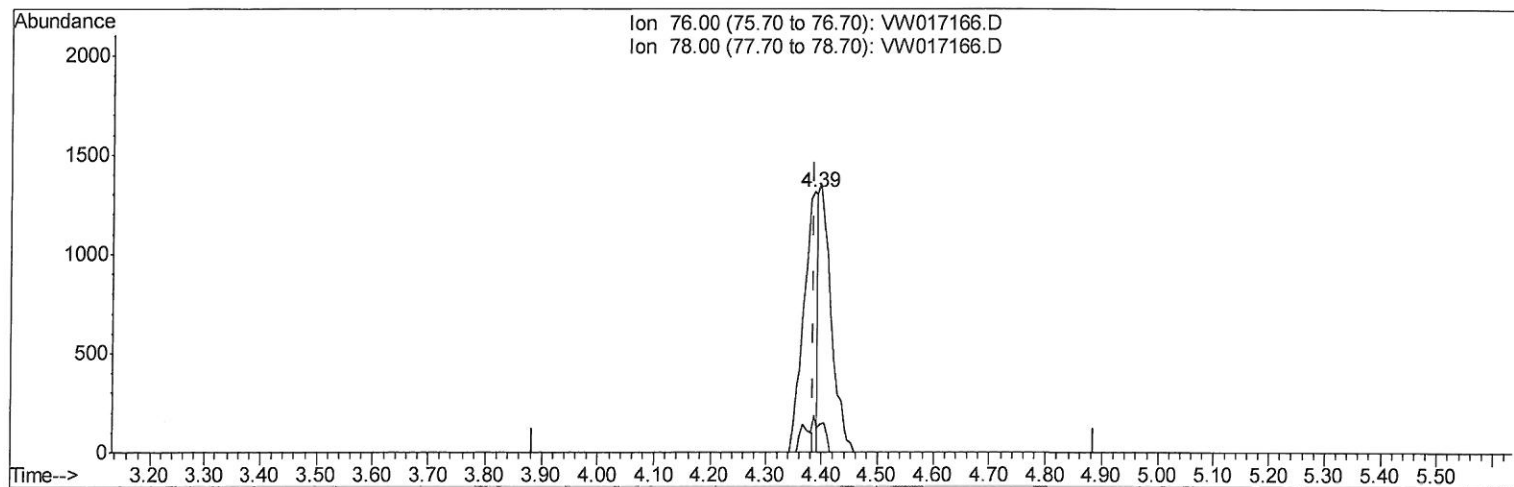

TIC: VW017166.D

(14) Carbon disulfide (T)
 4.385min (+0.000) 0.18ug/L
 response 2356

Ion	Exp%	Act%
76.00	100	100
78.00	9.50	14.11#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
Data File : VW017166.D
Acq On : 11 Nov 2020 16:11
Operator : SY/VA
Sample : VIBLK25
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK25

Manual Integrations
APPROVED

MMDadoda
11/13/2020 11:41:09 AM

Quant Time: Nov 12 03:16:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 12 03:07:51 2020
Response via : Initial Calibration

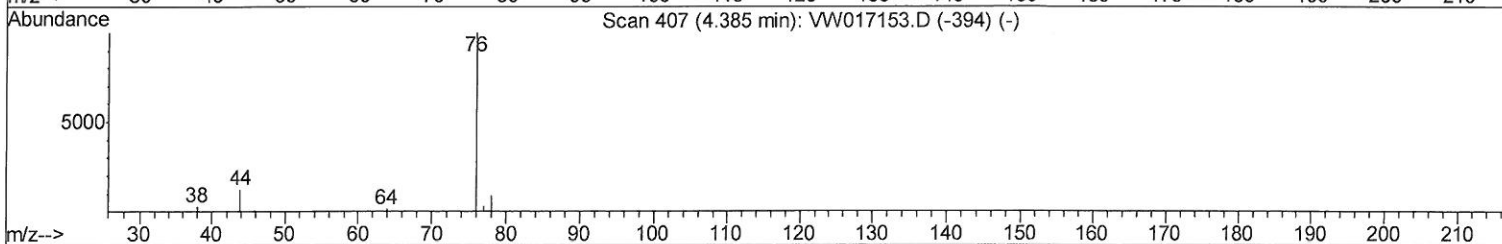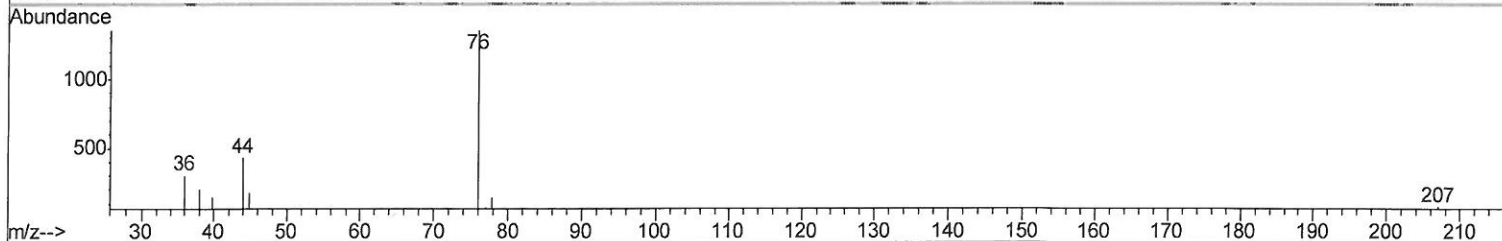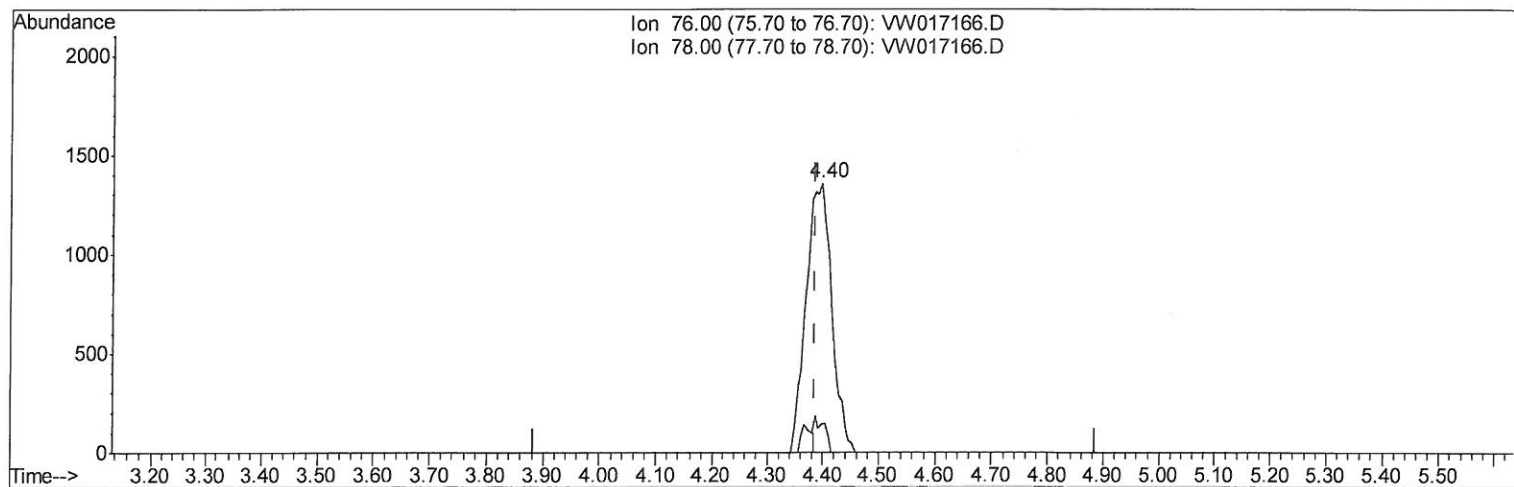

TIC: VW017166.D

(14) Carbon disulfide (T)

4.397min (+0.012) 0.33ug/L m

5/11/18/2020

response 4349

Ion	Exp%	Act%
76.00	100	100
78.00	9.50	10.46
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
Data File : VW017166.D
Acq On : 11 Nov 2020 16:11
Operator : SY/VA
Sample : VIBLK25
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK25

Manual Integrations
APPROVED

MMDadoda
11/13/2020 11:41:09 AM

Quant Time: Nov 12 03:16:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 12 03:07:51 2020
Response via : Initial Calibration

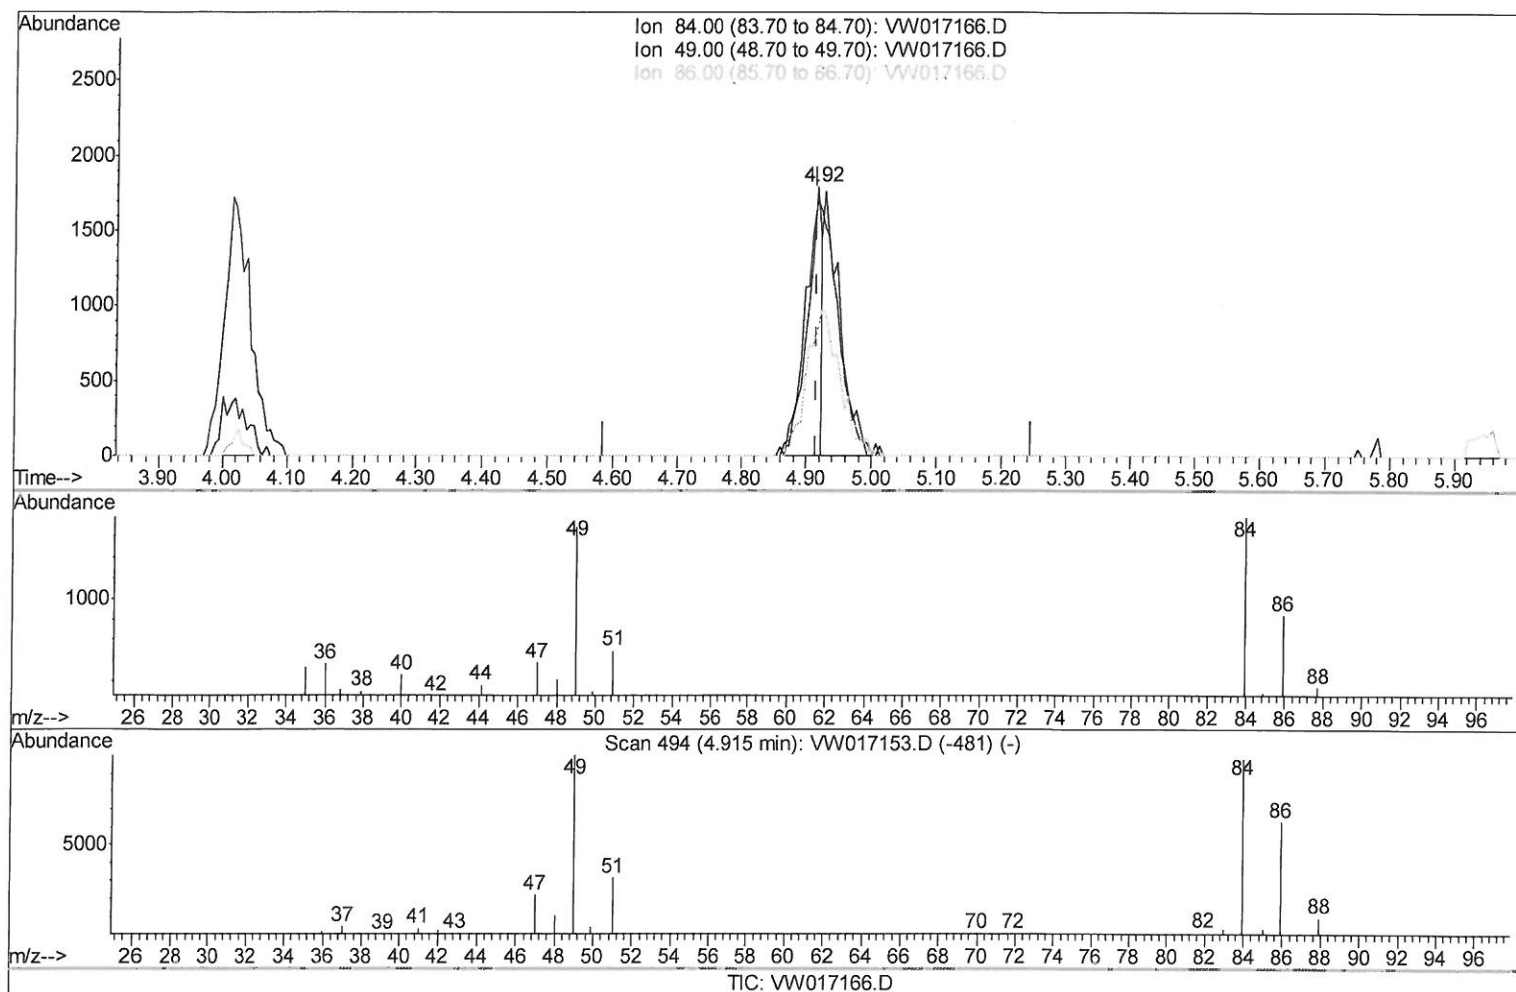

(16) Methylene chloride (T)

4.916min (+0.000) 0.52ug/L

response 2748

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	94.98
86.00	64.40	46.71
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
 Data File : VW017166.D
 Acq On : 11 Nov 2020 16:11
 Operator : SY/VA
 Sample : VIBLK25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK25

Manual Integrations
 APPROVED

MMDadoda
 11/13/2020 11:41:09 AM

Quant Time: Nov 12 03:16:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 03:07:51 2020
 Response via : Initial Calibration

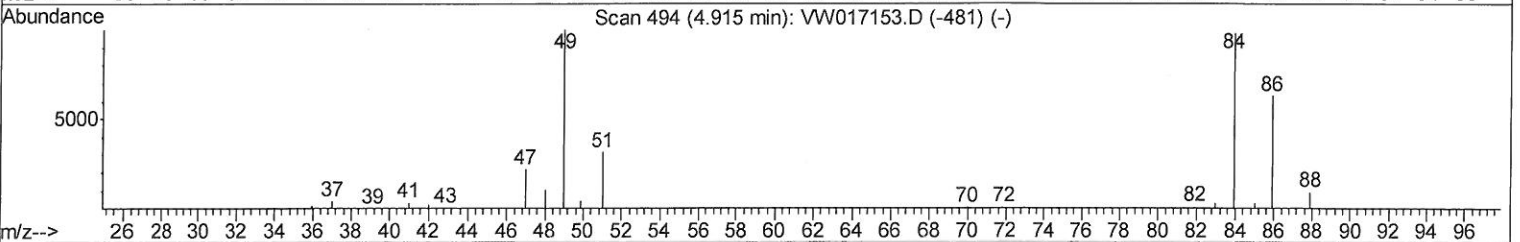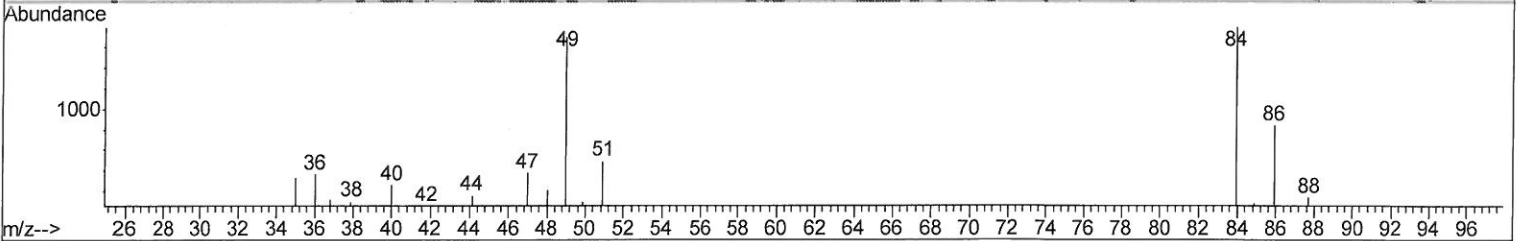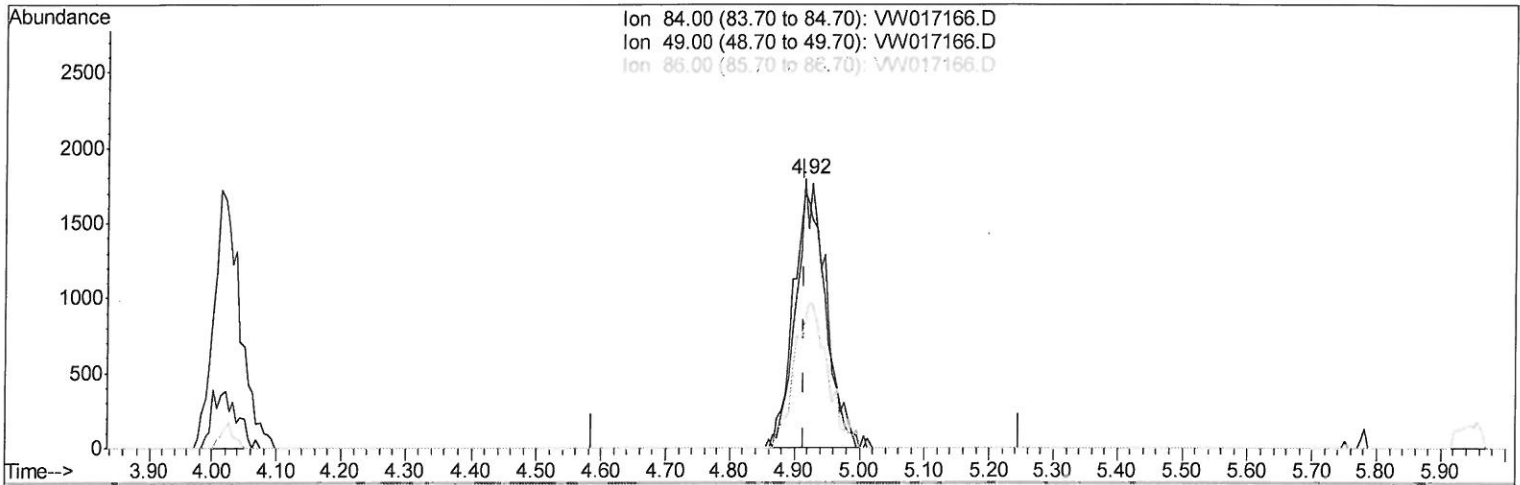

TIC: VW017166.D

(16) Methylene chloride (T)

4.916min (+0.000) 1.07ug/L m

response 5645

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	94.98
86.00	64.40	46.71
0.00	0.00	0.00

11/18/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
 Data File : VW017166.D
 Acq On : 11 Nov 2020 16:11
 Operator : SY/VA
 Sample : VIBLK25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK25

Manual Integrations
 APPROVED

MMDadoda
 11/13/2020 11:41:09 AM

Quant Time: Nov 12 05:50:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 12 03:07:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	392220	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	366459	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	173598	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	132458	26.81	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	107.24%		
7) Chloroethane-d5	2.89	69	109910	28.87	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	115.48%		
10) 1,1-Dichloroethene-d2	4.03	63	170163	19.26	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.04%		
20) 2-Butanone-d5	7.09	46	56466	51.11	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.22%		
24) Chloroform-d	7.65	84	259752	28.37	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	113.48%		
26) 1,2-Dichloroethane-d4	8.31	65	131490	28.89	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	115.56%		
29) Benzene-d6	8.27	84	492434	26.39	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.56%		
33) 1,2-Dichloropropane-d6	9.28	67	140592	27.24	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.96%		
37) Toluene-d8	10.32	98	461805	26.24	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	104.96%		
38) trans-1,3-Dichloropropene-	10.58	79	57011	24.50	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	98.00%		
39) 2-Hexanone-d5	10.93	63	46434	51.55	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.10%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	122367	27.21	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	108.84%		
61) 1,2-Dichlorobenzene-d4	13.85	152	175075	28.63	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	114.52%		

Target Compounds

					Ovalue
14) Carbon disulfide	4.40	76	4349m	0.328	ug/L
16) Methylene chloride	4.92	84	5645m	1.068	ug/L
43) 4-Methyl-2-pentanone	10.21	43	3155	1.137	ug/L
47) Tetrachloroethene	10.87	164	143084	29.421	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111120\
Data File : VW017166.D
Acq On : 11 Nov 2020 16:11
Operator : SY/VA
Sample : VIBLK25
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK25

Manual Integrations
APPROVED

MMDadoda
11/13/2020 11:41:09 AM

Quant Time: Nov 12 05:50:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 12 03:07:51 2020
Response via : Initial Calibration

