


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111120\
 Data File : VW017152.D
 Acq On : 11 Nov 2020 08:35
 Operator : SY/VA
 Sample : BFB03
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB03

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Title : VOC Analysis
 Last Update : Thu Nov 12 03:07:51 2020

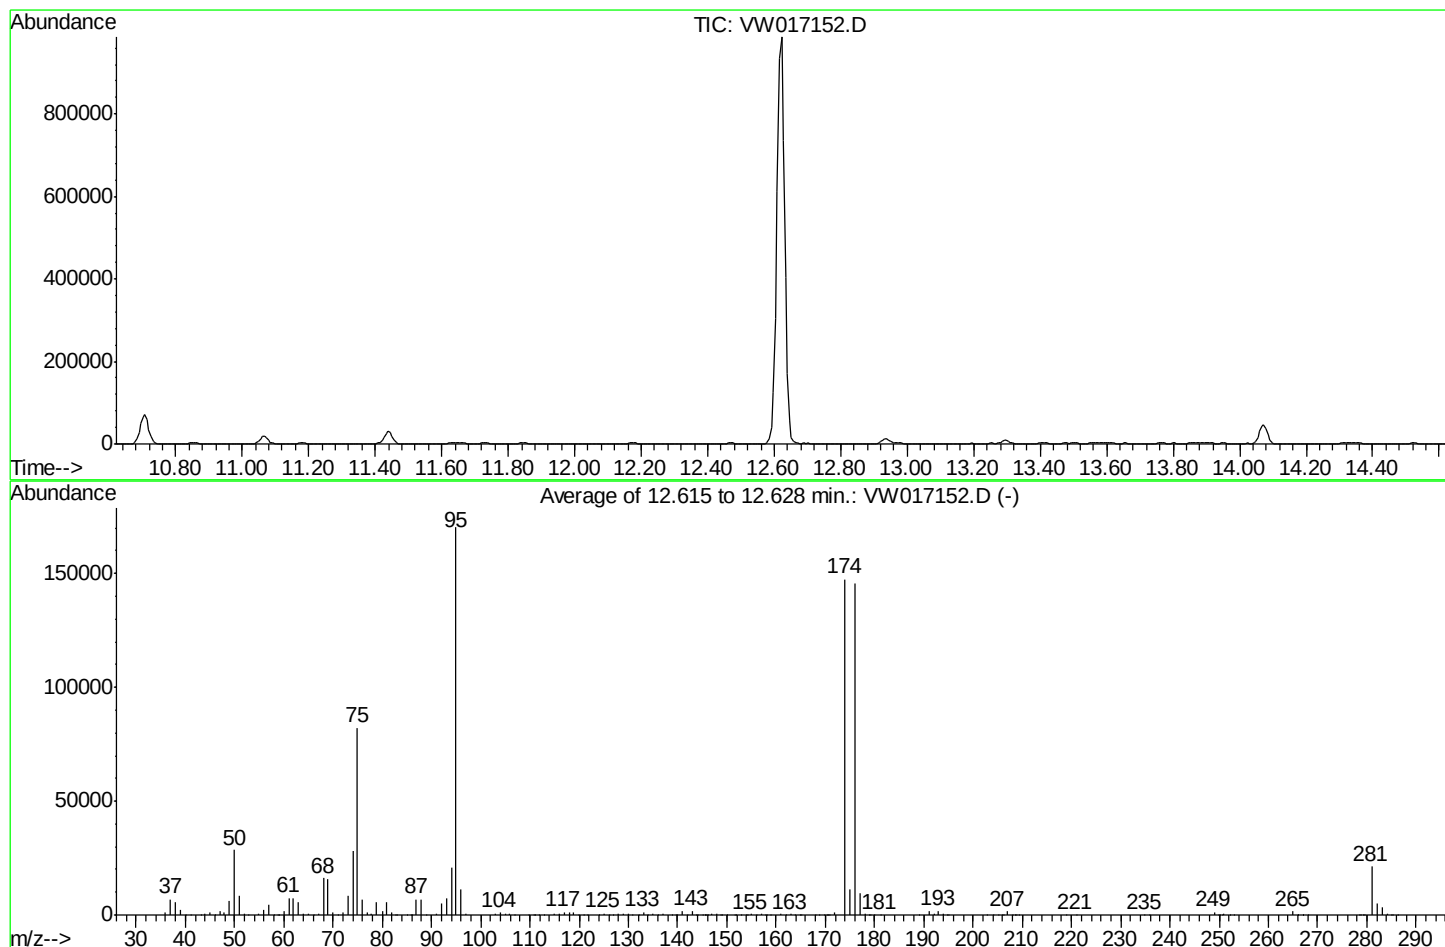

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	28666	PASS
75	95	30	80	48.2	82125	PASS
95	95	100	100	100.0	170261	PASS
96	95	5	9	6.7	11365	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.6	147477	PASS
175	174	5	9	7.7	11387	PASS
176	174	95	101	98.7	145520	PASS
177	176	5	9	6.6	9540	PASS

m/z	Abundance
36.00	1534.0
37.00	7723.0
38.00	7225.0
39.00	2674.0
40.10	217.0
41.00	59.0
43.00	155.0
44.10	1132.0
45.00	1519.0
45.90	177.0
47.00	1786.0
48.00	1026.0
49.00	7108.0
50.00	31496.0
51.00	9594.0
52.10	444.0
52.80	126.0
55.00	491.0
56.00	2621.0
57.00	4732.0
58.10	261.0
59.10	270.0
60.00	1696.0
61.00	8057.0
62.00	7842.0
63.00	5986.0
64.10	782.0
65.00	592.0
66.00	154.0
67.00	471.0
68.00	17392.0
69.00	17024.0
70.00	1436.0
72.00	982.0
73.00	10462.0
74.00	30344.0
75.00	87272.0
76.00	7376.0
77.00	1306.0
78.00	769.0
78.90	6139.0
79.90	1520.0
80.90	6435.0
81.90	1331.0
82.70	87.0
83.20	75.0
85.00	56.0
85.80	280.0
86.90	7426.0
88.00	7069.0
90.90	871.0
92.00	5192.0
93.00	7563.0
94.00	21200.0
95.00	176704.0
96.10	11785.0
97.00	454.0
102.90	481.0
104.00	1000.0
105.00	447.0
105.90	870.0
106.90	165.0
109.80	314.0
110.90	371.0
111.90	325.0
112.80	198.0
114.90	367.0
115.90	734.0
116.90	1334.0
117.90	1176.0
118.80	1341.0
119.90	122.0
121.00	106.0
124.00	197.0
125.00	941.0
126.00	148.0
126.80	87.0
127.90	580.0
128.90	317.0
130.00	508.0
130.90	253.0
133.10	2479.0
134.90	567.0
136.00	95.0
136.90	352.0
138.90	65.0
139.70	58.0
140.90	1893.0
141.90	272.0
143.00	1975.0
143.90	135.0
144.90	397.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

145.60	178.0
146.00	212.0
147.00	451.0
147.90	493.0
148.90	272.0
149.90	259.0
151.70	70.0
153.00	100.0
153.90	98.0
154.80	537.0
156.00	110.0
157.00	349.0
158.10	128.0
158.90	311.0
160.90	494.0
161.90	91.0
162.90	519.0
164.00	110.0
165.10	366.0
168.80	60.0
169.70	71.0
170.20	60.0
170.90	130.0
171.90	1169.0
174.00	139776.0
175.00	11453.0
175.90	140608.0
176.90	9023.0
178.00	332.0
178.90	712.0
180.00	217.0
181.10	86.0
189.10	271.0
191.00	2440.0
192.10	597.0
193.00	3057.0
194.00	649.0
195.00	355.0
202.90	334.0
204.00	51.0
205.00	486.0
205.90	146.0
207.00	2413.0
208.00	393.0
208.60	149.0
209.20	259.0
218.90	67.0
220.90	85.0
234.80	216.0
235.90	58.0
249.00	1837.0
250.00	476.0
251.00	801.0
252.20	163.0
252.90	61.0
265.10	2503.0
265.90	420.0
266.90	639.0
267.90	116.0
278.40	74.0
279.20	217.0
281.00	32224.0
282.10	8226.0
283.10	5416.0
284.10	975.0
284.90	365.0
286.20	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

m/z	Abundance
36.00	1475.0
37.00	7684.0
38.00	6067.0
39.00	2610.0
39.90	180.0
43.10	158.0
44.00	1040.0
45.00	1629.0
46.00	135.0
47.00	1804.0
48.00	916.0
49.00	7192.0
50.00	31720.0
51.00	9641.0
52.10	342.0
52.90	55.0
55.00	446.0
56.00	2837.0
57.00	4697.0
58.10	158.0
58.90	160.0
60.00	1691.0
61.00	8248.0
62.00	8185.0
63.00	6648.0
64.00	813.0
65.10	501.0
65.90	98.0
66.90	583.0
68.00	17944.0
69.00	17568.0
70.00	1596.0
70.90	73.0
72.10	956.0
73.00	9278.0
74.00	31328.0
75.00	92856.0
76.00	7816.0
76.90	1044.0
77.80	729.0
78.90	6284.0
80.00	1800.0
80.90	6317.0
81.90	1292.0
82.80	167.0
86.10	255.0
87.00	7787.0
87.90	7450.0
91.00	782.0
92.00	5485.0
93.00	8183.0
94.00	23776.0
95.00	191552.0
96.00	13217.0
97.00	258.0
102.90	299.0
104.00	1066.0
105.00	312.0
105.80	922.0
106.80	231.0
109.80	156.0
111.10	314.0
111.90	194.0
112.90	155.0
114.90	396.0
115.90	767.0
116.90	1311.0
118.00	865.0
118.80	1228.0
119.80	84.0
121.70	57.0
124.00	129.0
124.90	616.0
126.00	201.0
127.90	734.0
128.90	444.0
129.90	613.0
131.00	300.0
132.00	96.0
132.90	964.0
134.80	536.0
136.00	52.0
136.90	391.0
138.90	51.0
139.90	186.0
140.90	2078.0
141.80	260.0
142.90	2255.0
143.90	143.0
144.90	263.0
145.80	435.0
147.00	320.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

148.00	490.0
148.70	208.0
149.90	209.0
151.90	129.0
153.00	111.0
153.90	100.0
154.90	543.0
156.00	130.0
156.90	441.0
157.80	120.0
158.90	282.0
161.00	275.0
161.90	63.0
162.90	275.0
163.80	83.0
164.80	107.0
168.00	51.0
170.20	75.0
170.80	232.0
172.00	1167.0
173.90	164160.0
175.00	12924.0
176.00	167360.0
177.00	10894.0
178.00	539.0
179.10	456.0
179.90	87.0
188.90	152.0
191.00	1295.0
192.00	355.0
193.00	2064.0
194.00	424.0
194.70	217.0
202.90	289.0
205.10	244.0
206.10	77.0
207.10	1028.0
208.00	310.0
208.80	78.0
209.20	144.0
234.80	151.0
235.80	63.0
249.00	1376.0
250.10	316.0
250.90	633.0
252.20	85.0
265.00	1604.0
266.10	415.0
267.10	315.0
268.00	108.0
278.80	131.0
279.40	171.0
281.10	21864.0
282.00	4434.0
283.10	3071.0
284.10	563.0
285.20	160.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

m/z	Abundance
36.00	1089.0
37.00	5490.0
38.00	4478.0
39.00	2091.0
40.00	228.0
44.00	800.0
45.00	1037.0
46.10	119.0
46.90	1148.0
47.90	775.0
49.00	4894.0
50.00	22784.0
51.00	6812.0
52.00	376.0
53.00	91.0
54.90	391.0
56.00	2098.0
57.00	3490.0
57.90	107.0
58.80	145.0
60.00	1058.0
61.00	5700.0
62.00	5649.0
63.00	4390.0
64.00	446.0
65.20	309.0
65.90	70.0
67.00	366.0
68.00	13318.0
69.00	13218.0
70.10	955.0
72.00	796.0
73.00	6309.0
74.00	23144.0
75.00	66248.0
76.00	5449.0
77.00	891.0
77.80	687.0
78.90	4523.0
79.90	1408.0
80.90	4509.0
82.00	1119.0
83.00	188.0
85.80	176.0
87.00	5517.0
87.90	5975.0
88.80	163.0
91.00	576.0
92.00	4014.0
93.00	6275.0
94.00	16680.0
95.00	142528.0
96.00	9094.0
96.90	212.0
103.00	225.0
103.90	707.0
104.80	299.0
105.90	711.0
106.90	139.0
109.80	95.0
110.80	125.0
112.00	118.0
112.90	154.0
114.90	263.0
116.00	540.0
116.90	1155.0
117.90	726.0
118.90	826.0
119.80	94.0
124.00	119.0
125.10	335.0
126.10	59.0
127.90	599.0
128.90	295.0
129.80	471.0
130.80	269.0
133.10	628.0
133.90	151.0
134.90	272.0
137.00	385.0
138.90	52.0
139.90	144.0
140.80	1580.0
141.80	130.0
143.00	1679.0
144.10	88.0
145.00	236.0
145.70	193.0
146.10	230.0
146.80	154.0
147.80	325.0
149.00	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

150.00	186.0
151.70	92.0
153.00	62.0
154.10	82.0
154.90	316.0
156.00	104.0
156.90	344.0
157.80	113.0
158.10	138.0
158.90	237.0
161.00	185.0
162.90	155.0
163.70	53.0
165.00	87.0
170.60	118.0
172.00	984.0
173.90	138496.0
175.00	9786.0
176.00	128592.0
176.90	8705.0
178.10	221.0
179.00	274.0
189.00	102.0
191.10	620.0
192.00	118.0
193.00	630.0
194.00	208.0
194.90	194.0
202.90	88.0
205.20	153.0
207.00	834.0
208.00	179.0
208.90	77.0
234.90	83.0
248.90	505.0
249.80	149.0
250.60	148.0
251.10	167.0
265.00	562.0
266.00	164.0
266.80	193.0
268.10	64.0
281.10	9700.0
282.10	2590.0
283.10	1621.0
284.10	244.0
285.20	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

Scan 1749 (12.567 min): VW017152.D
BFB03

m/z	Abundance
39.90	180.0
44.00	239.0
133.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03