

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
 Data File : VW017183.D
 Acq On : 12 Nov 2020 14:34
 Operator : SY/VA
 Sample : VIBLK01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK01

Manual Integrations
 APPROVED

MMDadoda
 11/18/2020 10:51:12 AM

Quant Time: Nov 13 04:19:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 13 04:11:30 2020
 Response via : Initial Calibration

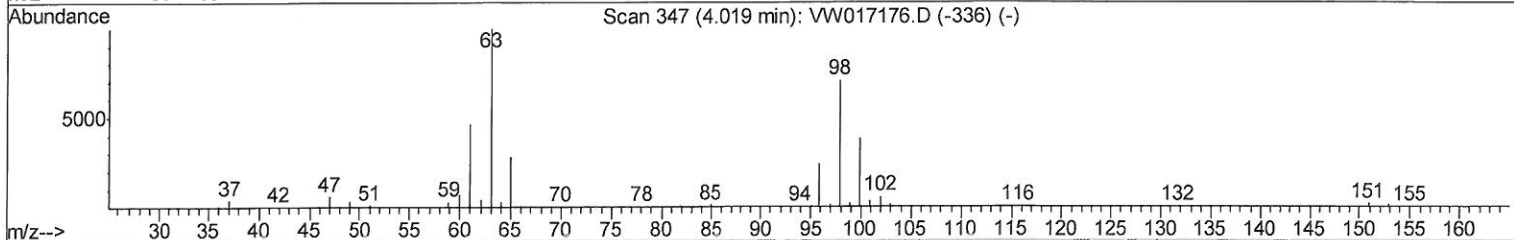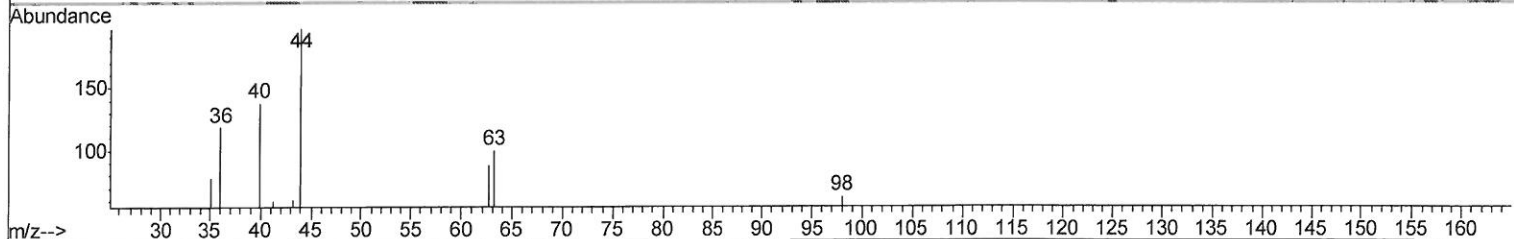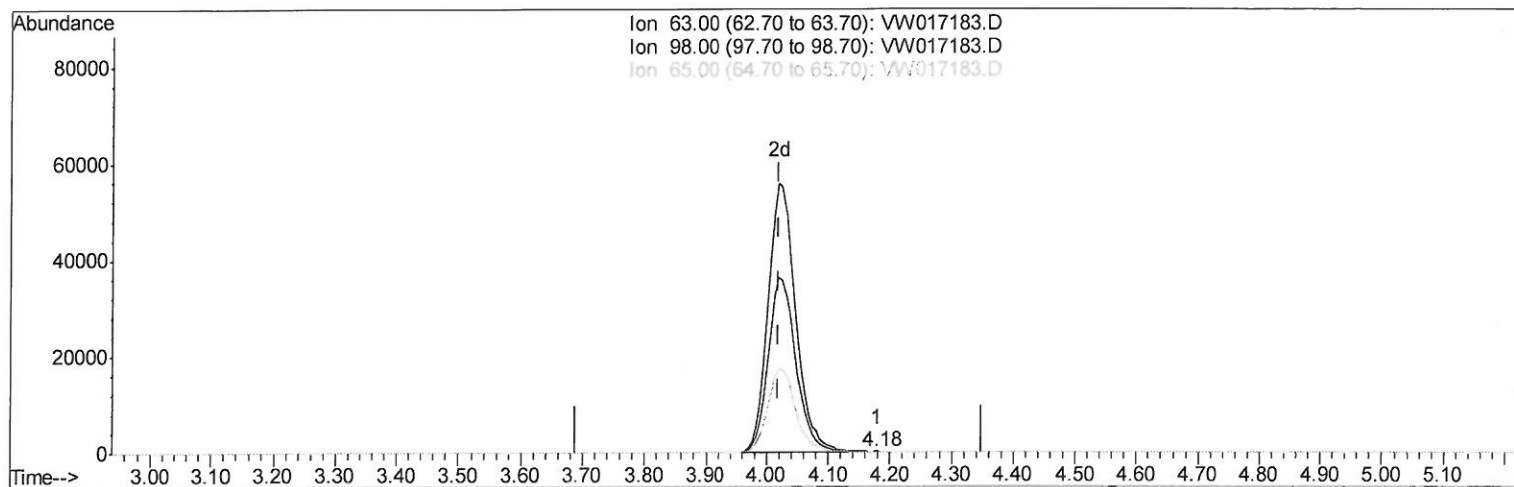

TIC: VW017183.D

(10) 1,1-Dichloroethene-d2 (S)

4.178min (+0.158) 0.02ug/L

response 182

Ion	Exp%	Act%
63.00	100	100
98.00	83.10	59.34
65.00	24.20	23.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
Data File : VW017183.D
Acq On : 12 Nov 2020 14:34
Operator : SY/VA
Sample : VIBLK01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK01

Manual Integrations
APPROVED

MMDadoda
11/18/2020 10:51:12 AM

Quant Time: Nov 13 04:19:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 13 04:11:30 2020
Response via : Initial Calibration

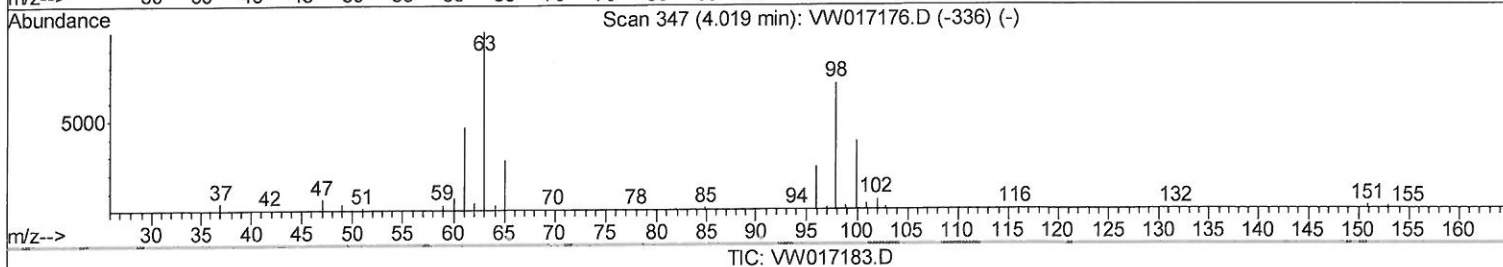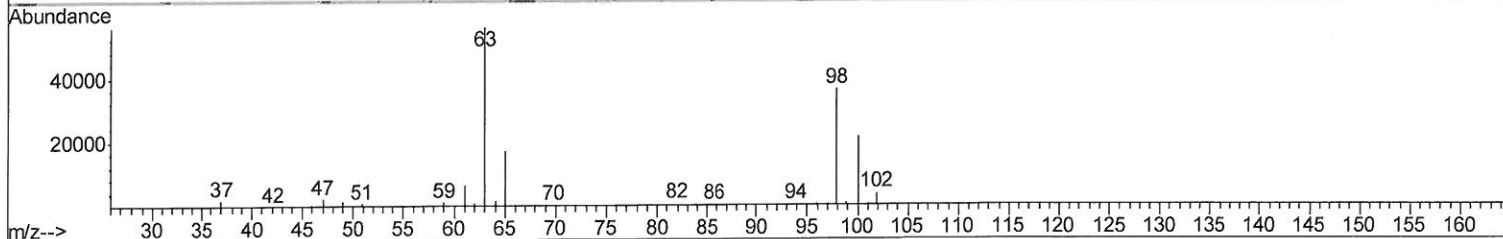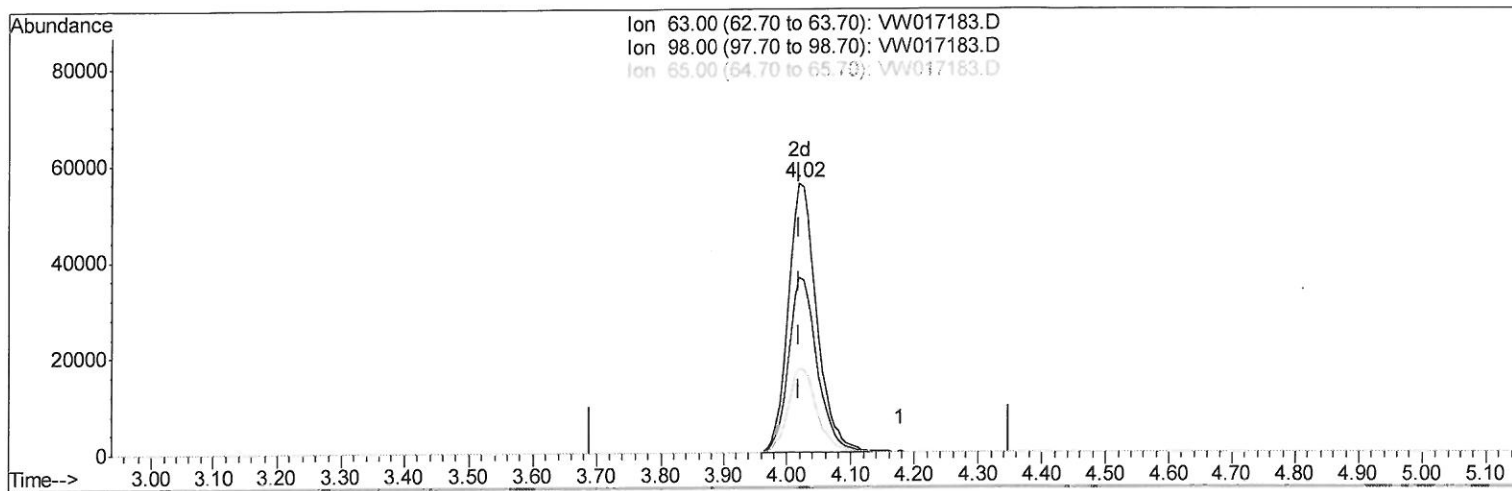

(10) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 18.13ug/L m

response 171545

Ion	Exp%	Act%
63.00	100	100
98.00	83.10	0.06#
65.00	24.20	0.03#
0.00	0.00	0.00

11/18/2020 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\WV111220\
 Data File : VW017183.D
 Acq On : 12 Nov 2020 14:34
 Operator : SY/VA
 Sample : VIBLK01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK01

Manual Integrations
 APPROVED

MMDadoda
 11/18/2020 10:51:12 AM

Quant Time: Nov 13 04:54:32 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M

Quant Title : VOC Analysis

QLast Update : Fri Nov 13 04:11:30 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	419915	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	393844	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	185698	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	131676	24.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 99.60%	
7) Chloroethane-d5	2.89	69	110321	27.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 108.28%	
10) 1,1-Dichloroethene-d2	4.02	63	171545m	18.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 72.52%	
20) 2-Butanone-d5	7.08	46	66247	56.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 112.02%	
24) Chloroform-d	7.65	84	265603	27.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 108.36%	
26) 1,2-Dichloroethane-d4	8.31	65	138103	28.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 113.36%	
29) Benzene-d6	8.28	84	510727	25.46	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 101.84%	
33) 1,2-Dichloropropane-d6	9.28	67	146719	26.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 105.80%	
37) Toluene-d8	10.33	98	478227	25.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 101.16%	
38) trans-1,3-Dichloropropene-	10.58	79	61152	24.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 97.80%	
39) 2-Hexanone-d5	10.93	63	51685	53.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 106.78%	
48) 1,1,2,2-Tetrachloroethane-	12.69	84	134287	27.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 111.16%	
61) 1,2-Dichlorobenzene-d4	13.85	152	185660	28.38	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 113.52%	

11/18/2020

Target Compounds					Ovalue
16) Methylene chloride	4.92	84	13361	2.360 ug/L	96
43) 4-Methyl-2-pentanone	10.21	43	3118	1.045 ug/L	98
47) Tetrachloroethene	10.87	164	2598	0.497 ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
Data File : VW017183.D
Acq On : 12 Nov 2020 14:34
Operator : SY/VA
Sample : VIBLK01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK01

Manual Integrations
APPROVED

MMDadoda
11/18/2020 10:51:12 AM

Quant Time: Nov 13 04:54:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 13 04:11:30 2020
Response via : Initial Calibration

