

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
Data File : VW017197.D
Acq On : 12 Nov 2020 20:03
Operator : SY/VA
Sample : VIBLK08
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VIBLK08

Manual Integrations
APPROVED

MMDadoda
11/18/2020 10:51:21 AM

Quant Time: Nov 13 04:22:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 13 04:11:30 2020
Response via : Initial Calibration

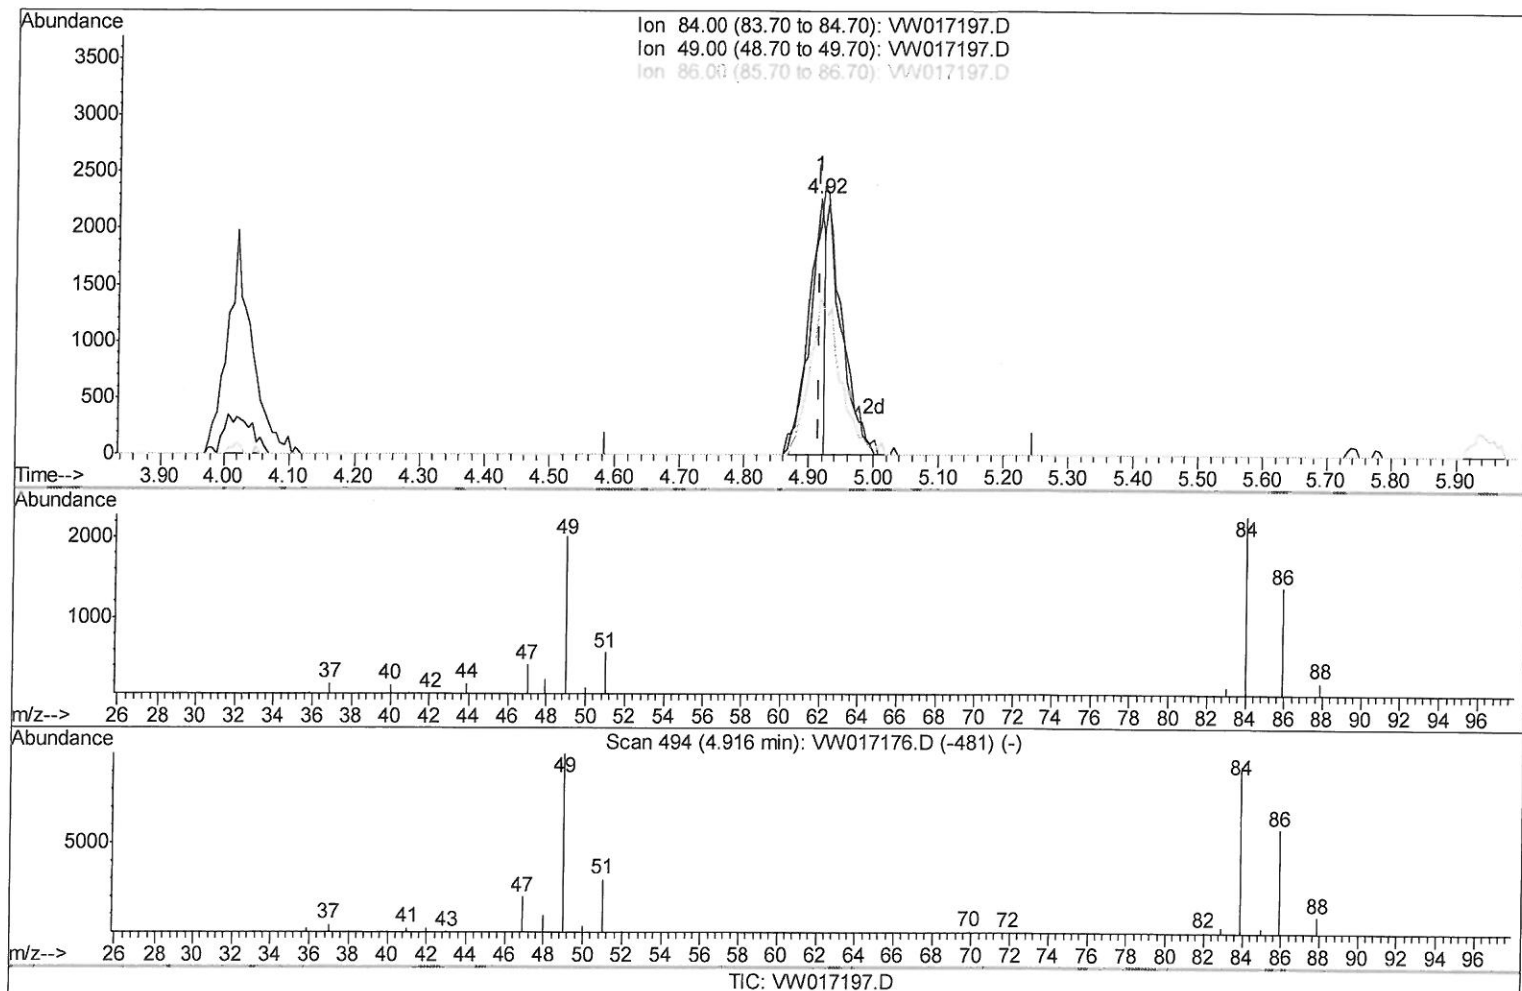

(16) Methylene chloride (T)

4.915min (-0.000) 0.67ug/L

response 3692

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	88.67
86.00	64.40	61.04
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
 Data File : VW017197.D
 Acq On : 12 Nov 2020 20:03
 Operator : SY/VA
 Sample : VIBLK08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK08

Manual Integrations
 APPROVED

MMDadoda
 11/18/2020 10:51:21 AM

Quant Time: Nov 13 04:22:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 13 04:11:30 2020
 Response via : Initial Calibration

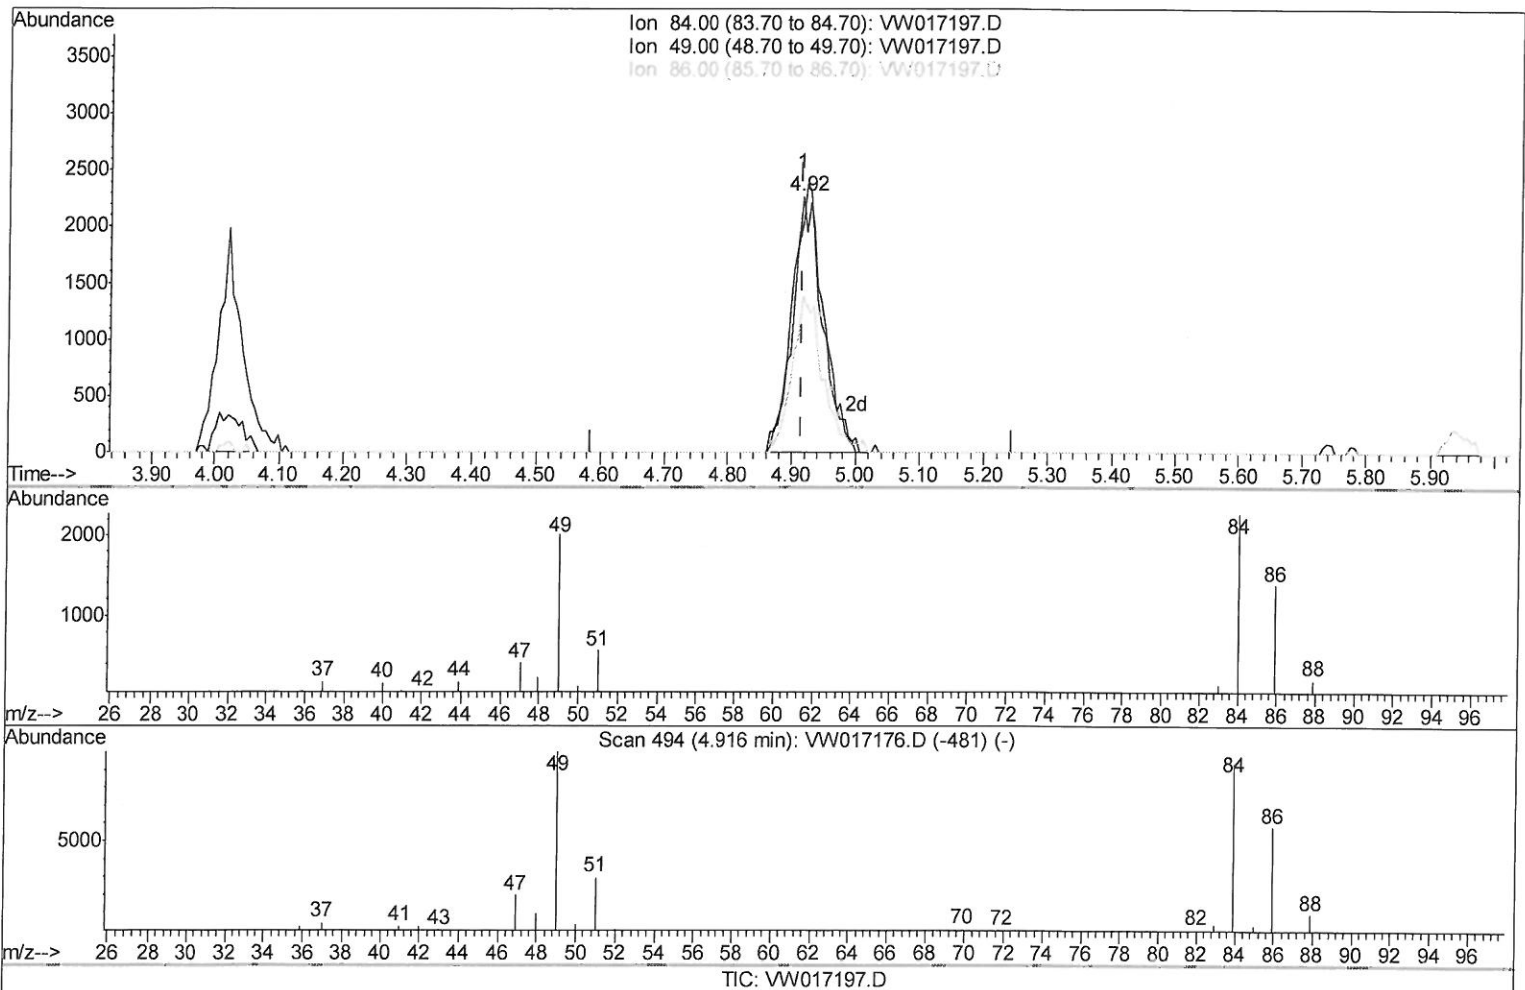

(16) Methylene chloride (T)

4.915min (-0.000) 1.36ug/L m

response 7563

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	88.67
86.00	64.40	61.04
0.00	0.00	0.00

11/18/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
 Data File : VW017197.D
 Acq On : 12 Nov 2020 20:03
 Operator : SY/VA
 Sample : VIBLK08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK08

Manual Integrations
 APPROVED

MMDadoda
 11/18/2020 10:51:21 AM

Quant Time: Nov 13 06:33:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 13 04:11:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	411430	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	371216	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	182146	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	107800	20.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.20%
7) Chloroethane-d5	2.89	69	93191	23.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.36%
10) 1,1-Dichloroethene-d2	4.02	63	156118	16.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.36%
20) 2-Butanone-d5	7.08	46	53709	46.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.70%
24) Chloroform-d	7.65	84	243631	25.37	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.48%
26) 1,2-Dichloroethane-d4	8.31	65	127801	26.76	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.04%
29) Benzene-d6	8.27	84	465640	24.63	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.52%
33) 1,2-Dichloropropane-d6	9.27	67	130562	24.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.88%
37) Toluene-d8	10.32	98	454152	25.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.92%
38) trans-1,3-Dichloropropene-	10.58	79	55875	23.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.80%
39) 2-Hexanone-d5	10.93	63	45624	50.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.00%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	114270	25.09	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	179738	28.01	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.04%

Target Compounds

16) Methylene chloride	4.92	84	7563m	Ovalue	1.363 ug/L
------------------------	------	----	-------	--------	------------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111220\
Data File : VW017197.D
Acq On : 12 Nov 2020 20:03
Operator : SY/VA
Sample : VIBLK08
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK08

Manual Integrations
APPROVED

MMDadoda
11/18/2020 10:51:21 AM

Quant Time: Nov 13 06:33:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 13 04:11:30 2020
Response via : Initial Calibration

