

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111221\
 Data File : VW020876.D
 Acq On : 13 Nov 2021 00:25
 Operator : SY/VA
 Sample : M4654-03
 Misc : 6.55g/5mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 15 00:14:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111021S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 13 07:30:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.945	168	76097	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.842	114	118593	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.628	117	102804	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.554	152	54118	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.305	65	36603	58.166	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 116.340%			
35) Dibromofluoromethane	7.884	113	34989	52.774	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 105.540%			
50) Toluene-d8	10.323	98	124280	47.911	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 95.820%			
62) 4-Bromofluorobenzene	12.615	95	49407	52.793	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 105.580%			
Target Compounds						
5) Bromomethane	2.776	94	39	Below Cal	#	2
16) Acetone	4.123	43	2070	16.901	ug/l	97
20) Methylene Chloride	4.915	84	902	Below Cal		97
31) Cyclohexane	7.945	56	3081	2.730	ug/l	# 62
36) 1,1-Dichloropropene	7.945	75	5177	5.281	ug/l	# 50
38) Carbon Tetrachloride	7.945	117	7120	6.934	ug/l	# 18
39) Methylcyclohexane	9.335	83	16354	12.719	ug/l	96
48) Methyl methacrylate	9.518	41	1941	4.519	ug/l	# 63
51) 4-Methyl-2-Pentanone	10.323	43	2921	6.113	ug/l	96
55) 1,1,2-Trichloroethane	10.762	97	17799	36.374	ug/l	# 20
56) Ethyl methacrylate	10.664	69	3085	4.569	ug/l	# 1
59) 2-Hexanone	10.933	43	21849	62.297	ug/l	# 30
67) Ethyl Benzene	11.725	91	14351	4.343	ug/l	97
68) m/p-Xylenes	11.841	106	8141	6.230	ug/l	96
69) o-Xylene	12.164	106	11591	9.558	ug/l	99
73) Isopropylbenzene	12.463	105	17396	5.153	ug/l	100
74) N-amyl acetate	12.249	43	63551	78.835	ug/l	# 67
75) 1,1,2,2-Tetrachloroethane	12.780	83	12644	20.981	ug/l	# 26
76) 1,2,3-Trichloropropane	12.859	75	919	2.209	ug/l	# 100
78) n-propylbenzene	12.804	91	64702	15.776	ug/l	99
79) 2-Chlorotoluene	12.896	91	7883	3.504	ug/l	# 41
80) 1,3,5-Trimethylbenzene	12.938	105	88451	31.448	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.615	75	24540	116.089	ug/l	# 8
82) 4-Chlorotoluene	13.097	91	11737	5.042	ug/l	75
83) tert-Butylbenzene	13.249	119	6897	2.612	ug/l	# 70
84) 1,2,4-Trimethylbenzene	13.249	105	57107	20.659	ug/l	99
85) sec-Butylbenzene	13.383	105	54689	14.488	ug/l	82
86) p-Isopropyltoluene	13.493	119	34126	10.549	ug/l	97
89) n-Butylbenzene	13.822	91	99892	33.168	ug/l	# 69
90) Hexachloroethane	14.097	117	14531	23.361	ug/l	# 7
92) 1,2-Dibromo-3-Chloropr...	14.493	75	678	5.607	ug/l	# 24
95) Naphthalene	15.359	128	8413	4.220	ug/l	# 68
96) 1,2,3-Trichlorobenzene	15.517	180	4912	5.580	ug/l	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_W
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111221\
Data File : VW020876.D
Acq On : 13 Nov 2021 00:25
Operator : SY/VA
Sample : M4654-03
Misc : 6.55g/5mL/MSVOA_W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 15 00:14:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111021S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 13 07:30:48 2021
Response via : Initial Calibration

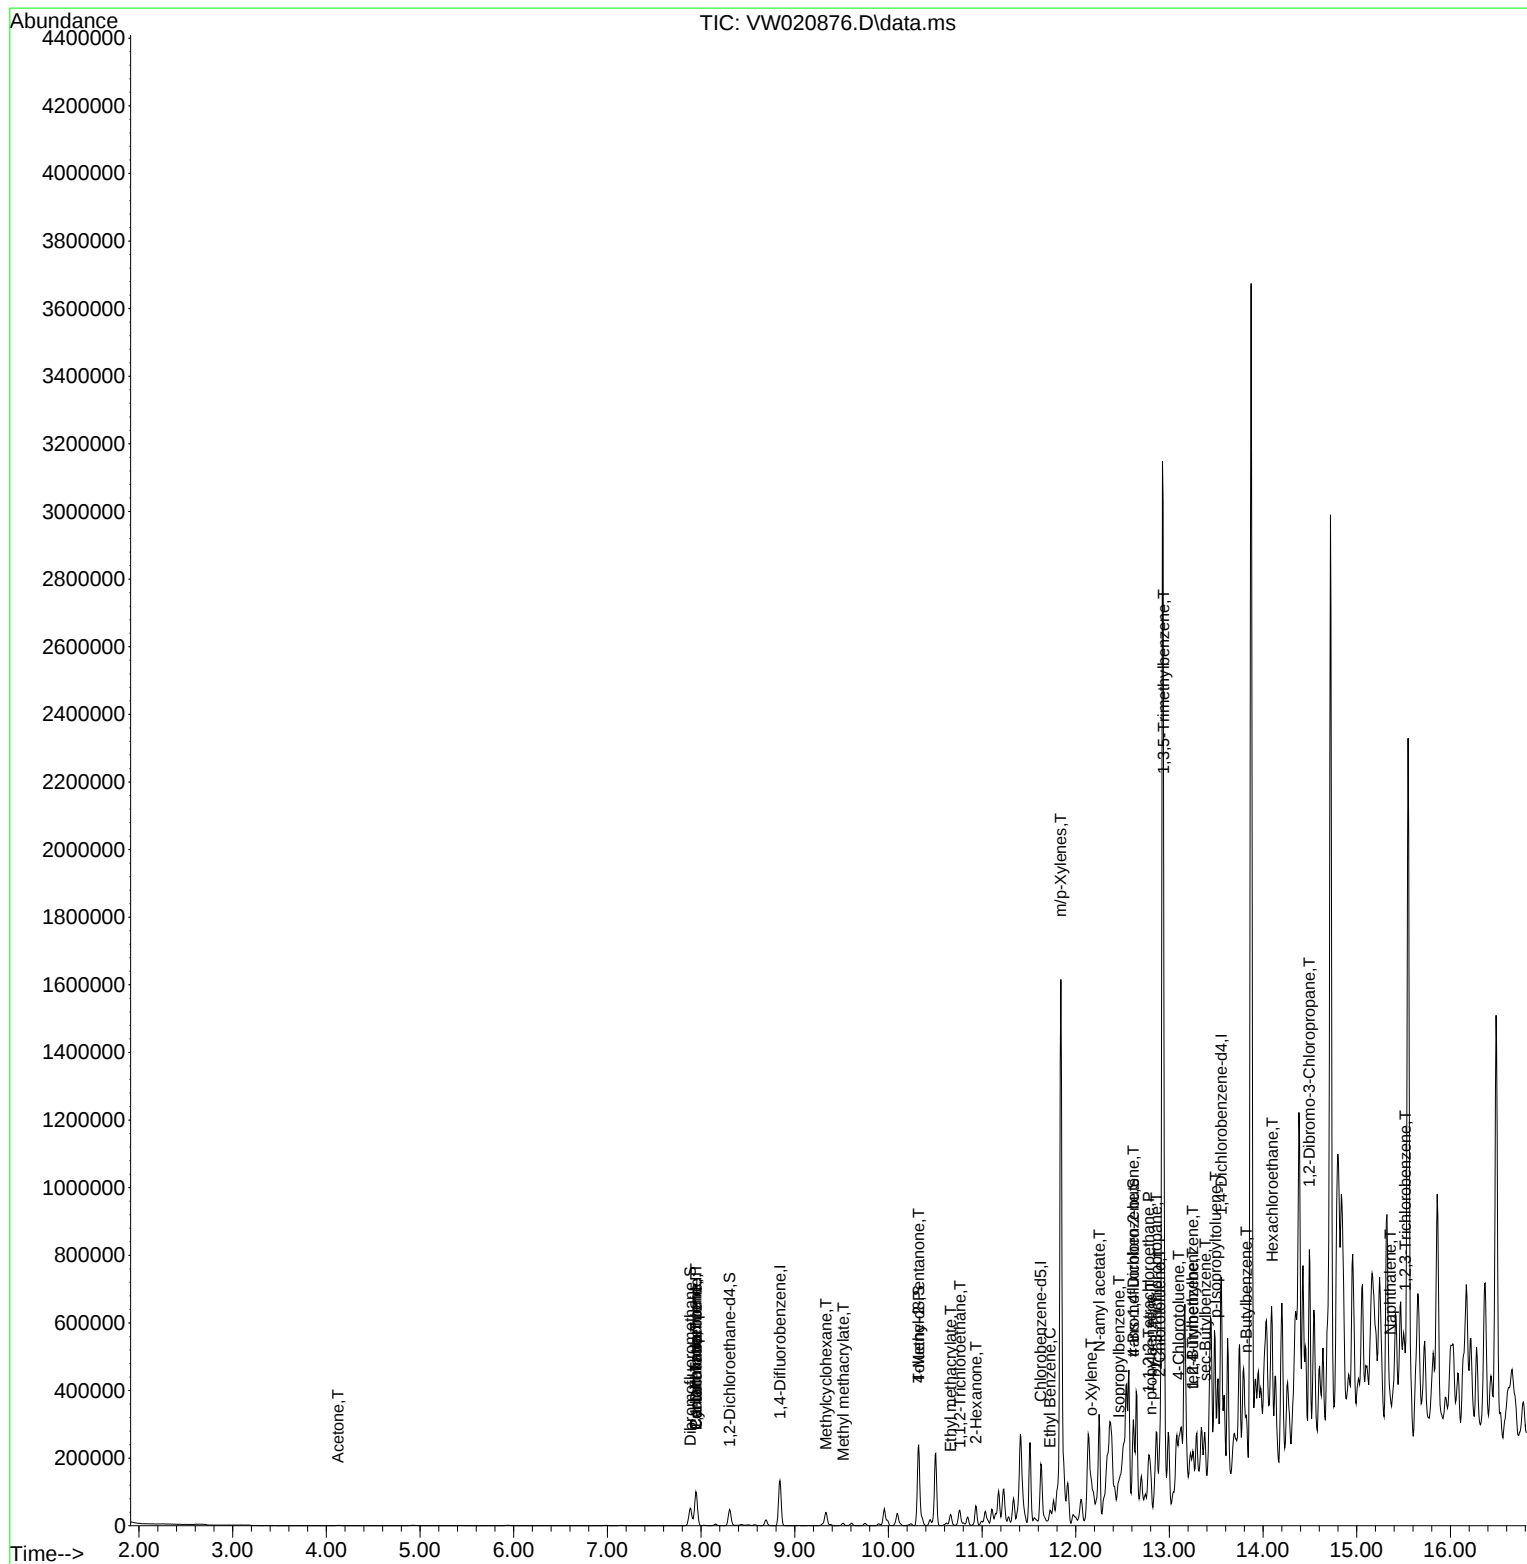






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.945 min Scan# 991
Delta R.T. -0.006 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Instrument :
MSVOA_W
ClientSampleId :



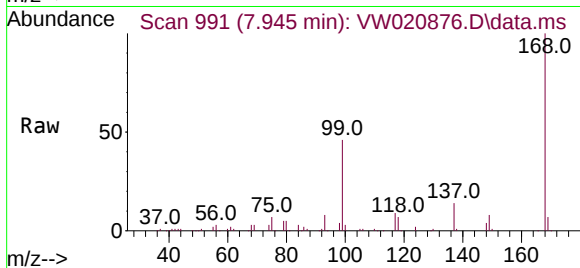



Tgt Ion:168 Resp: 76097
Ion Ratio Lower Upper
168 100
99 46.4 45.4 68.0

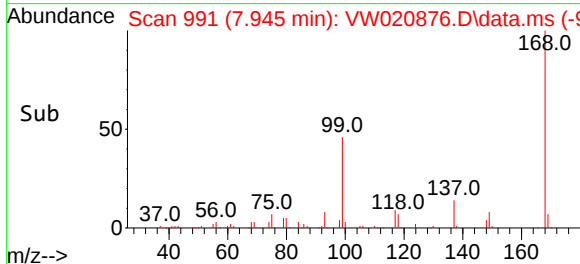

#16
Acetone
Concen: 16.901 ug/l
RT: 4.123 min Scan# 364
Delta R.T. -0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25


Tgt Ion: 43 Resp: 2070
Ion Ratio Lower Upper
43 100
58 32.0 24.2 36.2

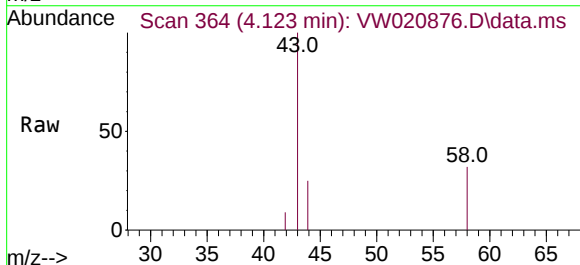






#20
Methylene Chloride
Concen: Below Cal
RT: 4.915 min Scan# 494
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Instrument :
MSVOA_W
ClientSampleId :



Tgt Ion: 84 Resp: 902




Ion	Ratio	Lower	Upper
84	100		
49	121.1	100.0	150.0
51	36.7	30.8	46.2
86	65.7	50.6	76.0




#31
Cyclohexane
Concen: 2.730 ug/l
RT: 7.945 min Scan# 991
Delta R.T. -0.012 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 56 Resp: 3081

Ion	Ratio	Lower	Upper
56	100		
69	103.7	27.2	40.8
84	95.5	71.8	107.6


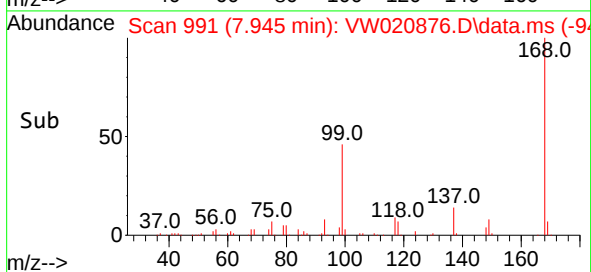




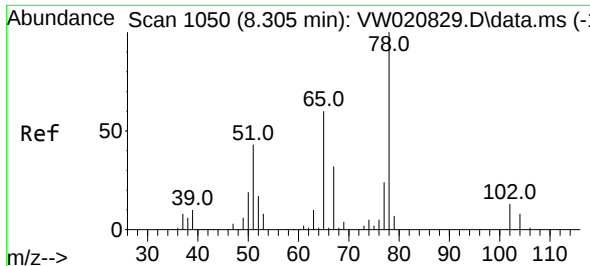

#33
 1,2-Dichloroethane-d4
 Concen: 58.166 ug/l
 RT: 8.305 min Scan# 1050
 Delta R.T. 0.000 min
 Lab File: VW020876.D
 Acq: 13 Nov 2021 00:25




Instrument :
 MSVOA_W
 ClientSampleId :


Tgt Ion: 65 Resp: 36603
 Ion Ratio Lower Upper
 65 100
 67 51.5 0.0 102.2

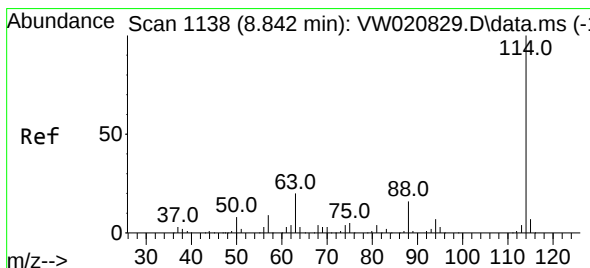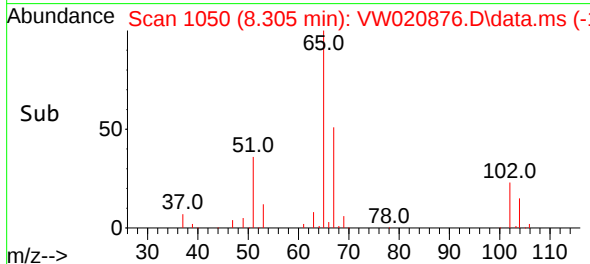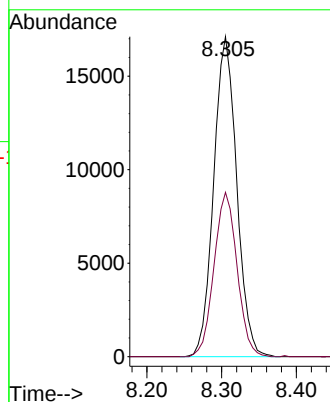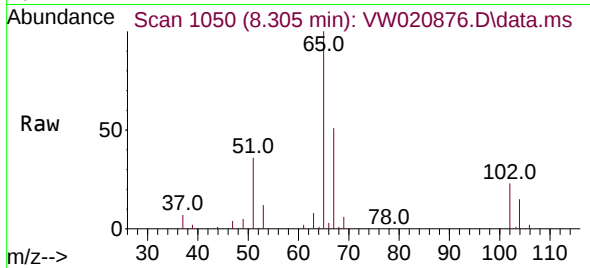

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.842 min Scan# 1138
 Delta R.T. 0.000 min
 Lab File: VW020876.D
 Acq: 13 Nov 2021 00:25

Tgt Ion: 114 Resp: 118593
 Ion Ratio Lower Upper
 114 100
 63 18.6 0.0 42.8
 88 15.2 0.0 33.0


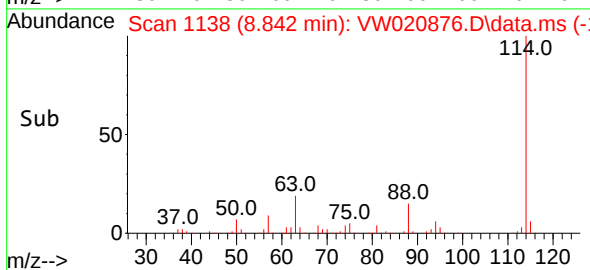

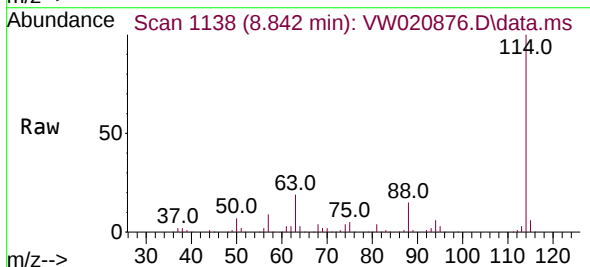


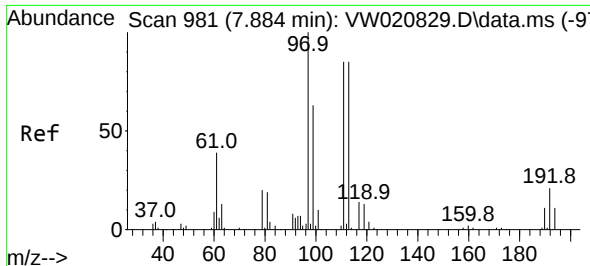

#35
Dibromofluoromethane
Concen: 52.774 ug/l
RT: 7.884 min Scan# 991
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:113 Resp: 34989
Ion Ratio Lower Upper
113 100
111 104.8 82.1 123.1
192 23.4 17.8 26.8

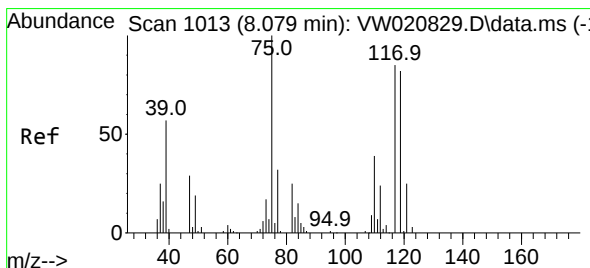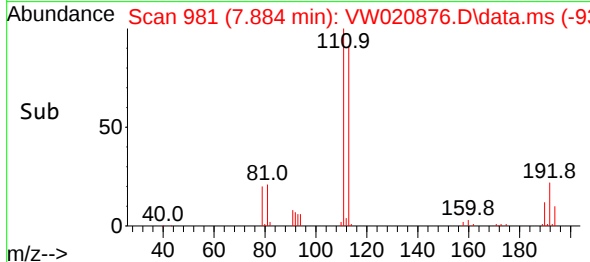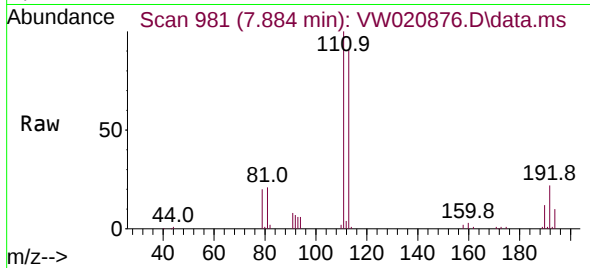

#36
1,1-Dichloropropene
Concen: 5.281 ug/l
RT: 7.945 min Scan# 991
Delta R.T. -0.134 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25


Tgt Ion: 75 Resp: 5177
Ion Ratio Lower Upper
75 100
110 8.6 17.1 51.3#
77 0.0 24.9 37.3#

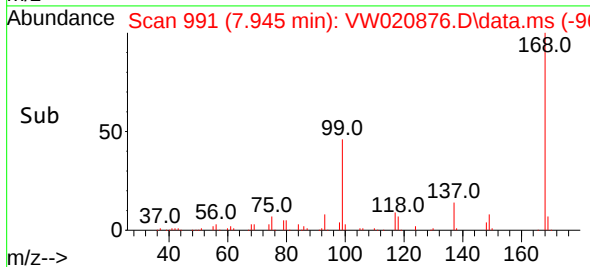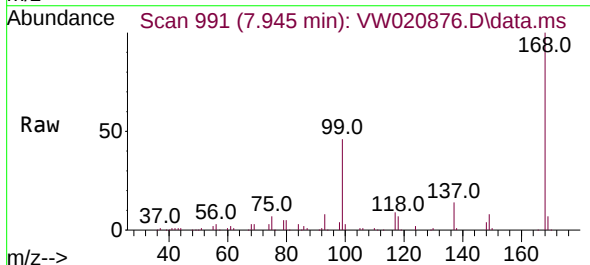






#38
Carbon Tetrachloride
Concen: 6.934 ug/l
RT: 7.945 min Scan# 991
Delta R.T. -0.122 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Instrument :
MSVOA_W
ClientSampleId :



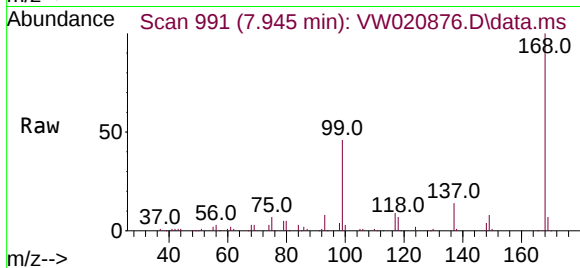



Tgt Ion:117 Resp: 7120
Ion Ratio Lower Upper
117 100
119 5.0 72.9 109.3#
121 0.0 23.4 35.0#



#39
Methylcyclohexane
Concen: 12.719 ug/l
RT: 9.335 min Scan# 1219
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 83 Resp: 16354
Ion Ratio Lower Upper
83 100
55 73.5 62.6 94.0
98 49.6 38.8 58.2


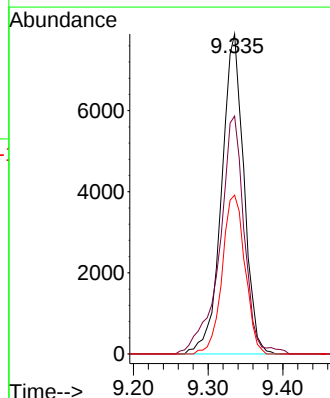

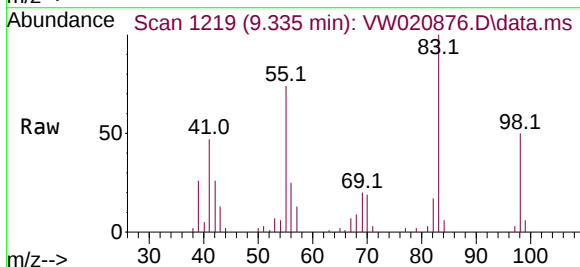




#48
Methyl methacrylate
Concen: 4.519 ug/l
RT: 9.518 min Scan# 1249
Delta R.T. 0.085 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 41 Resp: 1941
Ion Ratio Lower Upper
41 100
69 133.7 67.2 100.8#
39 49.7 47.0 70.6

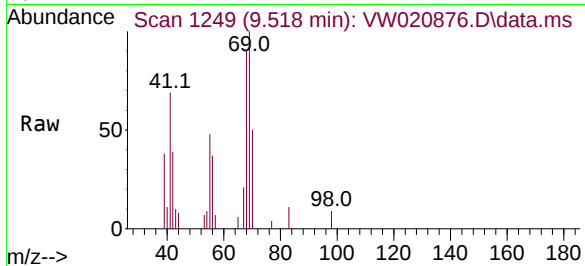

#50
Toluene-d8
Concen: 47.911 ug/l
RT: 10.323 min Scan# 1381
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 98 Resp: 124280
Ion Ratio Lower Upper
98 100
100 64.0 53.2 79.8

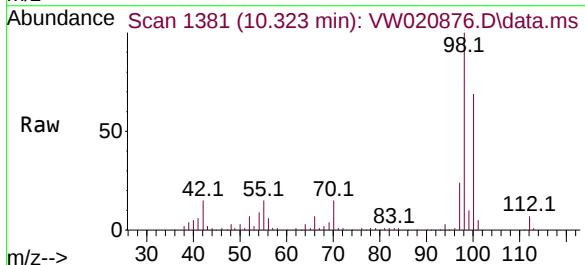



#51

4-Methyl-2-Pentanone

Concen: 6.113 ug/l

RT: 10.323 min Scan# 11

Delta R.T. 0.116 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 43 Resp: 2921

Ion Ratio Lower Upper

43 100

58 35.6 30.6 46.0



#55

1,1,2-Trichloroethane

Concen: 36.374 ug/l

RT: 10.762 min Scan# 1453

Delta R.T. -0.024 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25

Tgt Ion: 97 Resp: 17799




Ion Ratio Lower Upper


97 100

83 8.7 69.0 103.4#

85 4.8 44.3 66.5#

99 0.0 51.8 77.6#









#56
Ethyl methacrylate
Concen: 4.569 ug/l
RT: 10.664 min Scan# 1437
Delta R.T. 0.018 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 69 Resp: 3085
Ion Ratio Lower Upper
69 100
41 169.2 56.6 85.0#
39 91.7 29.6 44.4#



#59
2-Hexanone
Concen: 62.297 ug/l
RT: 10.933 min Scan# 1481
Delta R.T. -0.037 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25


Tgt Ion: 43 Resp: 21849
Ion Ratio Lower Upper
43 100
58 3.3 26.4 79.2#

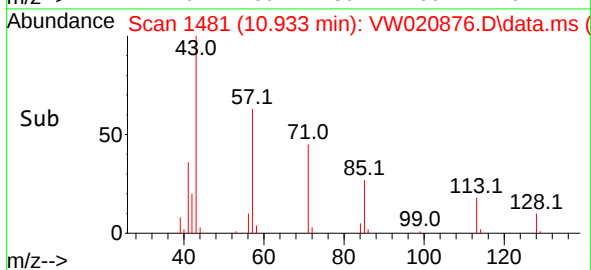






#62
4-Bromofluorobenzene
Concen: 52.793 ug/l
RT: 12.615 min Scan# 1757
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion: 95 Resp: 49407
Ion Ratio Lower Upper
95 100
174 84.0 0.0 166.4
176 80.2 0.0 159.8

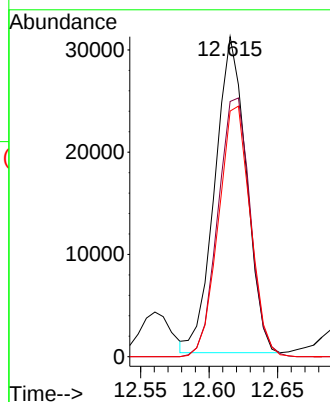

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.628 min Scan# 1595
Delta R.T. -0.006 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 117 Resp: 102804
Ion Ratio Lower Upper
117 100
82 50.6 45.6 68.4
119 35.9 25.0 37.4

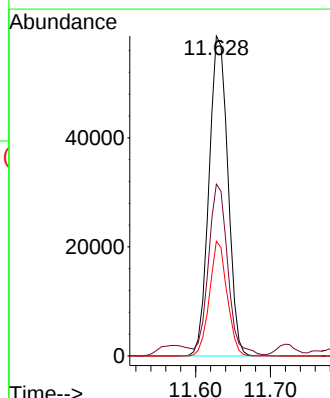



#67

Ethyl Benzene

Concen: 4.343 ug/l

RT: 11.725 min Scan# 1

Delta R.T. -0.006 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 91 Resp: 14351

Ion Ratio Lower Upper

91 100

106 31.9 24.4 36.6



#68

m/p-Xylenes

Concen: 6.230 ug/l

RT: 11.841 min Scan# 1630

Delta R.T. 0.006 min

Lab File: VW020876.D




Acq: 13 Nov 2021 00:25


Tgt Ion:106 Resp: 8141

Ion Ratio Lower Upper

106 100

91 214.6 166.4 249.6




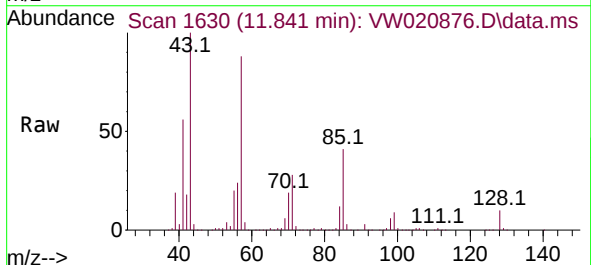




#69
o-Xylene
Concen: 9.558 ug/l
RT: 12.164 min Scan# 1
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:106 Resp: 11591
Ion Ratio Lower Upper
106 100
91 219.4 110.9 332.6



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.554 min Scan# 1911
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion:152 Resp: 54118
Ion Ratio Lower Upper
152 100
115 62.5 29.6 88.9
150 153.2 0.0 352.6


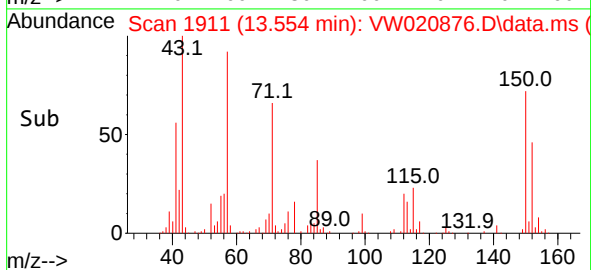






#73
Isopropylbenzene
Concen: 5.153 ug/l
RT: 12.463 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:105 Resp: 17396
Ion Ratio Lower Upper
105 100
120 26.2 13.0 39.0



#74
N-ethyl acetate
Concen: 78.835 ug/l
RT: 12.249 min Scan# 1697
Delta R.T. -0.018 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 43 Resp: 63551
Ion Ratio Lower Upper
43 100
70 20.5 33.4 50.2#
55 34.5 20.1 30.1#
61 0.0 18.9 28.3#


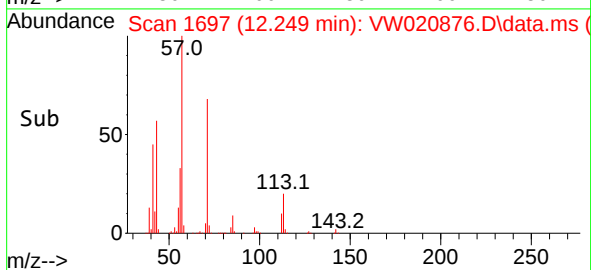






#75
1,1,2,2-Tetrachloroethane
Concen: 20.981 ug/l
RT: 12.780 min Scan# 1773
Delta R.T. 0.067 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 12644
Ion Ratio Lower Upper
83 100
131 0.0 5.8 17.3#
85 0.0 31.8 95.4#

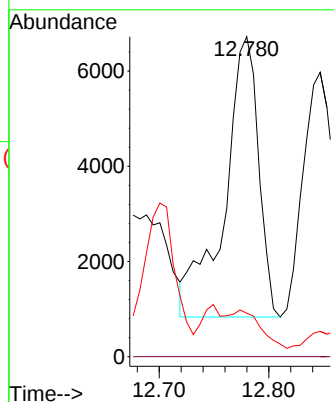

#76
1,2,3-Trichloropropane
Concen: 2.209 ug/l
RT: 12.859 min Scan# 1797
Delta R.T. 0.091 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 75 Resp: 919
Ion Ratio Lower Upper
75 100
77 1428.1 0.0 0.0#

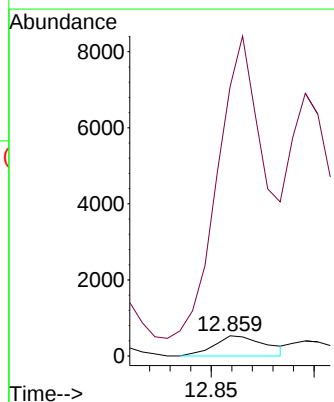



#78

n-propylbenzene

Concen: 15.776 ug/l

RT: 12.804 min Scan# 11

Delta R.T. 0.000 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 91 Resp: 64702

Ion Ratio Lower Upper

91 100

120 23.8 11.7 35.0

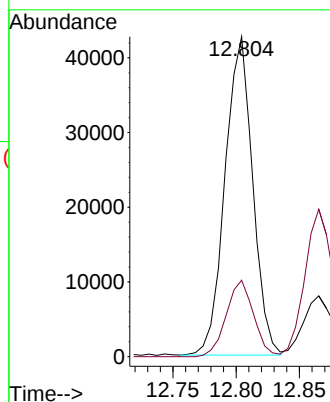

#79

2-Chlorotoluene

Concen: 3.504 ug/l

RT: 12.896 min Scan# 1803

Delta R.T. 0.006 min

Lab File: VW020876.D




Acq: 13 Nov 2021 00:25


Tgt Ion: 91 Resp: 7883

Ion Ratio Lower Upper

91 100

126 0.0 16.7 50.0#









#80
1,3,5-Trimethylbenzene
Concen: 31.448 ug/l
RT: 12.938 min Scan# 11
Delta R.T. -0.006 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:105 Resp: 88451
Ion Ratio Lower Upper
105 100
120 51.4 24.3 72.9

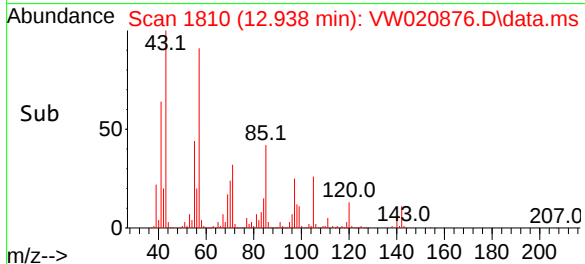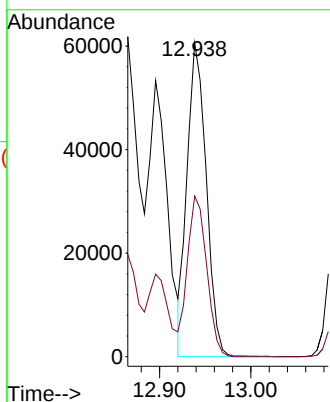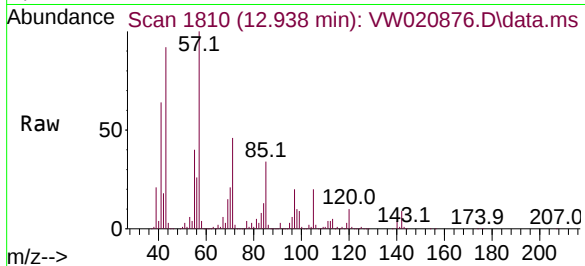

#81
trans-1,4-Dichloro-2-butene
Concen: 116.089 ug/l
RT: 12.615 min Scan# 1757
Delta R.T. 0.104 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 75 Resp: 24540
Ion Ratio Lower Upper
75 100
53 0.0 83.7 125.5#
89 1.0 36.7 55.1#


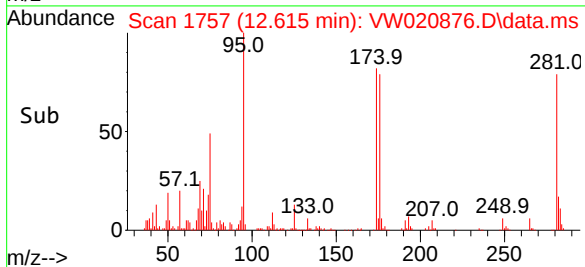
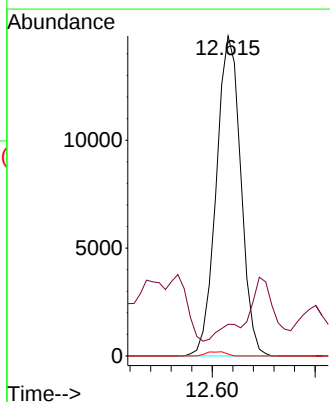
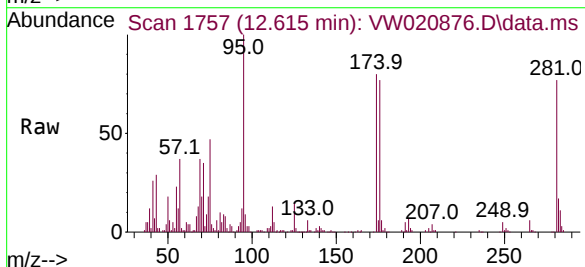




#82
4-Chlorotoluene
Concen: 5.042 ug/l
RT: 13.097 min Scan# 1836
Delta R.T. 0.110 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 91 Resp: 11737
Ion Ratio Lower Upper
91 100
126 19.2 16.8 50.4

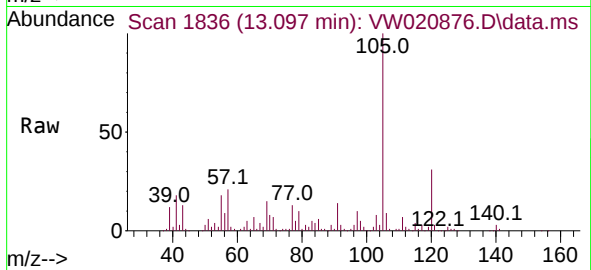

#83
tert-Butylbenzene
Concen: 2.612 ug/l
RT: 13.249 min Scan# 1861
Delta R.T. 0.049 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 119 Resp: 6897
Ion Ratio Lower Upper
119 100
91 83.7 32.9 98.7
134 0.0 12.4 37.2#


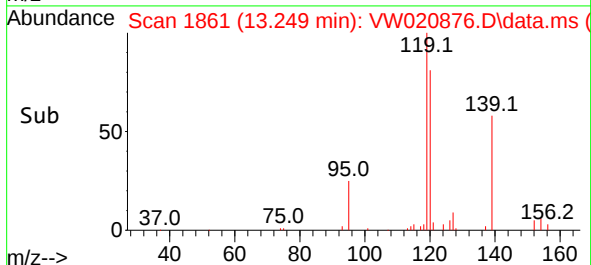
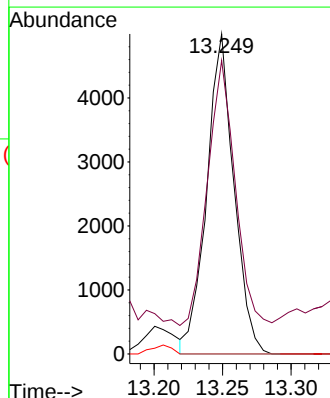





#84
1,2,4-Trimethylbenzene
Concen: 20.659 ug/l
RT: 13.249 min Scan# 1861
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:105 Resp: 57107
Ion Ratio Lower Upper
105 100
120 45.5 22.6 67.7

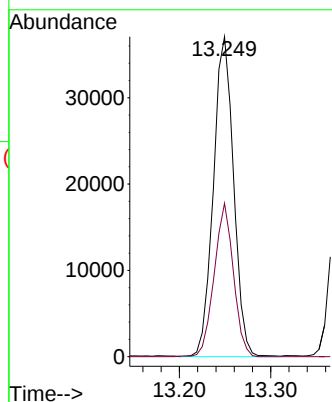

#85
sec-Butylbenzene
Concen: 14.488 ug/l
RT: 13.383 min Scan# 1883
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion:105 Resp: 54689
Ion Ratio Lower Upper
105 100
134 28.4 10.1 30.3


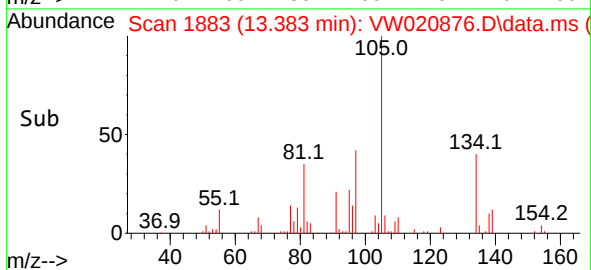
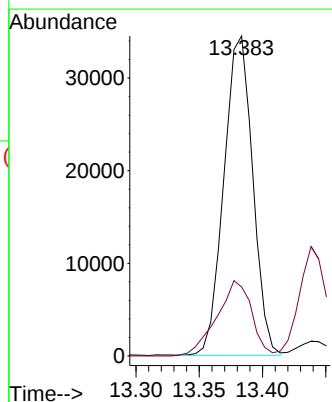





#86
p-Isopropyltoluene
Concen: 10.549 ug/l
RT: 13.493 min Scan# 1901
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:119 Resp: 34126
Ion Ratio Lower Upper
119 100
134 27.4 13.0 38.9
91 25.1 12.0 36.0

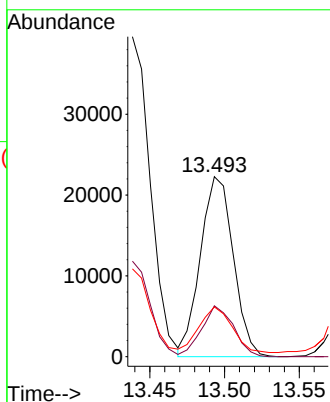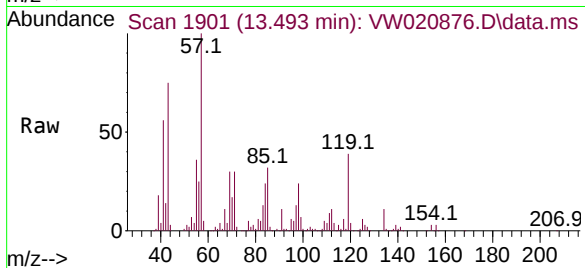

#89
n-Butylbenzene
Concen: 33.168 ug/l
RT: 13.822 min Scan# 1955
Delta R.T. 0.000 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion: 91 Resp: 99892
Ion Ratio Lower Upper
91 100
92 39.2 27.1 81.2
134 0.0 13.4 40.1#

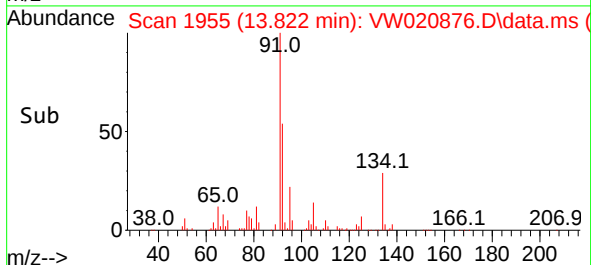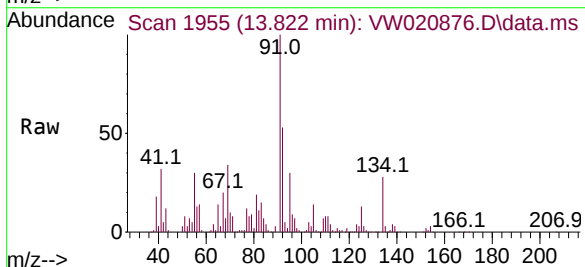



#90

Hexachloroethane

Concen: 23.361 ug/l

RT: 14.097 min Scan# 20

Delta R.T. 0.006 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:117 Resp: 14531

Ion Ratio Lower Upper

117 100

201 0.0 42.4 127.3#

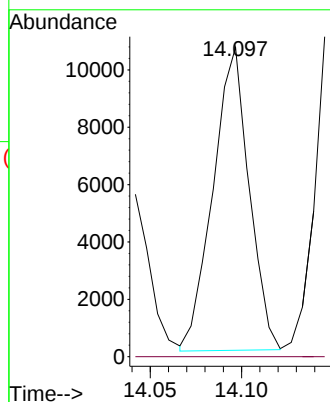

#92

1,2-Dibromo-3-Chloropropane

Concen: 5.607 ug/l

RT: 14.493 min Scan# 2065

Delta R.T. 0.012 min

Lab File: VW020876.D

Acq: 13 Nov 2021 00:25




Tgt Ion: 75 Resp: 678


Ion Ratio Lower Upper

75 100

155 123.3 42.5 127.6

157 0.0 53.4 160.2#









#95
Naphthalene
Concen: 4.220 ug/l
RT: 15.359 min Scan# 2207
Delta R.T. -0.006 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion:128 Resp: 8413
Ion Ratio Lower Upper
128 100
127 0.0 11.1 16.7#
129 0.0 8.9 13.3#



#96
1,2,3-Trichlorobenzene
Concen: 5.580 ug/l
RT: 15.517 min Scan# 2233
Delta R.T. -0.030 min
Lab File: VW020876.D
Acq: 13 Nov 2021 00:25

Tgt Ion:180 Resp: 4912
Ion Ratio Lower Upper
180 100
182 29.4 46.4 139.2#
145 310.4 15.7 47.0#

