
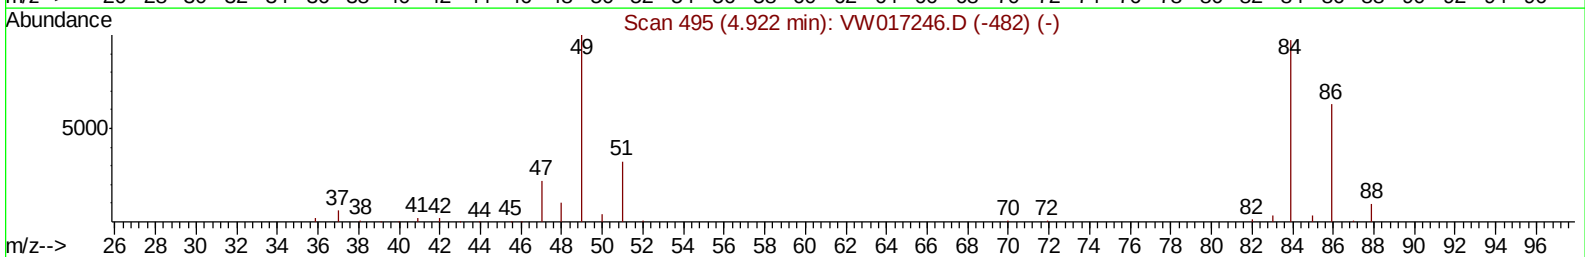
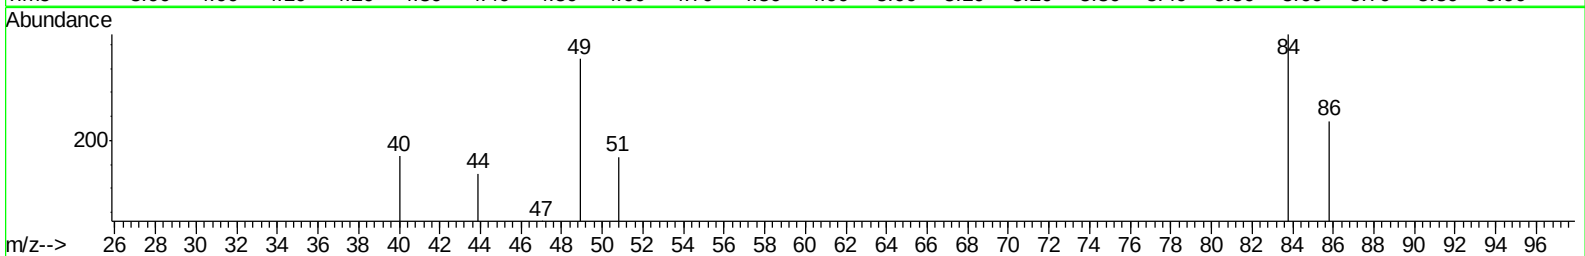


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
Data File : VW017263.D
Acq On : 16 Nov 2020 17:41
Operator : SY/VA
Sample : L4727-10RE
Misc : 4.38G/10ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 17 06:12:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 17 06:08:23 2020
Response via : Initial Calibration

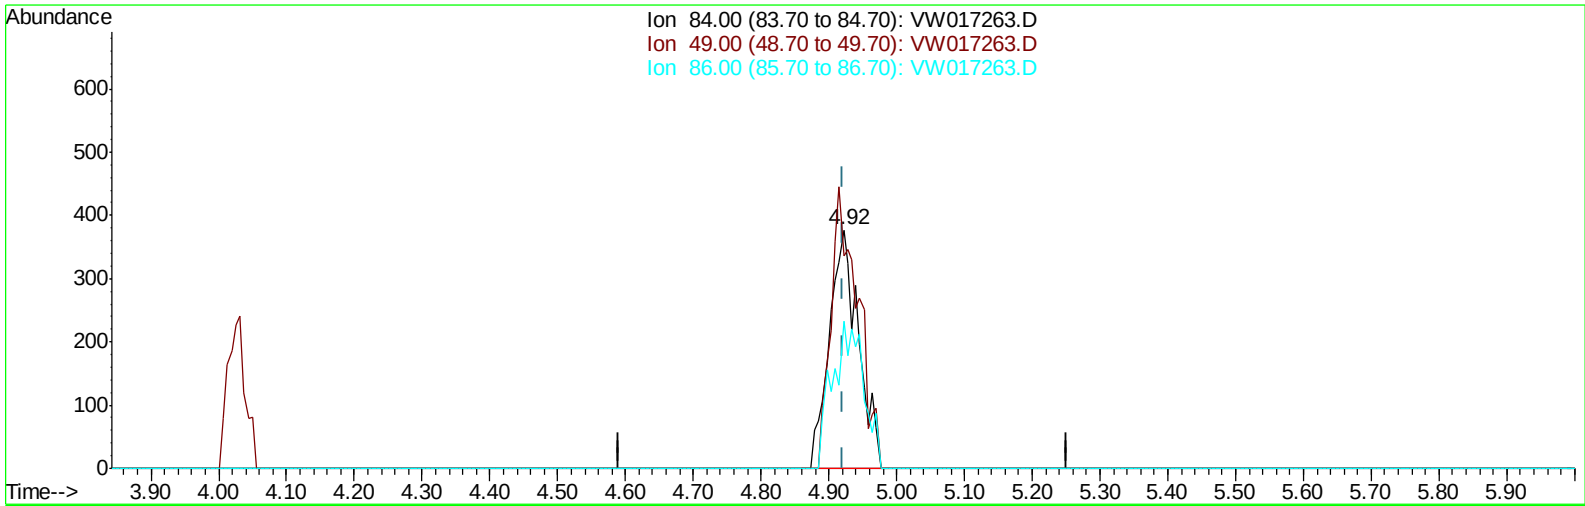

TIC: VW017263.D

(16) Methylene chloride (T)

4.921min (-0.000) 2.43ug/L m

response 1123

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	89.12
86.00	64.40	61.54
0.00	0.00	0.00