

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 GB0Z9

Manual Integrations
APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:11:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

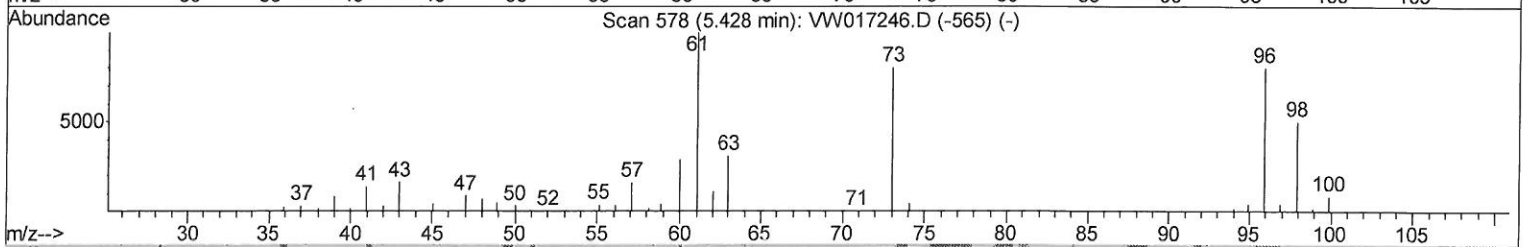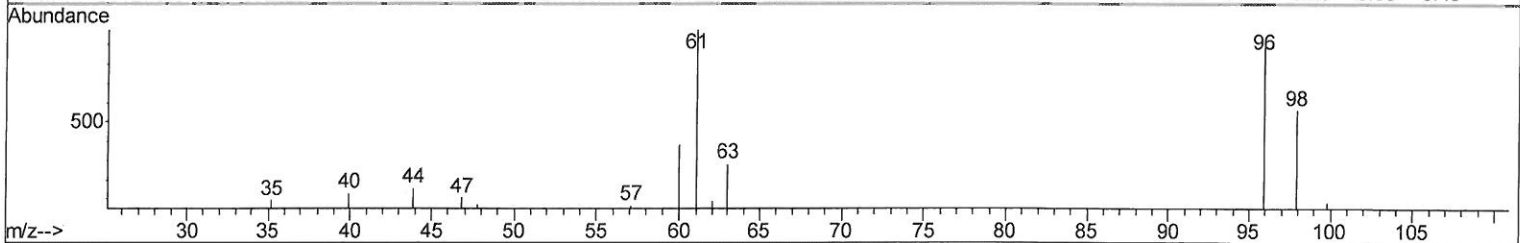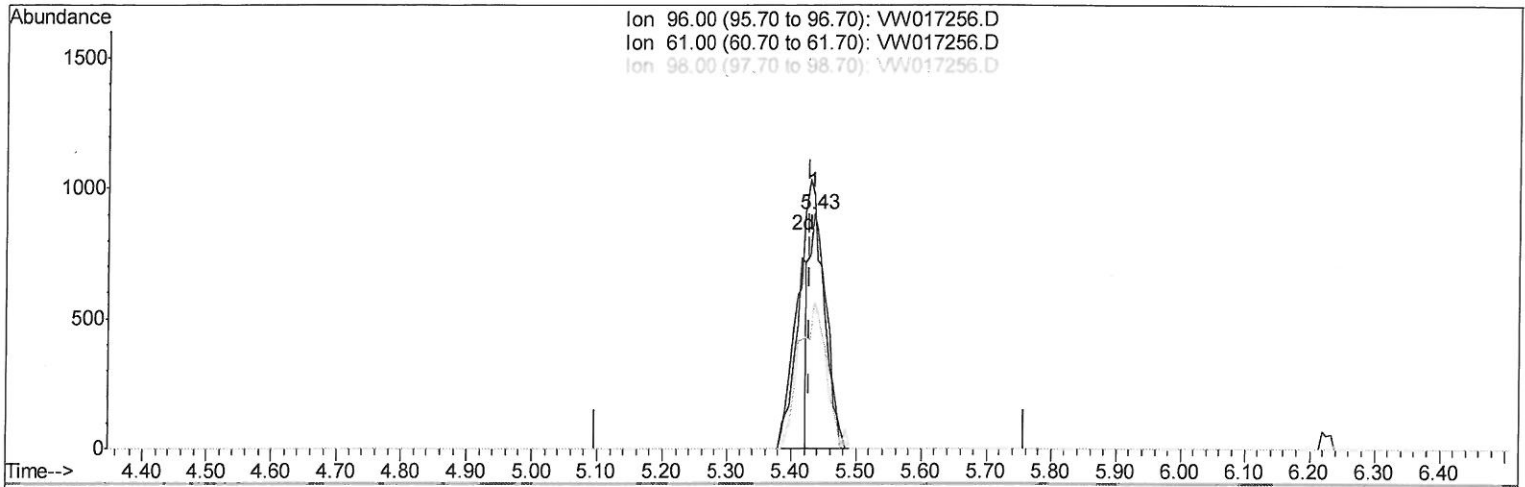

TIC: VW017256.D

(18) trans-1,2-Dichloroethene (T)

5.434min (+0.006) 0.29ug/L

response 1598

Ion	Exp%	Act%
96.00	100	100
61.00	124.00	108.54
98.00	63.40	62.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 GB0Z9

Manual Integrations
APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:11:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

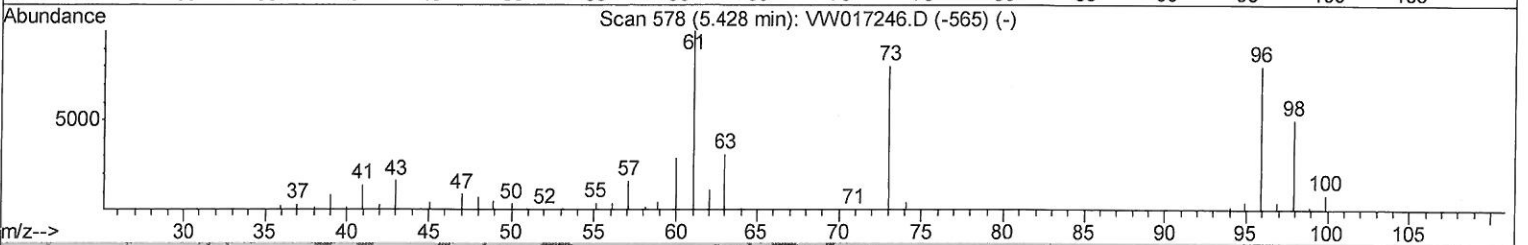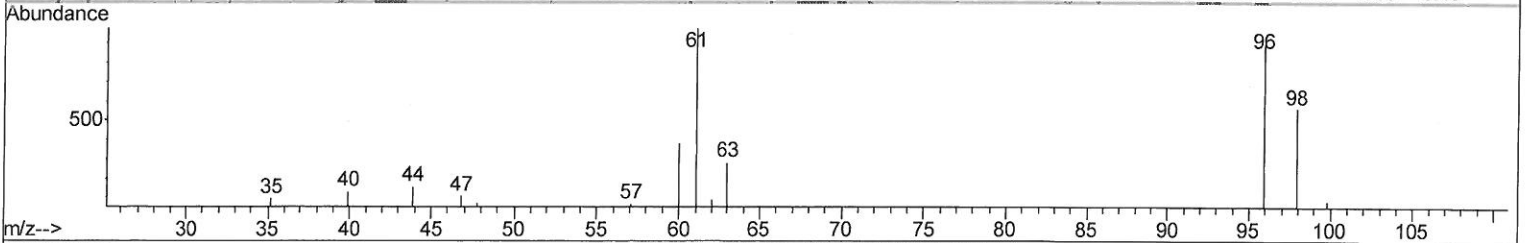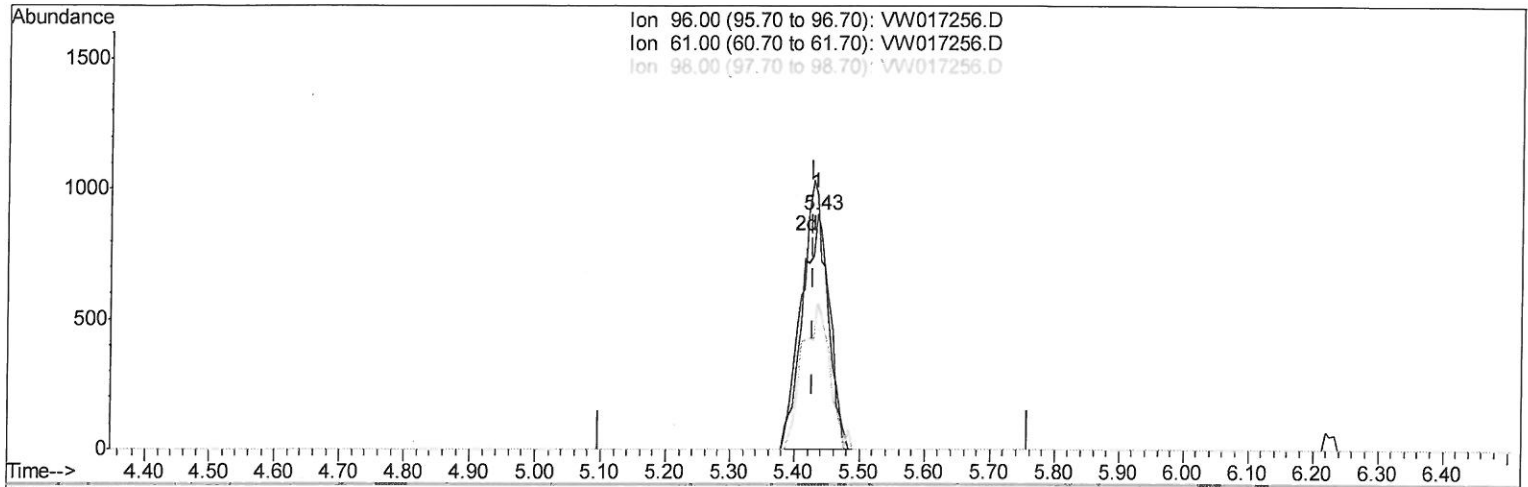

TIC: VW017256.D

(18) trans-1,2-Dichloroethene (T)

5.434min (+0.006) 0.47ug/L m

response 2574

Ion	Exp%	Act%
96.00	100	100
61.00	124.00	108.54
98.00	63.40	62.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 GB0Z9

Manual Integrations
APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:11:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

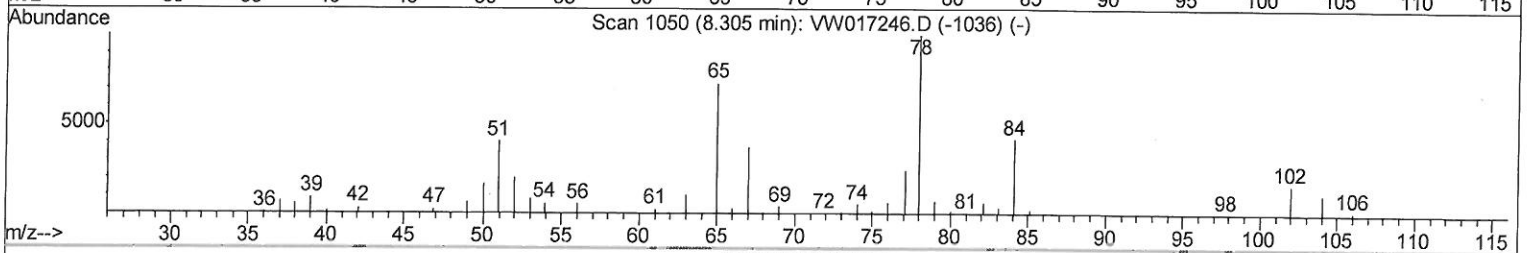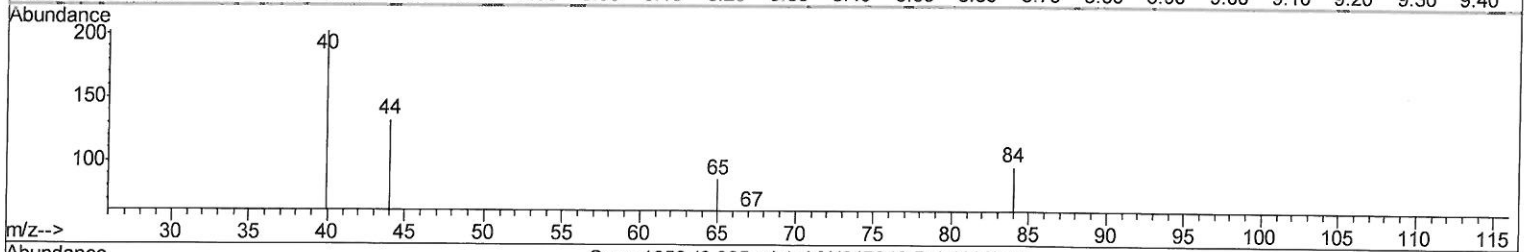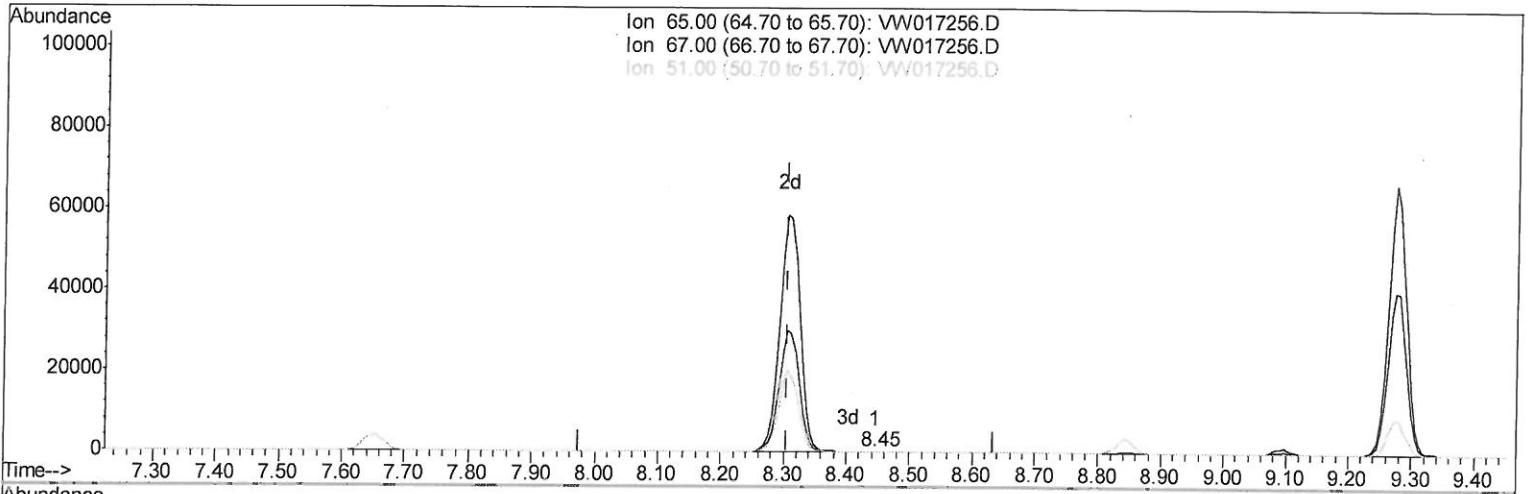

TIC: VW017256.D

(26) 1,2-Dichloroethane-d4 (S)

8.445min (+0.140) 0.02ug/L

response 82

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	64.63
51.00	92.10	68.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GB0Z9

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:11:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

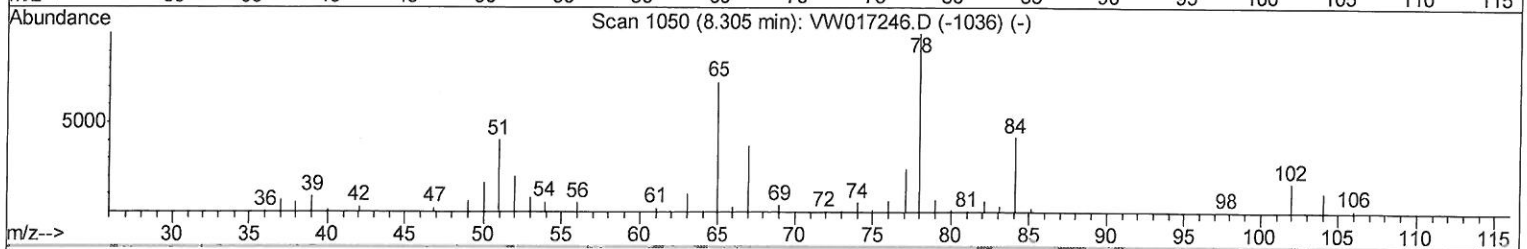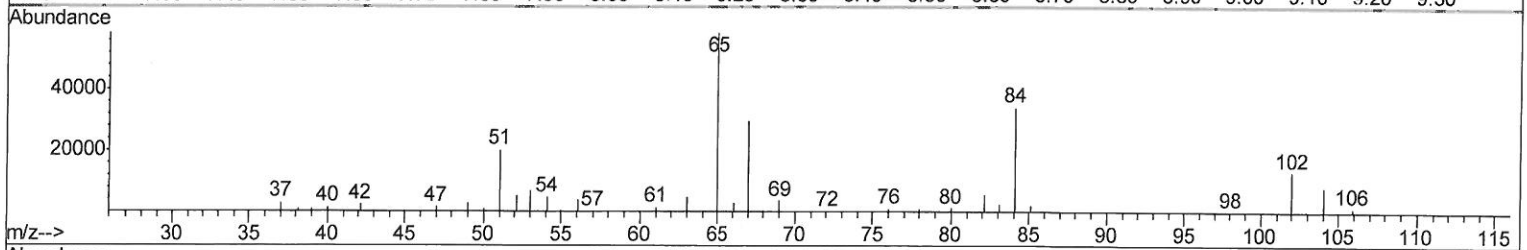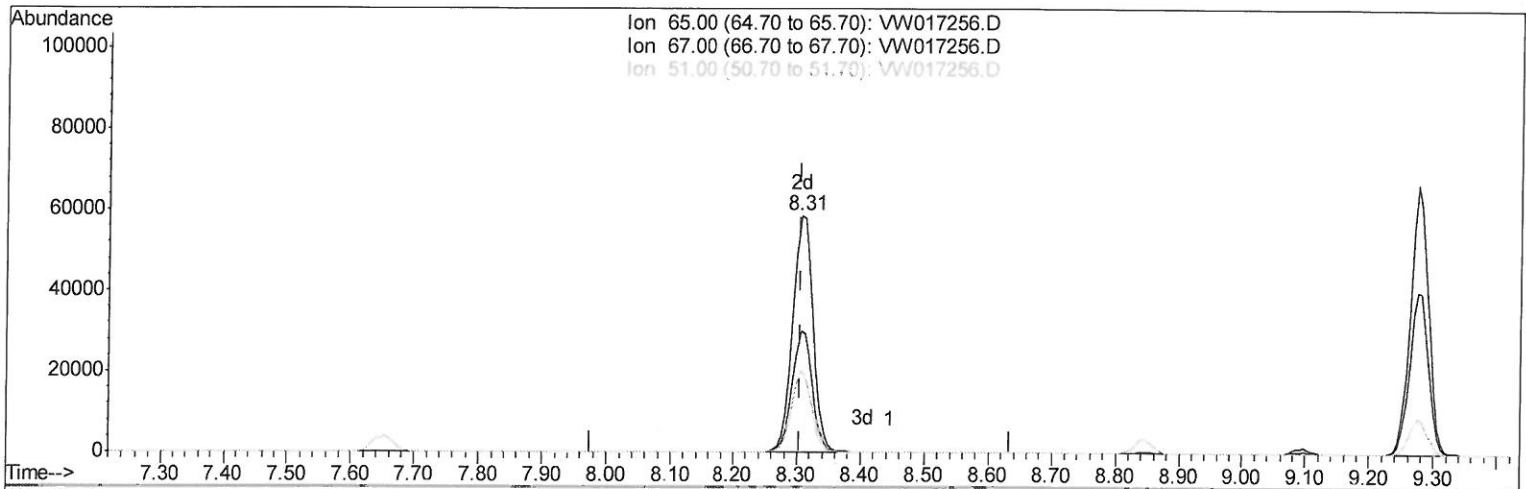

TIC: VW017256.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 26.05ug/L m

response 130131

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	0.04#
51.00	92.10	0.04#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB0Z9

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:56:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	430337	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	334101	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	106750	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	103576	19.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.44%
7) Chloroethane-d5	2.89	69	92885	22.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.96%
10) 1,1-Dichloroethene-d2	4.02	63	155637	16.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.20%
20) 2-Butanone-d5	7.08	46	56644	46.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.46%
24) Chloroform-d	7.65	84	242931	24.18	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.72%
26) 1,2-Dichloroethane-d4	8.31	65	130131m	26.05	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.20%
29) Benzene-d6	8.27	84	465170	27.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.36%
33) 1,2-Dichloropropane-d6	9.27	67	129902	27.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.40%
37) Toluene-d8	10.33	98	414745	25.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.40%
38) trans-1,3-Dichloropropene-	10.58	79	53702	25.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.24%
39) 2-Hexanone-d5	10.93	63	43904	53.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	90789	22.15	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.60%
61) 1,2-Dichlorobenzene-d4	13.86	152	86498	23.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.00%

Target Compounds

					Ovalue	
5) Vinyl chloride	2.36	62	7115	1.238	ug/L	# 43
13) Acetone	4.13	43	21076	25.968	ug/L	95
18) trans-1,2-Dichloroethene	5.43	96	2574m	0.466	ug/L	97
22) cis-1,2-Dichloroethene	7.17	96	202568	34.652	ug/L	99
35) Trichloroethene	9.09	95	203134	41.335	ug/L	91
44) Toluene	10.39	91	6224	0.322	ug/L	82
47) Tetrachloroethene	10.87	164	1474	0.332	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
Data File : VW017256.D
Acq On : 16 Nov 2020 14:56
Operator : SY/VA
Sample : L4739-12
Misc : 6.30G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB0Z9

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:56:15 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 17 06:08:23 2020
Response via : Initial Calibration

