

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017256.D
 Acq On : 16 Nov 2020 14:56
 Operator : SY/VA
 Sample : L4739-12
 Misc : 6.30G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB0Z9

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:56:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	430337	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	334101	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	106750	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	103576	19.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.44%
7) Chloroethane-d5	2.89	69	92885	22.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.96%
10) 1,1-Dichloroethene-d2	4.02	63	155637	16.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.20%
20) 2-Butanone-d5	7.08	46	56644	46.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.46%
24) Chloroform-d	7.65	84	242931	24.18	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.72%
26) 1,2-Dichloroethane-d4	8.31	65	130131m	26.05	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.20%
29) Benzene-d6	8.27	84	465170	27.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.36%
33) 1,2-Dichloropropane-d6	9.27	67	129902	27.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.40%
37) Toluene-d8	10.33	98	414745	25.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.40%
38) trans-1,3-Dichloropropene-	10.58	79	53702	25.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.24%
39) 2-Hexanone-d5	10.93	63	43904	53.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	90789	22.15	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.60%
61) 1,2-Dichlorobenzene-d4	13.86	152	86498	23.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.00%

Target Compounds

					Ovalue
5) Vinyl chloride	2.36	62	7115	1.238 ug/L	# 43
13) Acetone	4.13	43	21076	25.968 ug/L	95
18) trans-1,2-Dichloroethene	5.43	96	2574m	0.466 ug/L	
22) cis-1,2-Dichloroethene	7.17	96	202568	34.652 ug/L	97
35) Trichloroethene	9.09	95	203134	41.335 ug/L	99
44) Toluene	10.39	91	6224	0.322 ug/L	91
47) Tetrachloroethene	10.87	164	1474	0.332 ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111620\
Data File : VW017256.D
Acq On : 16 Nov 2020 14:56
Operator : SY/VA
Sample : L4739-12
Misc : 6.30G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GB0Z9

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:53:37 PM

Quant Time: Nov 17 06:56:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 17 06:08:23 2020
Response via : Initial Calibration

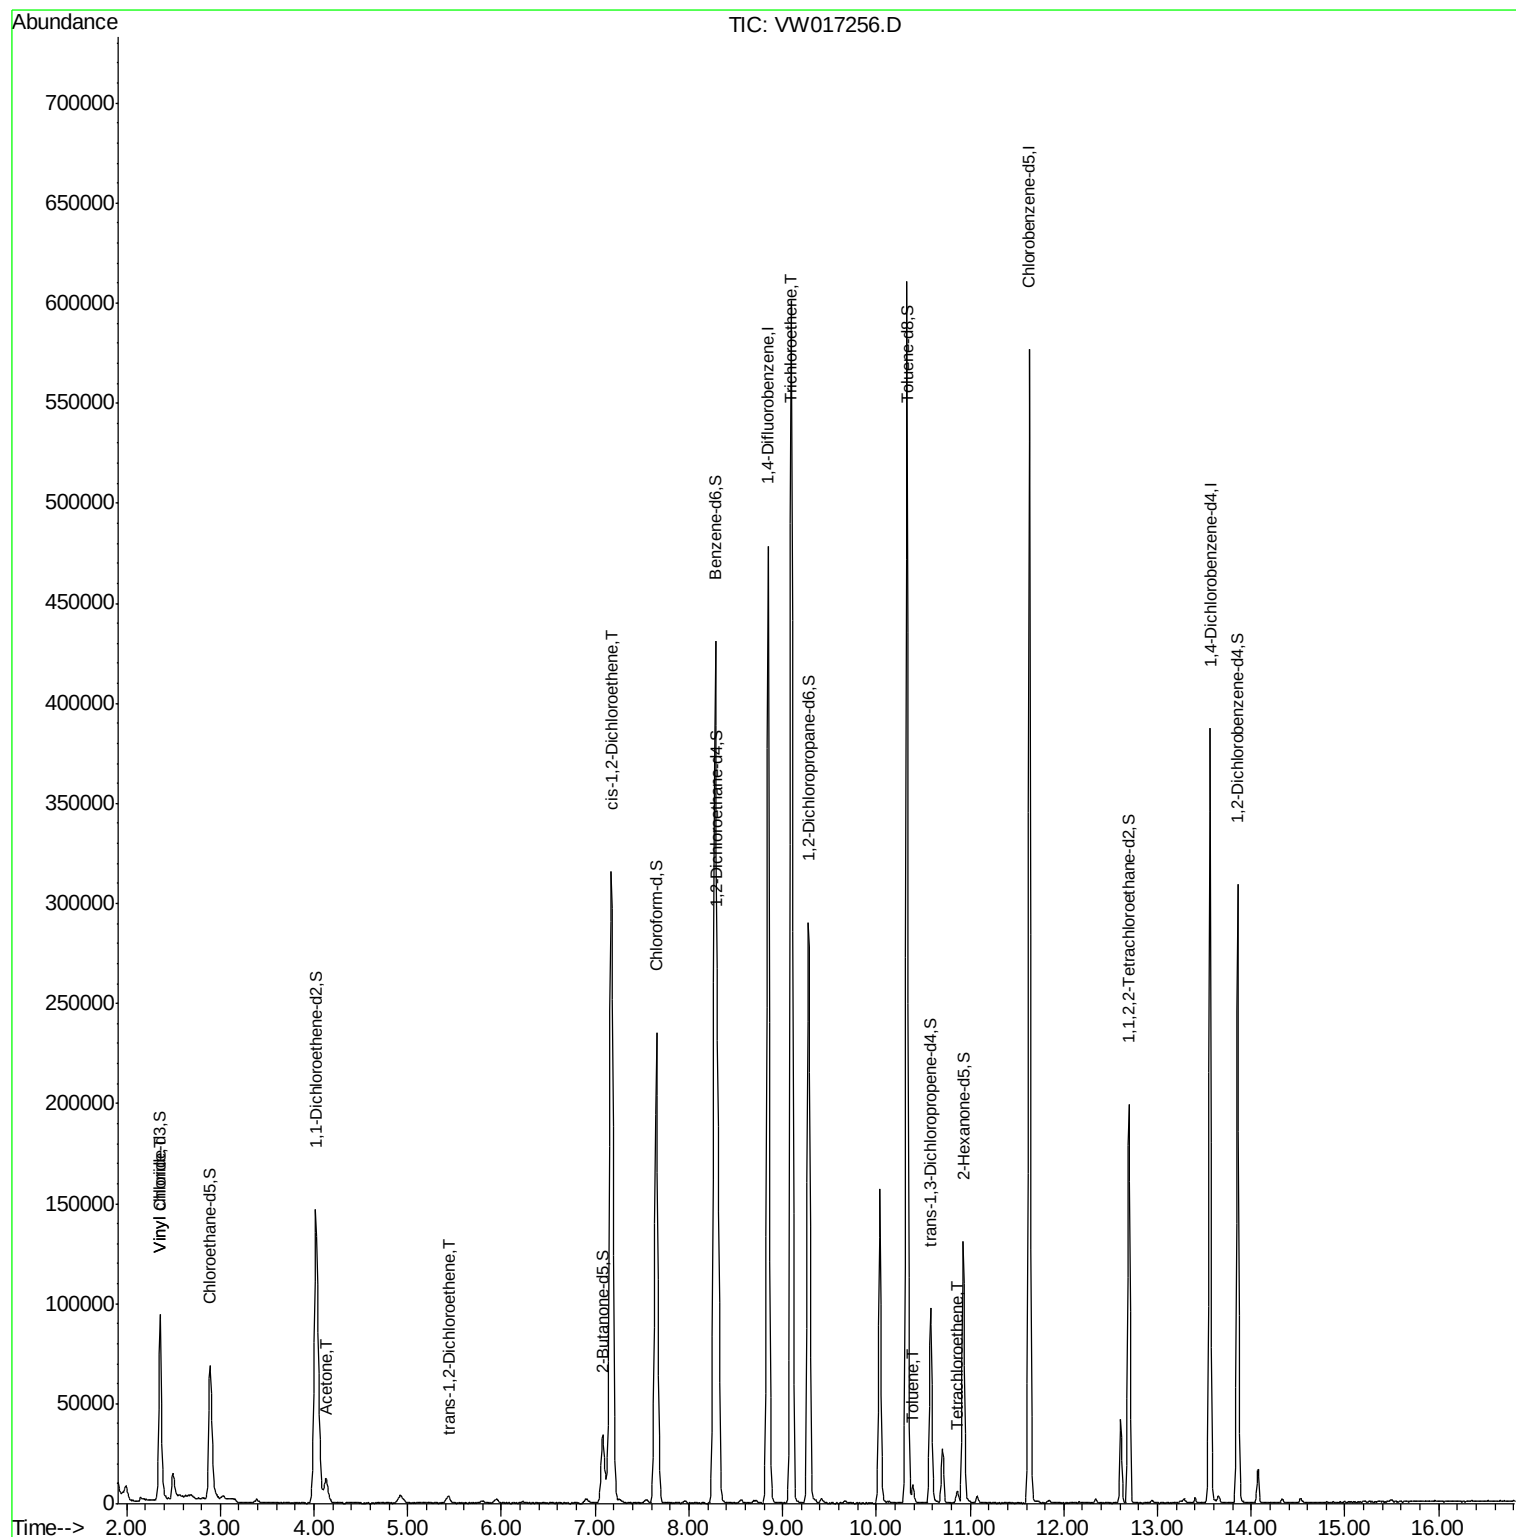

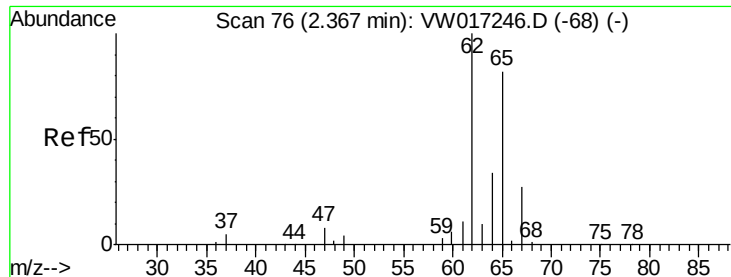

#5

Vinyl chloride

Concen: 1.238 ug/L

RT: 2.36 min Scan# 75

Delta R.T. -0.01 min

Lab File: VW017256.D

Acq: 16 Nov 2020 14:56

Instrument :

MSVOA_W

ClientSampleId :

GB0Z9

Tot Ion: 62 Resp: 7115

Ion Ratio Lower Upper

62 100





64 65.7 23.3 43.3#

Manual Integrations

APPROVED

MMDadoda

11/17/2020 6:53:37 PM

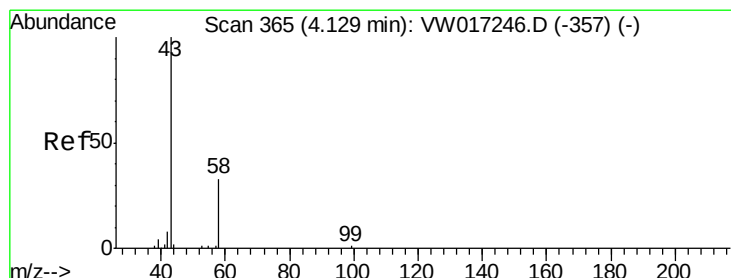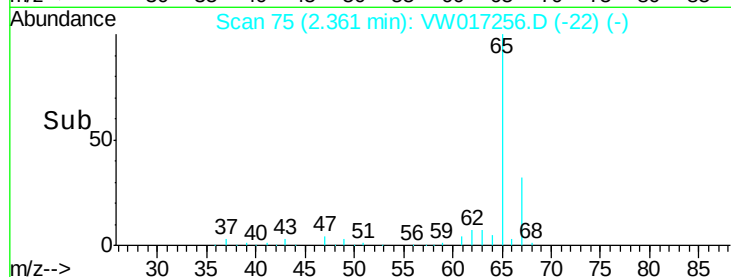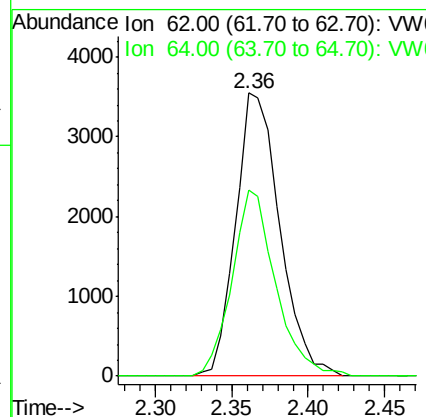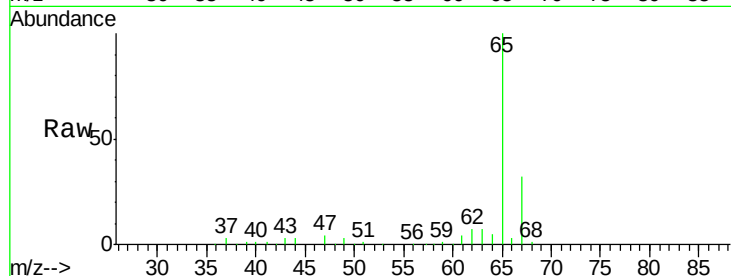

#13

Acetone

Concen: 25.968 ug/L

RT: 4.13 min Scan# 365

Delta R.T. -0.00 min

Lab File: VW017256.D




Acq: 16 Nov 2020 14:56


Tgt Ion: 43 Resp: 21076

Ion Ratio Lower Upper

43 100

58 31.8 0.0 69.2

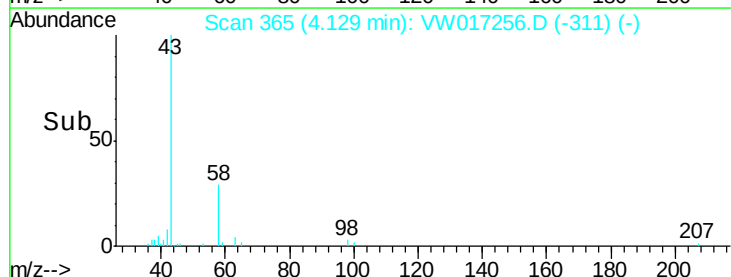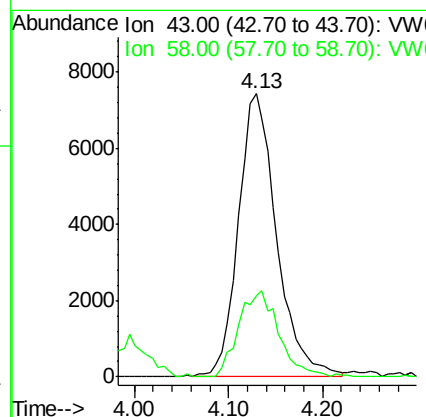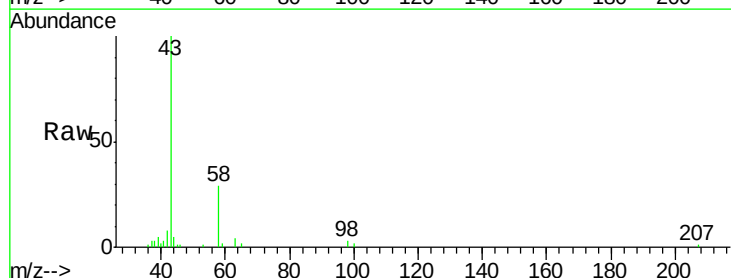

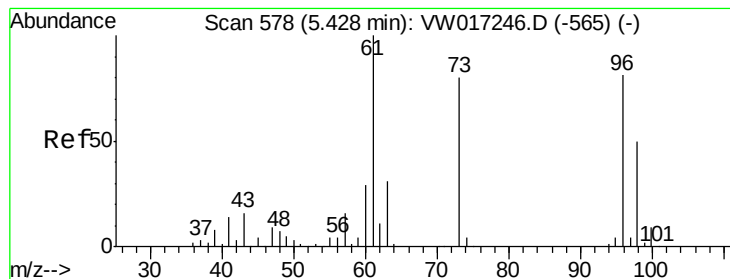

#18

trans-1,2-Dichloroethene

Concen: 0.466 ug/L m

RT: 5.43 min Scan# 579

Delta R.T. 0.01 min

Lab File: VW017256.D

Acq: 16 Nov 2020 14:56

Instrument :

MSVOA_W

ClientSampled :

GB0Z9

Tot Ion: 96 Resp: 2574

Ion Ratio Lower Upper

96 100

61 108.5 86.8 161.2


98 62.4 44.4 82.4

Manual Integrations

APPROVED

MMDadoda




11/17/2020 6:53:37 PM

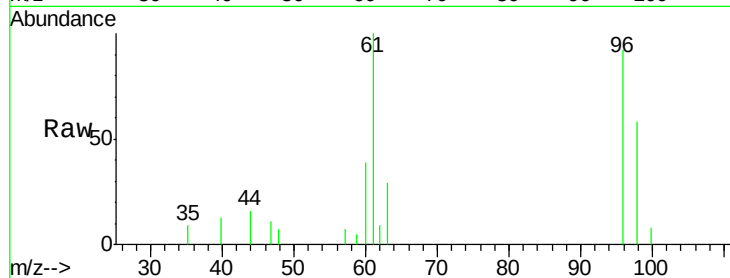

Abundance Ion 96.00 (95.70 to 96.70): VW

Ion 61.00 (60.70 to 61.70): VW

Ion 98.00 (97.70 to 98.70): VW

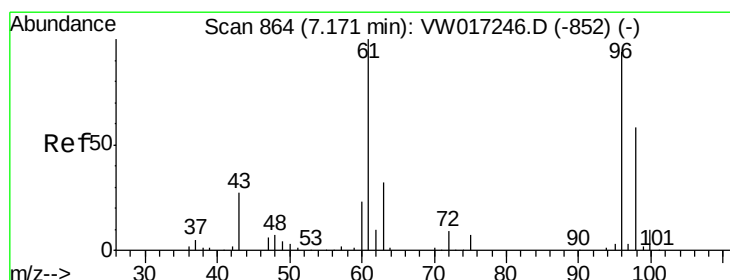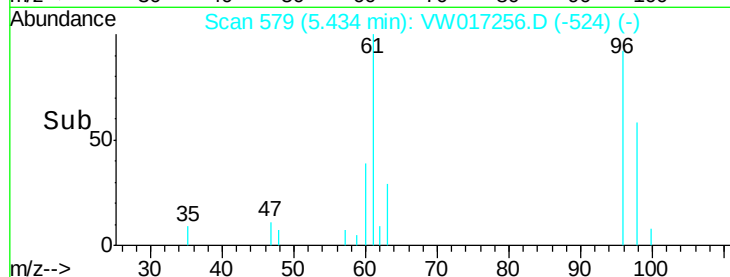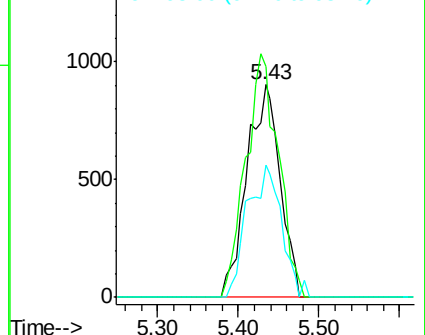

#22

cis-1,2-Dichloroethene

Concen: 34.652 ug/L

RT: 7.17 min Scan# 864

Delta R.T. -0.00 min

Lab File: VW017256.D

Acq: 16 Nov 2020 14:56


Tgt Ion: 96 Resp: 202568

Ion Ratio Lower Upper

96 100

61 115.2 77.4 143.8



98 65.3 45.1 83.7

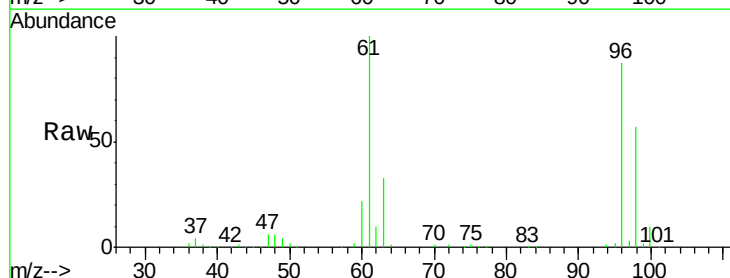


Abundance Ion 96.00 (95.70 to 96.70): VW

Ion 61.00 (60.70 to 61.70): VW

Ion 98.00 (97.70 to 98.70): VW

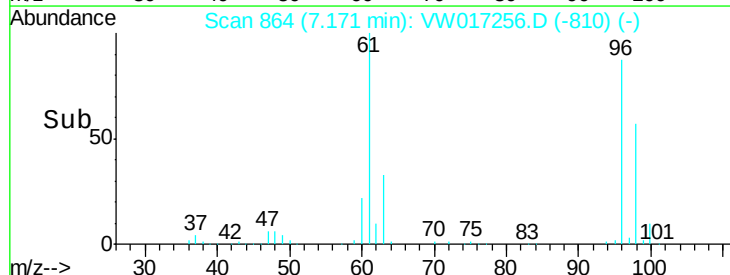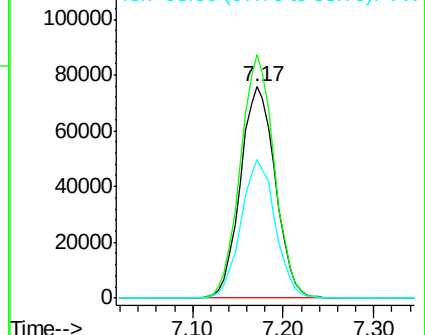

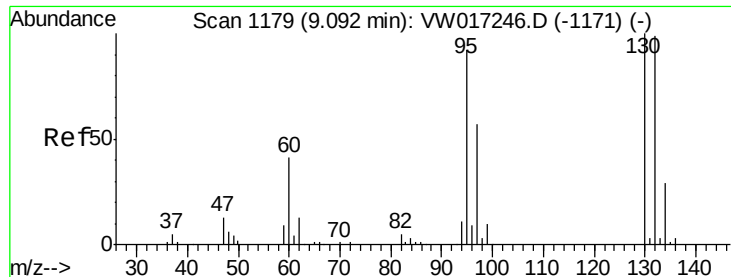





#35
 Trichloroethene
 Concen: 41.335 ug/L
 RT: 9.09 min Scan# 1179
 Delta R.T. -0.00 min
 Lab File: VW017256.D
 Acq: 16 Nov 2020 14:56

Instrument :
 MSVOA_W
 ClientSampleId :
 GB0Z9

Tot Ion	Ratio	Resp	Lower	Upper
95	100	203134		
97	64.8	45.0	83.6	
132	105.0	73.7	136.9	
130	109.1	77.1	143.1	




Manual Integrations
 APPROVED


MMDadoda
 11/17/2020 6:53:37 PM

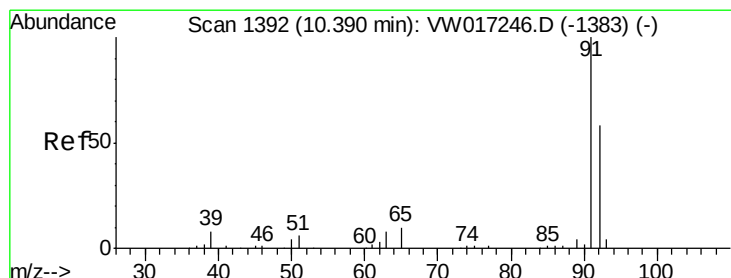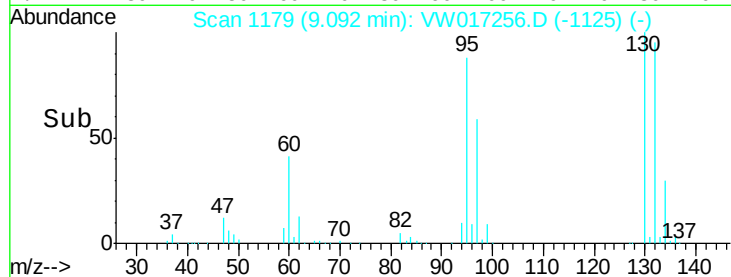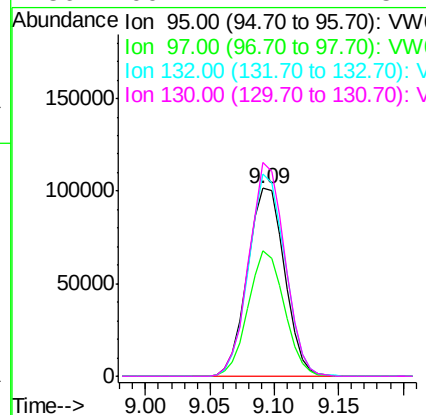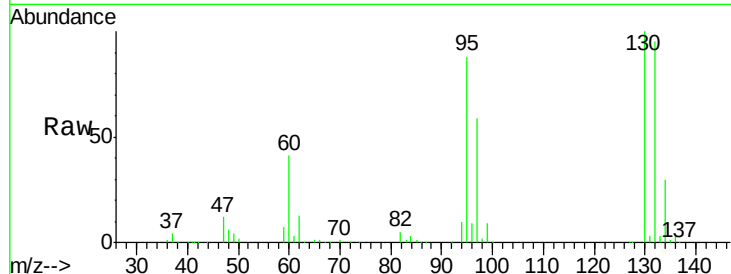

#44
 Toluene
 Concen: 0.322 ug/L
 RT: 10.39 min Scan# 1392
 Delta R.T. -0.00 min
 Lab File: VW017256.D
 Acq: 16 Nov 2020 14:56

Tgt Ion	Ratio	Resp	Lower	Upper
91	100	6224		
92	52.2	41.4	76.8	

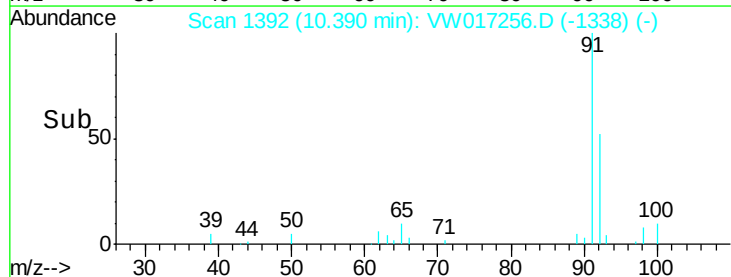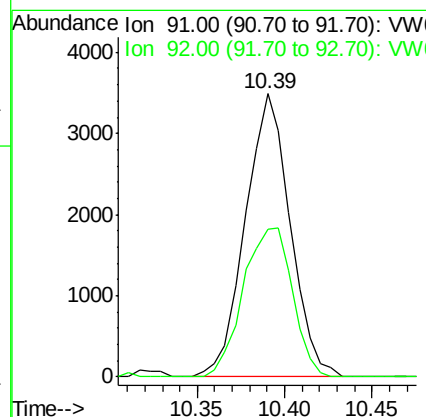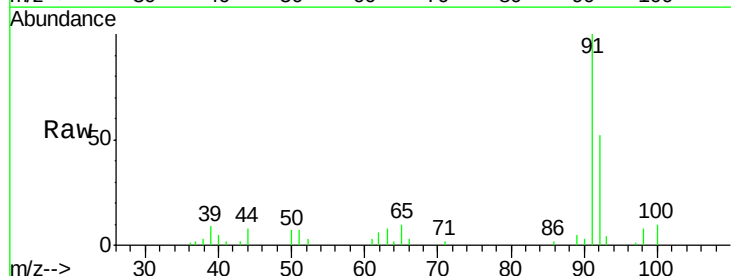

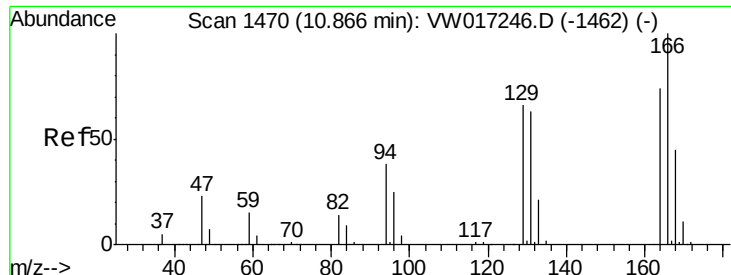

#47

Tetrachloroethene

Concen: 0.332 ug/L

RT: 10.87 min Scan# 1470

Delta R.T. -0.00 min

Lab File: VW017256.D


Acq: 16 Nov 2020 14:56

Instrument :

MSVOA_W

ClientSampleId :

GB0Z9

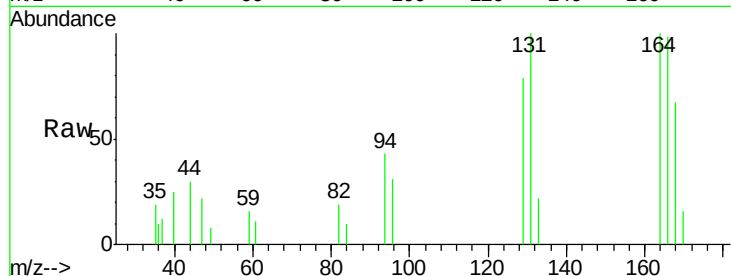

Tot Ion:164 Resp: 1474

Ion Ratio Lower Upper

164 100

129 79.7 62.9 116.7

131 100.3 63.3 117.5


166 98.0 92.0 170.8

Manual Integrations

APPROVED

MMDadoda

11/17/2020 6:53:37 PM

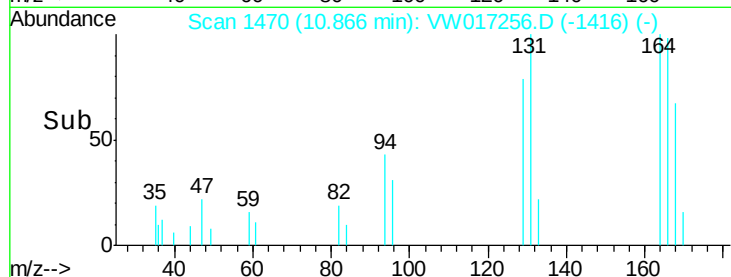

Abundance

Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

